


Notice of Simulator Solution File Review

At the request of the State Toxicologist a review of the following simulator solution records has been accomplished. The following file consists of simulator solution analyses performed and completed by the State Toxicology Laboratory for a specific batch number. The file contains the simulator solution data entry form along with a file review record and the chromatograms generated by the Toxicology Laboratory during the analyses of the solutions. This file has been reviewed by Tpr. Ken Denton and Mr. Rod Gullberg for accuracy and completeness. Where computations regarding simulator solution values have been found to be incorrect, the corrected values have been written in by Mr. Rod Gullberg along with initials and date. The corrected values were then evaluated to ensure that the solution still conformed to those standards established by the State Toxicologist.

Where computation values changed for a specific batch number, the analysts employed by the State Toxicology Laboratory were asked to review the revisions, ensure the solution complied with the criteria established by the State Toxicologist and then re-sign their affidavit. Their signature will appear on their original affidavit along with a statement regarding their review of the results.


Where a dating error occurred that analyst will have made the correction on the original data form including their initials and date and then re-signed their original affidavit.



10/15/2007

Tpr. Ken Denton

Date

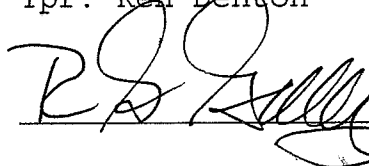

10-15-07

Rod G. Gullberg

Date

Washington State Toxicology Laboratory

Simulator Solution Data Entry Review Form

Reviewer KEN DENTON / ROD GULLBERG Date 10-10-07
Location TOX LAB SEATTLE Batch Number 05002

Form Review Criteria

Preparation date precedes all analysis dates: Okay Not Okay

Data entry corresponds to all chromatograms: Okay Not Okay

All signatures present: Okay Not Okay

Computations:

Avg. solution concentration: Correct Not Correct

Standard deviation: Correct Not Correct

Range: Correct Not Correct

Precision: Correct Not Correct

Equivalent vapor concent.: Correct Not Correct

External Control Information
(lot # and future date): Correct Not Correct


Complies with accuracy and precision requirements established by the
State Toxicologist: Yes No

Corrections Necessary:

Comments:

Reviewer Signature: 

Date: 10-10-07

Reviewer Signature: 

Date: 10/10/2007

WASHINGTON STATE TOXICOLOGY LABORATORY
FORENSIC LABORATORY SERVICES BUREAU
 WASHINGTON STATE PATROL
 2203 AIRPORT WAY S, SUITE 360
 SEATTLE, WASHINGTON 98134-2027
 (206) 262-6100 FAX (206) 262-6145

Preparation and certification of **0.04 g/210L Quality Assurance solution**

Batch number **05002**

Date: 1/7/2005

Preparation: 11.1 mL of absolute ethyl alcohol diluted to 18 Liters with water

Concentration of ethanol (g/100mL) measured by gas chromatography:

	Anal 1	Anal 2	Anal 3	Anal 4	Anal 5	Anal 6	Anal 7	Anal 8	Anal 9	Anal 10	Anal 11	Anal 12
1	0.051	0.051	0.050									
2	0.051	0.051	0.050									
3	0.051	0.051	0.051									
4	0.051	0.050	0.050									
5	0.051	0.051	0.050									
Ctrl	0.100	0.099	0.098									

External Control:

Lot #: A028603 Exp date: 12/07

Target concentration: 0.10 g/100mL

Statistics:




Avg. solution concent.: 0.0507 g/100 mL

SD: 0.00049

Range (3xSD): 0.0492 to 0.0522

Precision CV (%): 0.9624 %

Equivalent vapor concent.: 0.0412 g/210L

Analyst	Name	Signature	Date
1	Estuardo J. Miranda		01/07/2005
2	Brian Capron		01/10/2005
3	Kari Gruendell		01/11/2005
4			
5			
6			
7			
8			
9			
10			
11			
12			

Prepared by: Estuardo J. Miranda according to the approved protocol



STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY
2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION
CERTIFICATION

I, Estuardo J. Miranda, do certify under penalty of perjury as follows:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: Bachelor of Science in Chemistry, Master of Science in Zoology, seven years experience in biochemical research and six years experience in Forensic Toxicology.

The quality assurance solution, Lot Number 05002 was prepared in the Washington State Toxicology Laboratory. I examined and tested this solution. The mean concentration of the alcohol was 0.0507 grams per 100ml.

Dated: 1/24/05
Seattle, WA

Estuardo J. Miranda
Forensic Toxicologist

EM/la
EMQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.

10-15-2007



STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION
CERTIFICATION

I, Brian Capron, do certify under penalty of perjury as follows:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: BS degree in Biology and eight years of experience in forensic toxicology.

The quality assurance solution, Lot Number 05002, was prepared in the Washington State Toxicology Laboratory. I examined and tested this solution. The mean concentration of the alcohol was 0.0507 grams per 100ml.

Dated: 1/24/05
Seattle, WA

Brian Capron
Forensic Toxicologist

BC/la
BCQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.



STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION
CERTIFICATION


I, Kari D. Gruendell, do certify under penalty of perjury as follows:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: BS degree in Biology and a minor in Chemistry and two years of analytical laboratory experience.

The quality assurance solution, Lot Number 05002, was prepared in the Washington State Toxicology Laboratory. I examined and tested this solution. The mean concentration of the alcohol was 0.0507 grams per 100ml.

Dated: 1/24/05
Seattle, WA


Kari D. Gruendell
Forensic Toxicologist

KDG/la
KDGQA



Sequence Parameters:

Operator: Estuardo J. Miranda
 Data File Naming: Auto
 Data Directory: D:\HPCHEM\1\DATA\
 Data Subdirectory: 050107EM
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none
 Sequence Comment:

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	Blank	BLDALCO	1	Sample		
2	Vial 2	Q.A. Sol 05002-1	BLDALCO	1	Sample		
3	Vial 3	Q.A. Sol 05002-2	BLDALCO	1	Sample		
4	Vial 4	Q.A. Sol 05002-3	BLDALCO	1	Sample		
5	Vial 5	Q.A. Sol 05002-4	BLDALCO	1	Sample		
6	Vial 6	Q.A. Sol 05002-5	BLDALCO	1	Sample		
7	Vial 7	0.100 Control EM	BLDALCO	1	Ctrl Samp		
8	Vial 8	Blank	BLDALCO	1	Sample		
9	Vial 9	Q.A. Sol 05003-1	BLDALCO	1	Sample		
10	Vial 10	Q.A. Sol 05003-2	BLDALCO	1	Sample		
11	Vial 11	Q.A. Sol 05003-3	BLDALCO	1	Sample		
12	Vial 12	Q.A. Sol 05003-4	BLDALCO	1	Sample		
13	Vial 13	Q.A. Sol 05003-5	BLDALCO	1	Sample		
14	Vial 14	0.100 Control EM	BLDALCO	1	Ctrl Samp		
15	Vial 15	Blank	BLDALCO	1	Sample		
16	Vial 16	050141	BLDALCO	1	Sample		
17	Vial 17	0.100 Control EM	BLDALCO	1	Ctrl Samp		
18	Vial 18	Blank	BLDALCO	1	Sample		


Sequence Table (Back Injector):

No entries - empty table!

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:12:08 PM
 Instrument 4
 DB-ALC1


Blank
 Estuardo J. Miranda

vial # 1

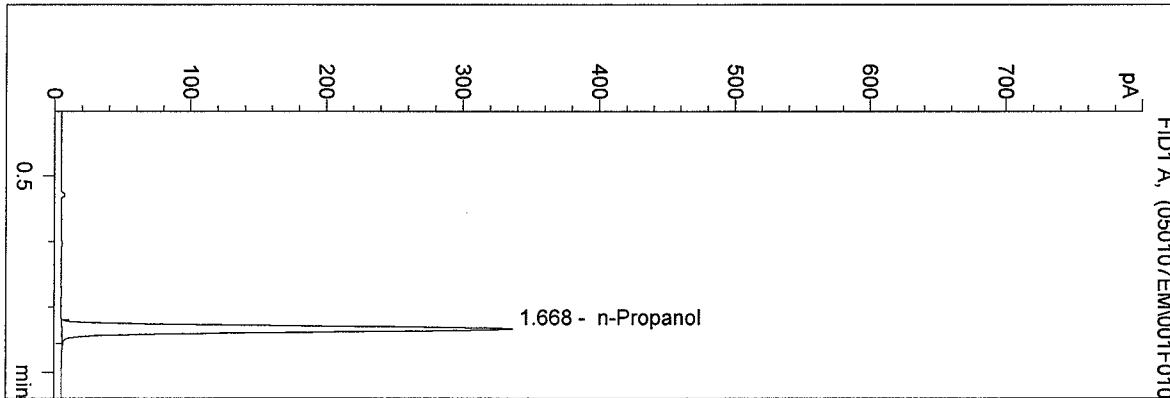


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1096	1.668

Totals:

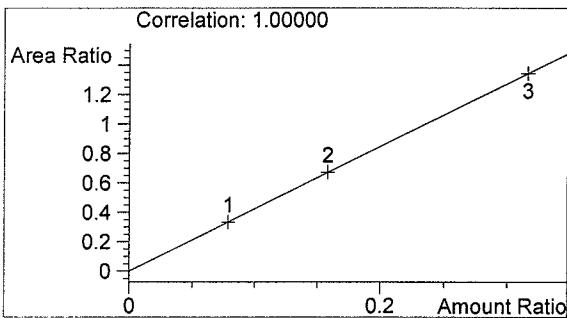

Ethanol 0.000 g/100ml

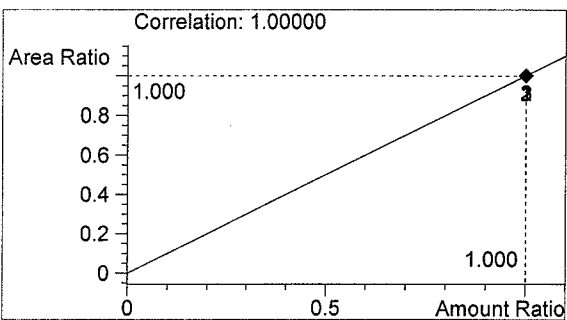


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:15:23 PM
 Instrument 4
 DB-ALC1


Q.A. Sol 05002-1
 Estuardo J. Miranda

vial # 2

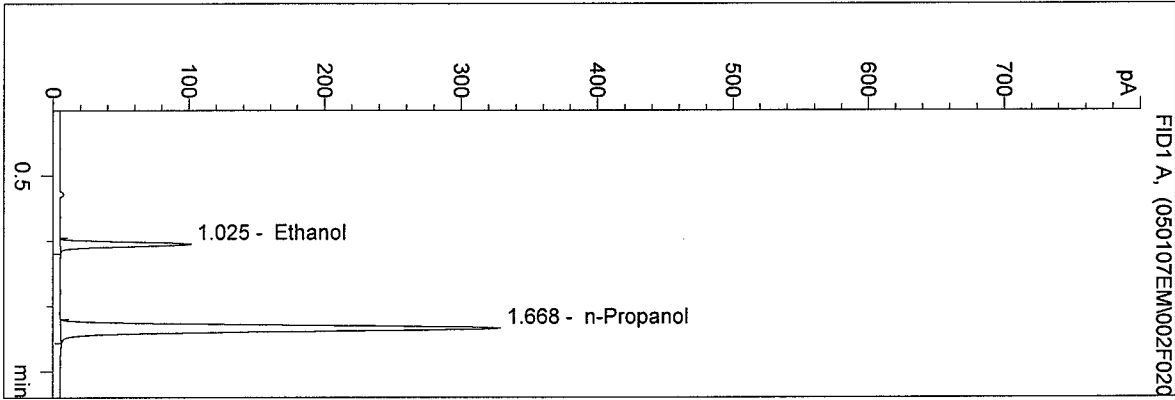


#	Compound	Area	RT
1	Ethanol	229	1.025
2	n-Propanol	1066	1.668

Totals:

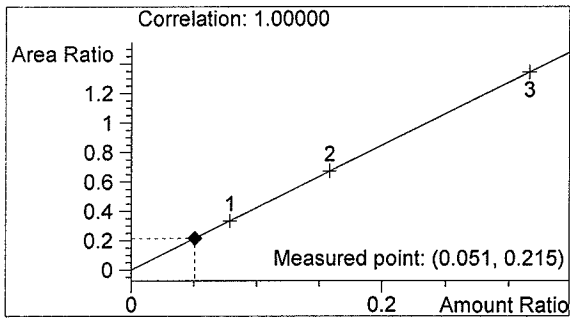

Ethanol 0.051 g/100ml

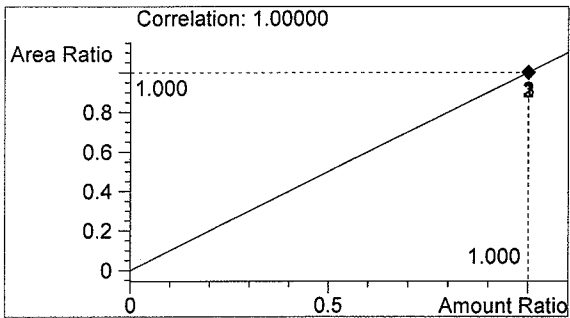


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:18:34 PM
 Instrument 4
 DB-ALC1


Q.A. Sol 05002-2
 Estuardo J. Miranda

vial # 3

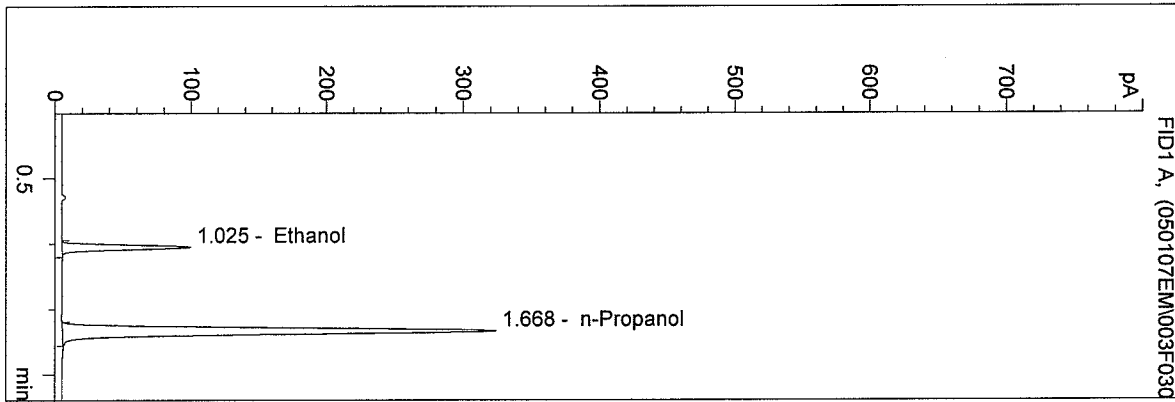


#	Compound	Area	RT
1	Ethanol	225	1.025
2	n-Propanol	1050	1.668

Totals:

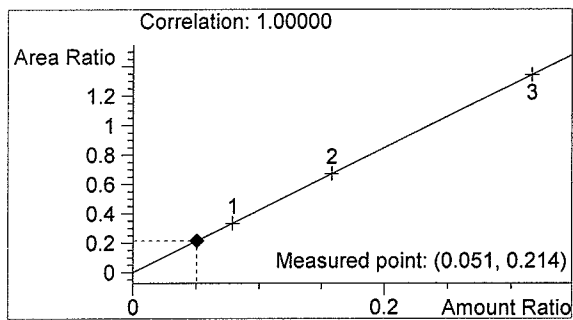

Ethanol 0.051 g/100ml

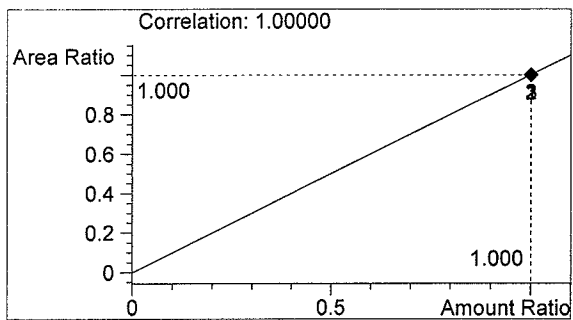


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:21:44 PM
 Instrument 4
 DB-ALC1


Q.A. Sol 05002-3
 Estuardo J. Miranda

vial # 4

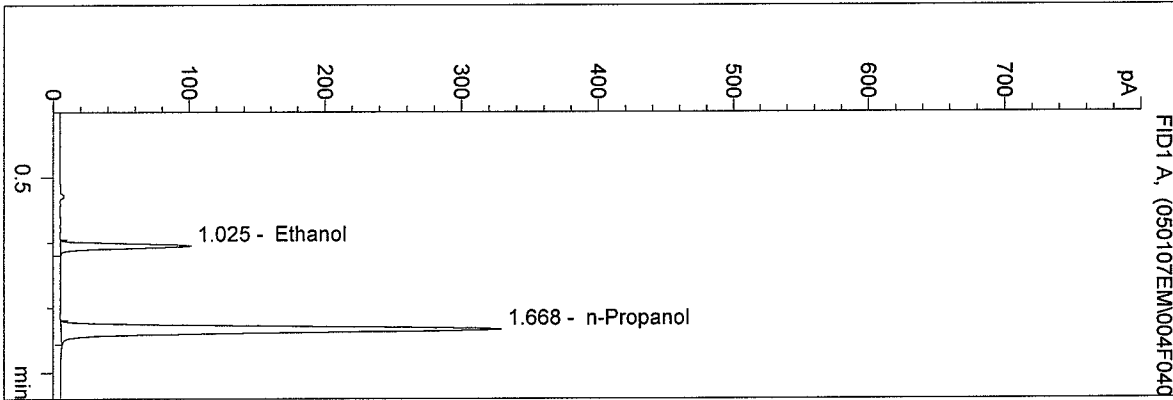


#	Compound	Area	RT
1	Ethanol	229	1.025
2	n-Propanol	1068	1.668

Totals:

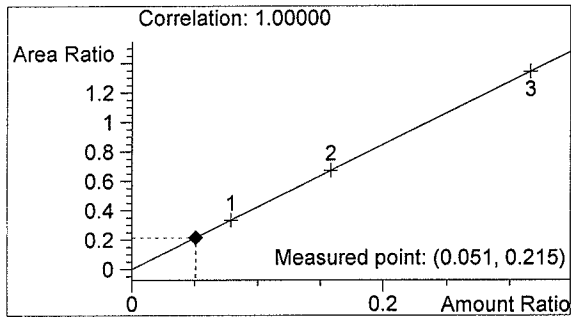

Ethanol 0.051 g/100ml

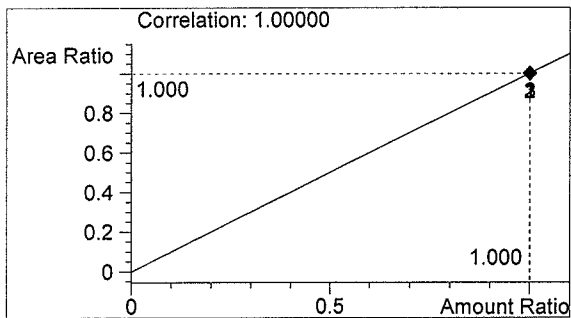


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:24:53 PM
 Instrument 4
 DB-ALC1


Q.A. Sol 05002-4
 Estuardo J. Miranda

vial # 5

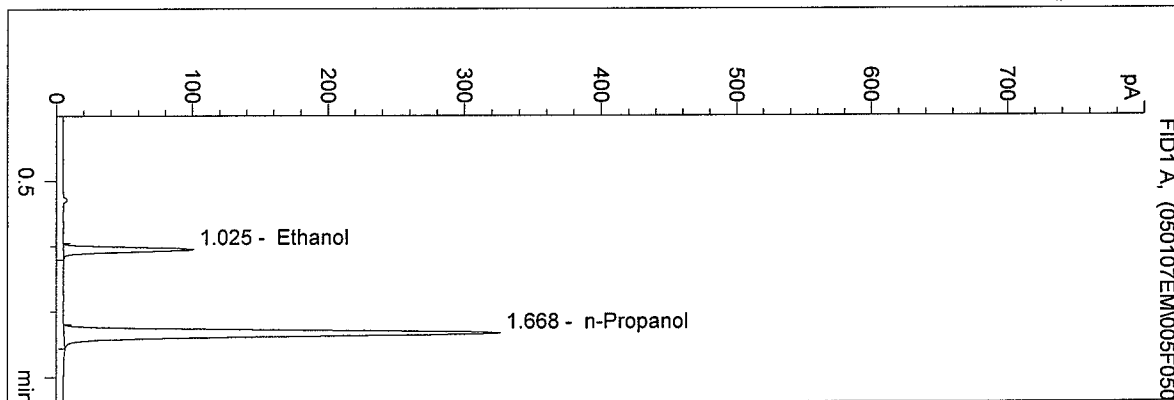


#	Compound	Area	RT
1	Ethanol	228	1.025
2	n-Propanol	1057	1.668

Totals:

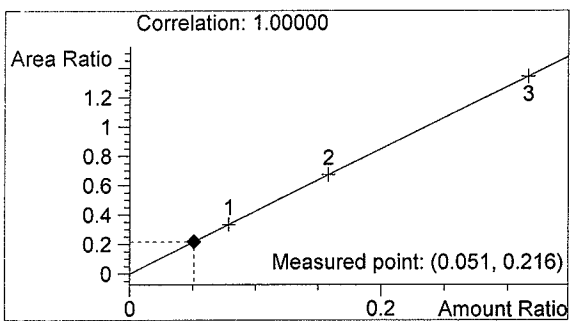

Ethanol 0.051 g/100ml

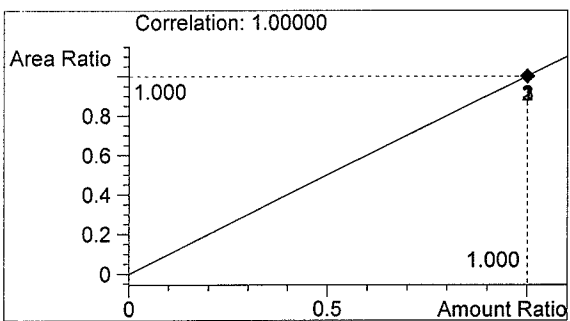


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:28:05 PM
 Instrument 4
 DB-ALC1


Q.A. Sol 05002-5
 Estuardo J. Miranda

vial # 6

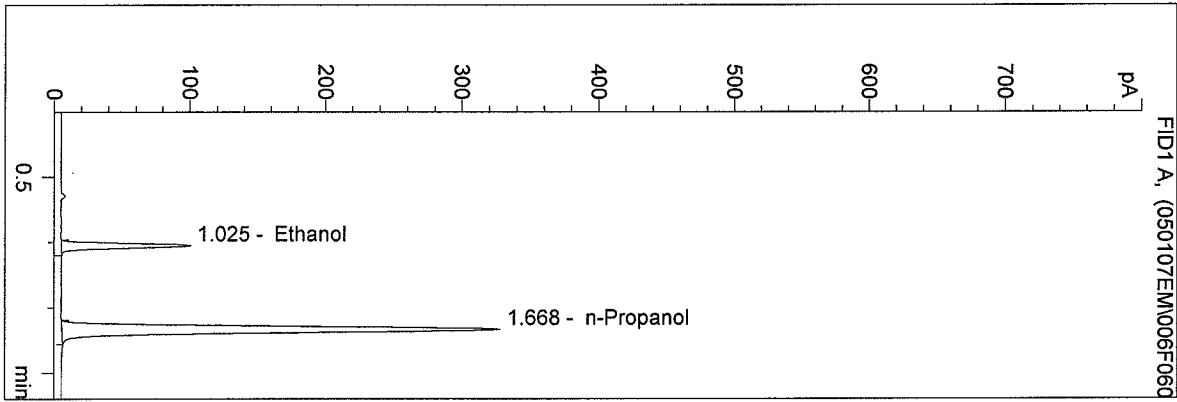


#	Compound	Area	RT
1	Ethanol	229	1.025
2	n-Propanol	1065	1.668

Totals:

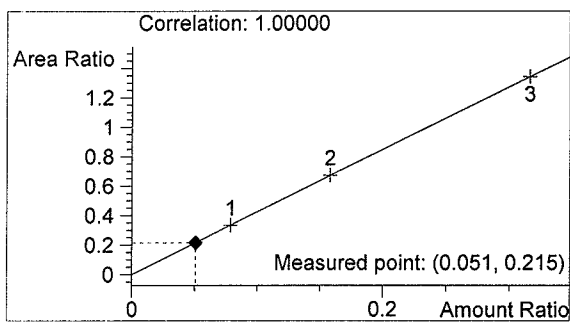

Ethanol 0.051 g/100ml

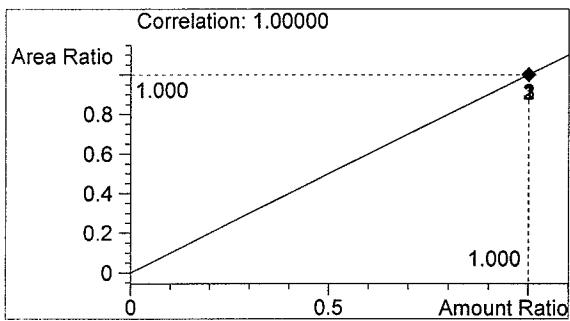


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:33:40 PM
 Instrument 4
 DB-ALC1


0.100 Control EM
 Estuardo J. Miranda

vial # 7

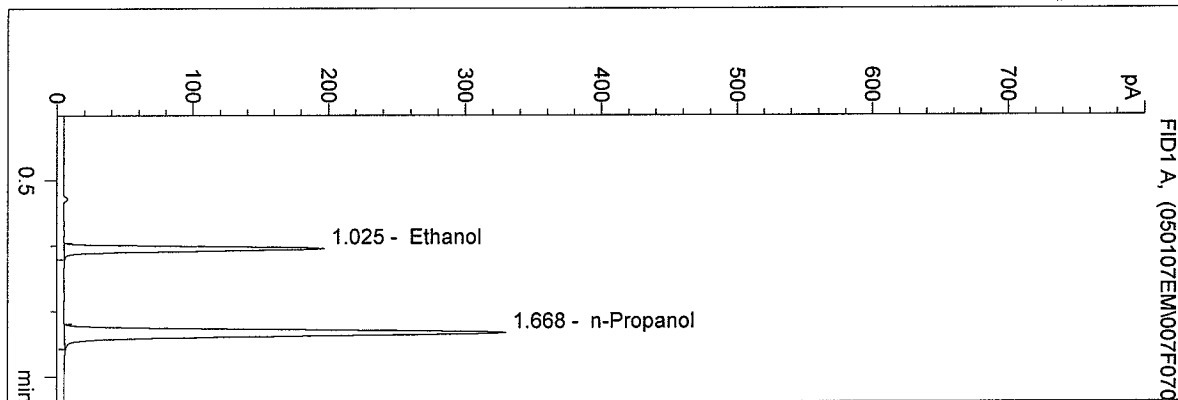


#	Compound	Area	RT
1	Ethanol	457	1.025
2	n-Propanol	1072	1.668

Totals:

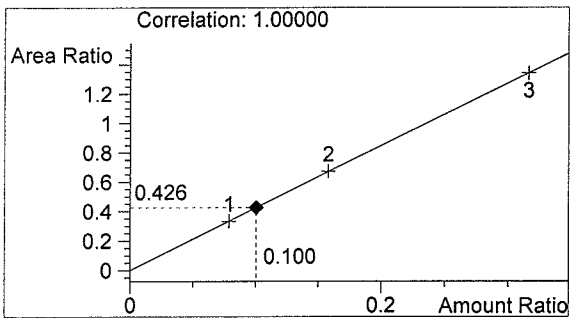

Ethanol 0.100 g/100ml

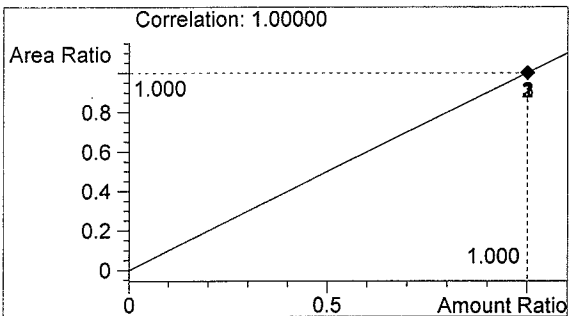


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/7/2005 3:36:52 PM
 Instrument 4
 DB-ALC1


Blank
 Estuardo J. Miranda

vial # 8

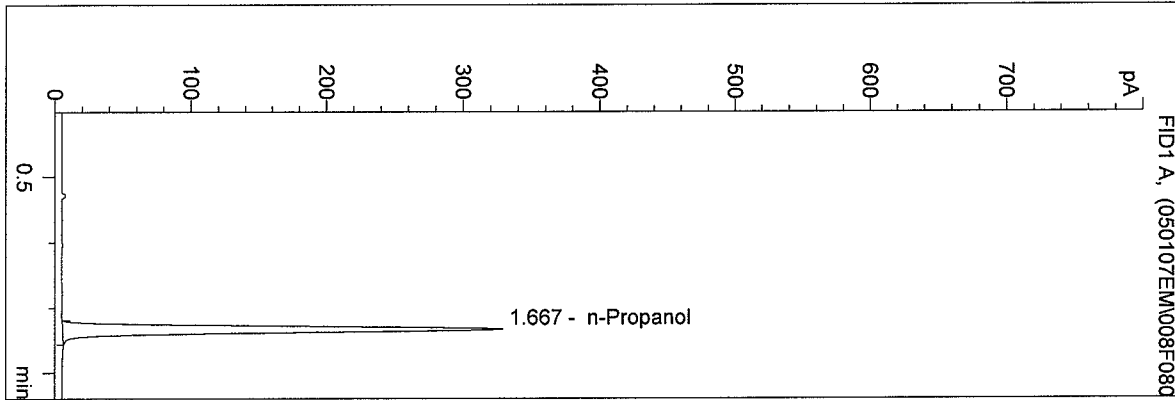


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1068	1.667

Totals:

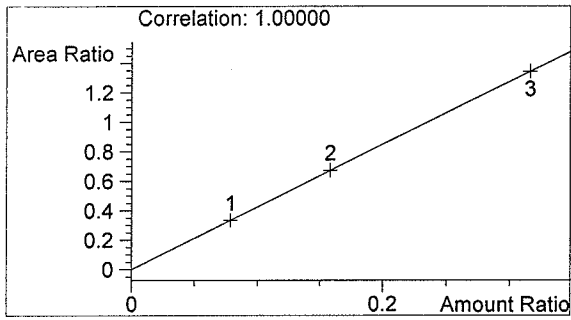

Ethanol 0.000 g/100ml

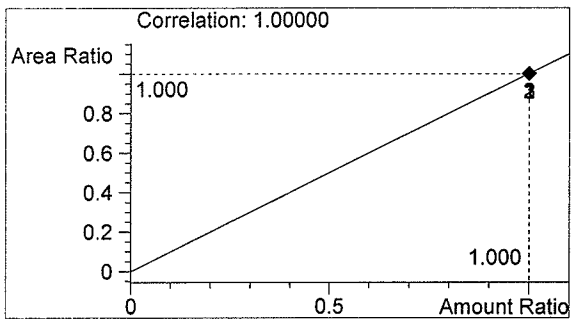


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:34:57 PM
 Instrument 4
 DB-ALC1


0.10 control
 bcapron

vial # 54

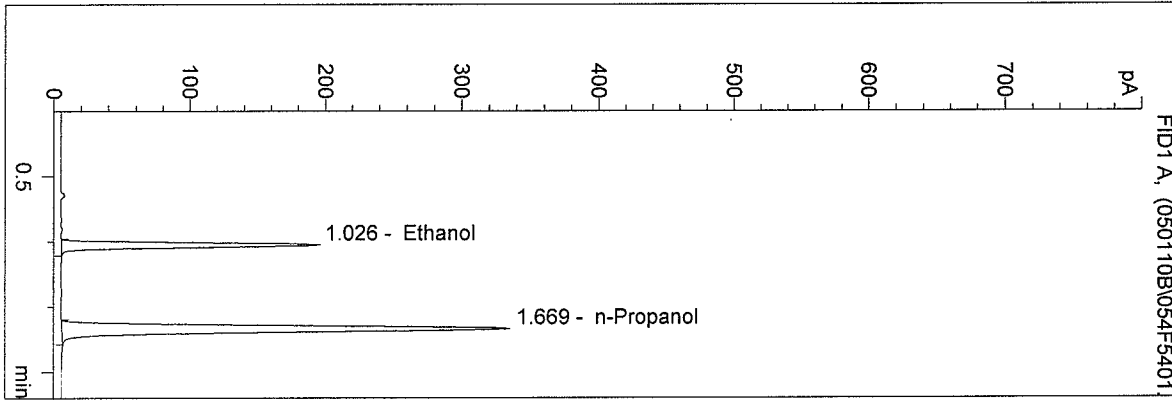


#	Compound	Area	RT
1	Ethanol	465	1.026
2	n-Propanol	1101	1.669

Totals:

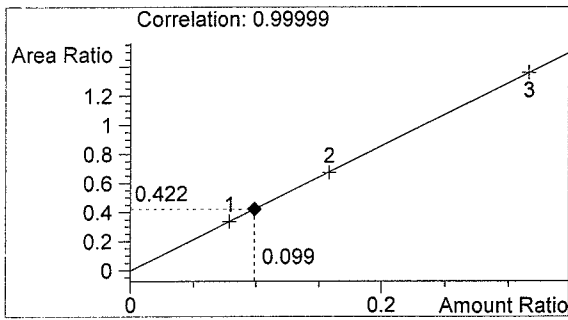

Ethanol 0.099 g/100ml

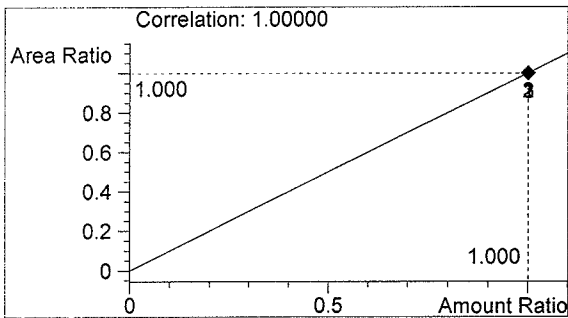


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:38:04 PM
 Instrument 4
 DB-ALC1


blank
 bcapron

vial # 55

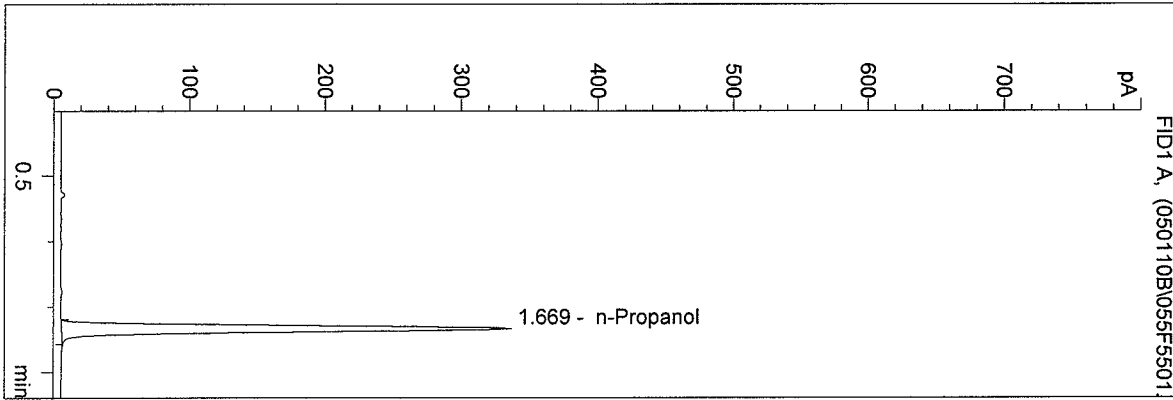


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1108	1.669

Totals:

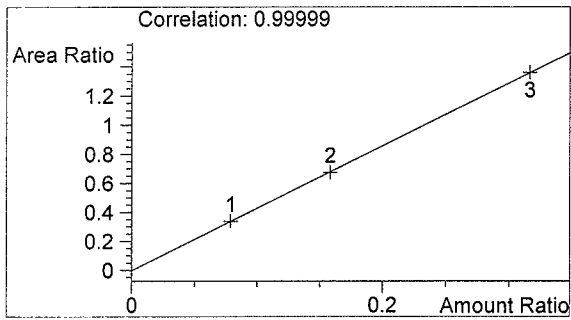

Ethanol 0.000 g/100ml

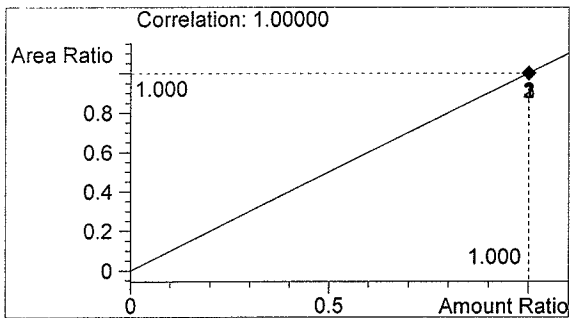


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:41:21 PM
 Instrument 4
 DB-ALC1


05002
 bcapron

vial # 56

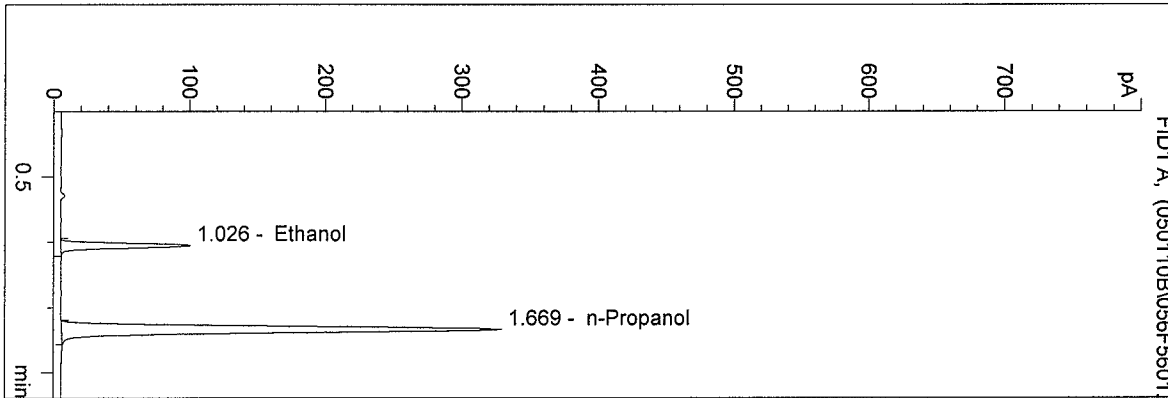


#	Compound	Area	RT
1	Ethanol	235	1.026
2	n-Propanol	1082	1.669

Totals:

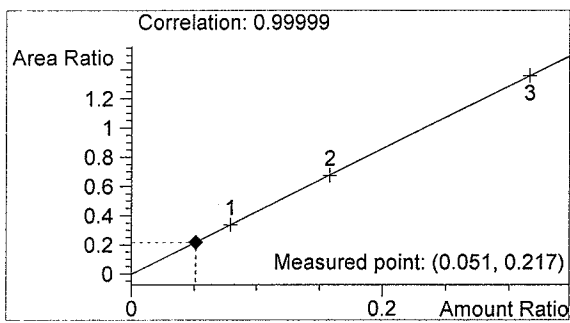

Ethanol 0.051 g/100ml

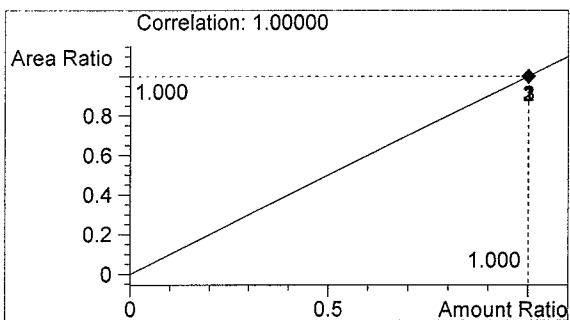


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:44:36 PM
 Instrument 4
 DB-ALC1


05002
 bcapron

vial # 57

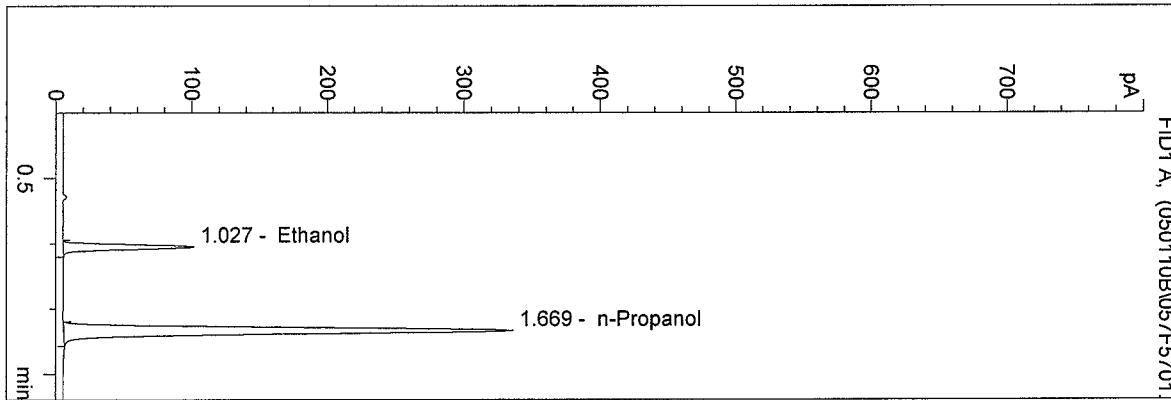


#	Compound	Area	RT
1	Ethanol	237	1.027
2	n-Propanol	1105	1.669

Totals:

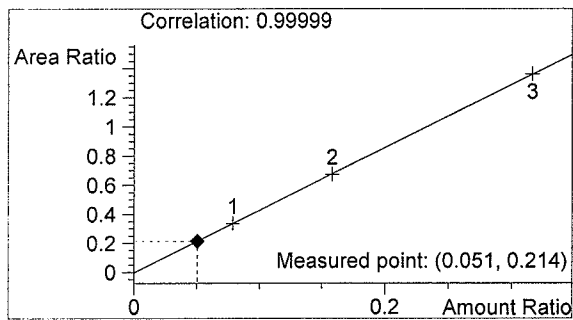

Ethanol 0.051 g/100ml

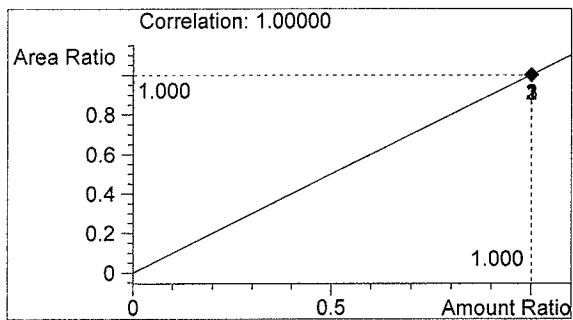


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:47:47 PM
 Instrument 4
 DB-ALC1


05002
 bcapron

vial # 58

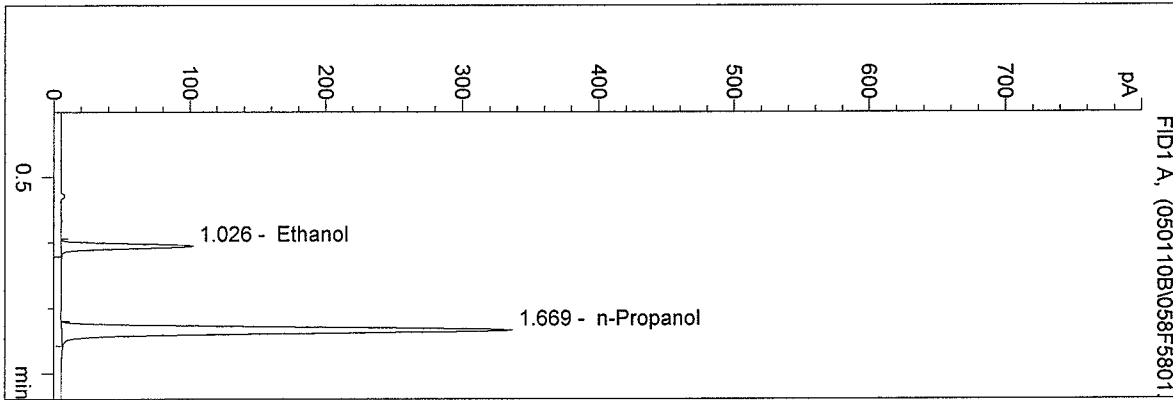


#	Compound	Area	RT
1	Ethanol	239	1.026
2	n-Propanol	1106	1.669

Totals:

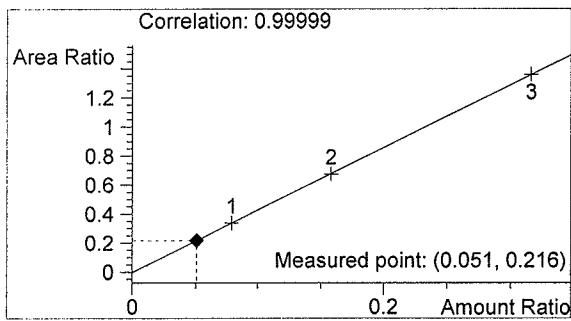

Ethanol 0.051 g/100ml

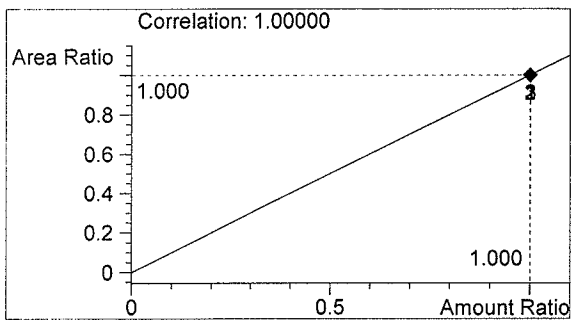


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:50:55 PM
 Instrument 4
 DB-ALC1


05002
 bcapron

vial # 59

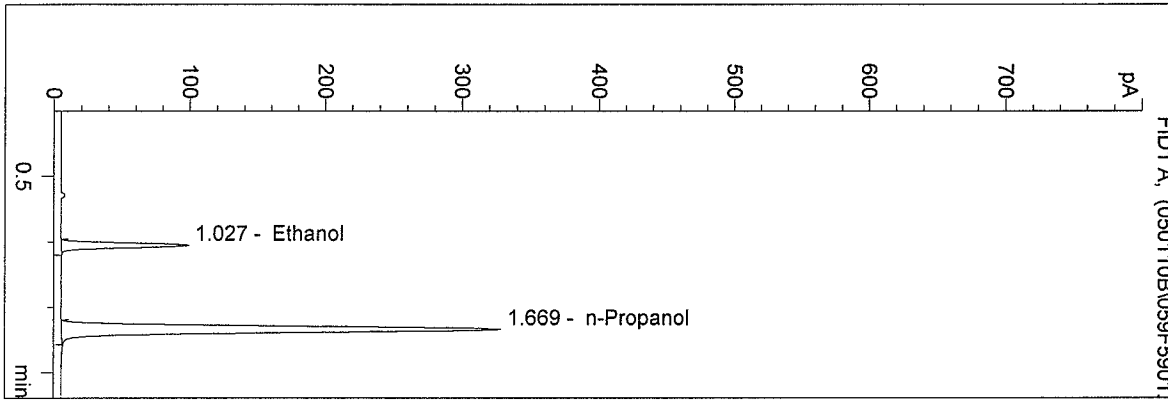


#	Compound	Area	RT
1	Ethanol	231	1.027
2	n-Propanol	1079	1.669

Totals:

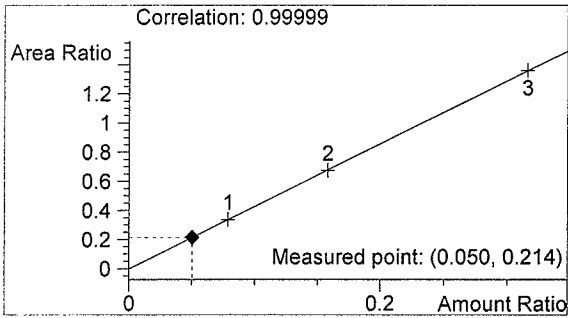

Ethanol 0.050 g/100ml

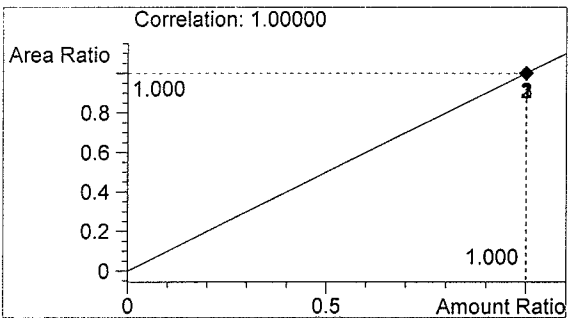


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 1/10/2005 12:54:02 PM
 Instrument 4
 DB-ALC1


05002
 bcapron

vial # 60

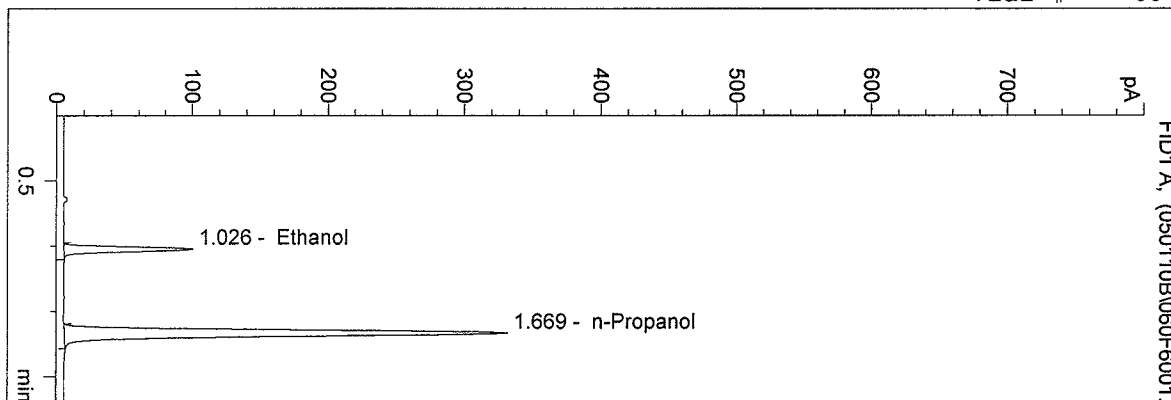


#	Compound	Area	RT
1	Ethanol	233	1.026
2	n-Propanol	1089	1.669

Totals:

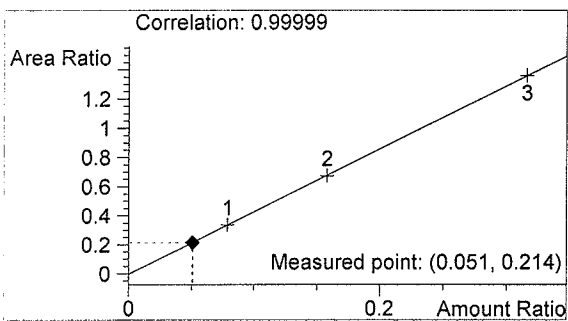

Ethanol 0.051 g/100ml

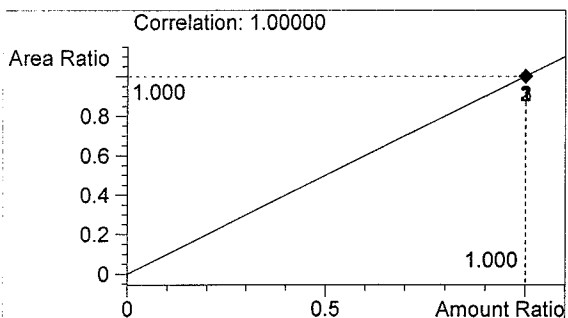


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 2:41:53 PM
 Instrument 5
 DB-ALC2


05002 QA #1
 Kari Gruendell

vial # 64

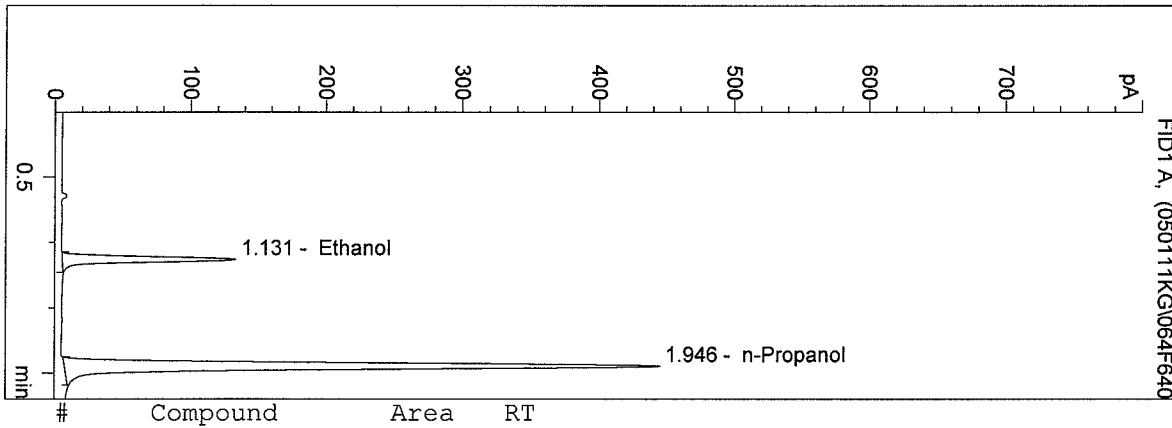


#	Compound	Area	RT
1	Ethanol	363	1.131
2	n-Propanol	1488	1.946

Totals:

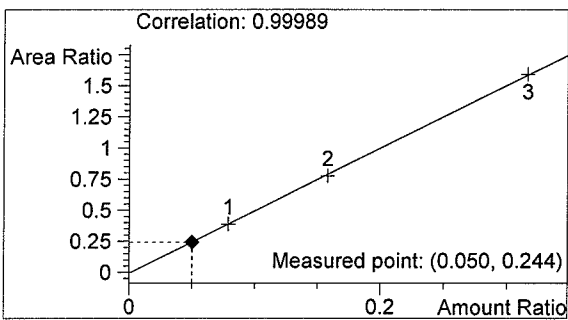

Ethanol 0.050 g/100ml

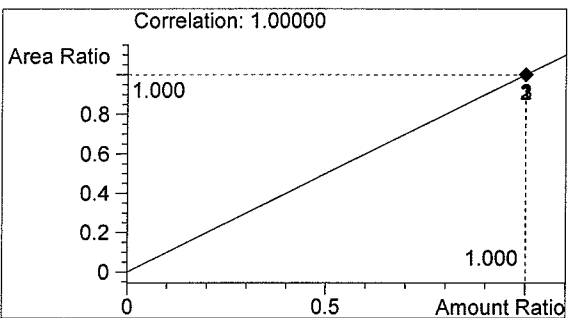


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 2:44:39 PM
 Instrument 5
 DB-ALC2


05002 QA #2
 Kari Gruendell

vial # 65

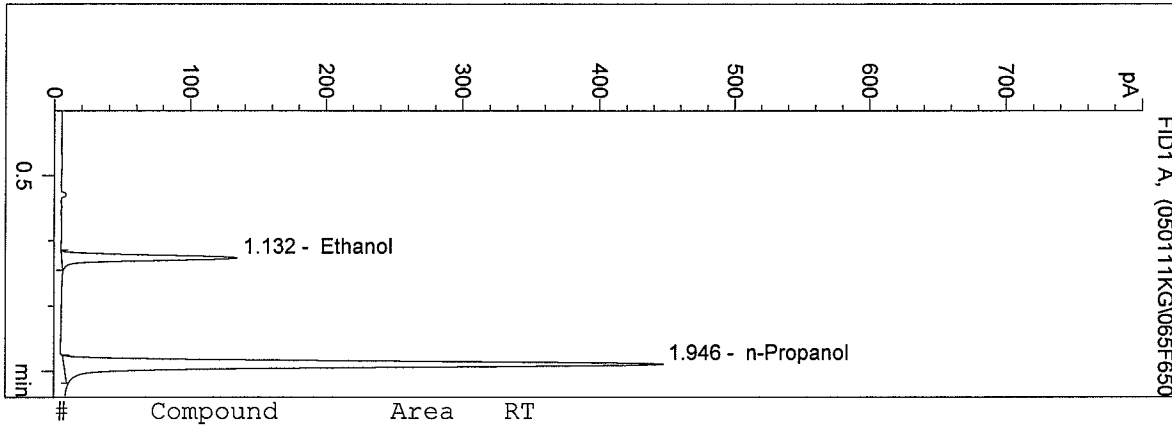


#	Compound	Area	RT
1	Ethanol	367	1.132
2	n-Propanol	1501	1.946

Totals:

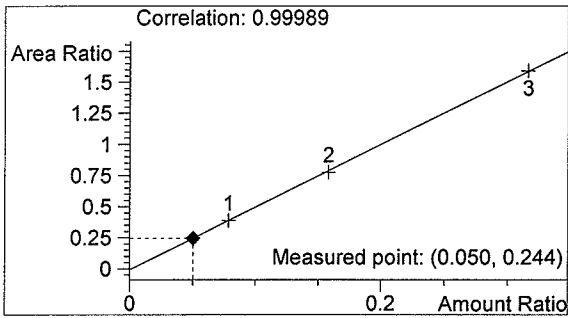

Ethanol 0.050 g/100ml

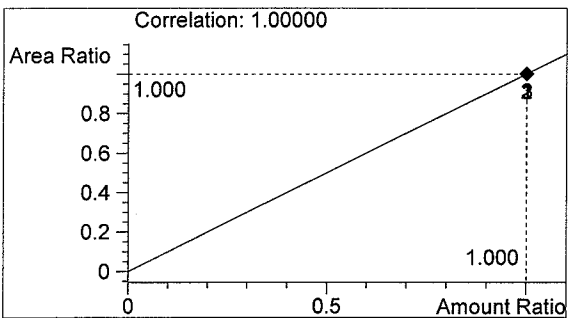


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 2:48:09 PM
 Instrument 5
 DB-ALC2


05002 QA #3
 Kari Gruendell

vial # 66

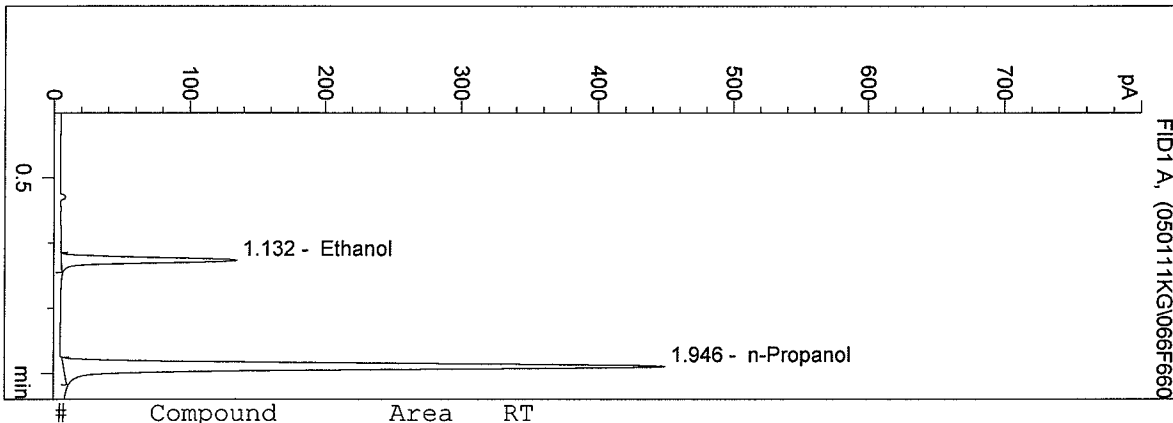


#	Compound	Area	RT
1	Ethanol	372	1.132
2	n-Propanol	1510	1.946

Totals:

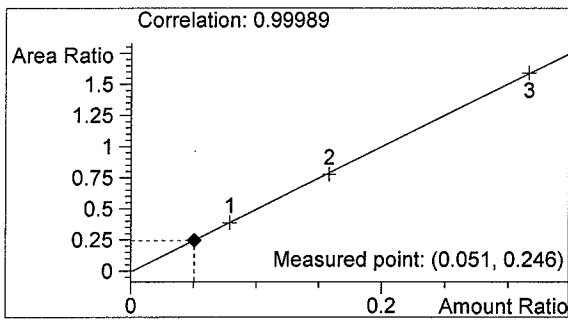

Ethanol 0.051 g/100ml

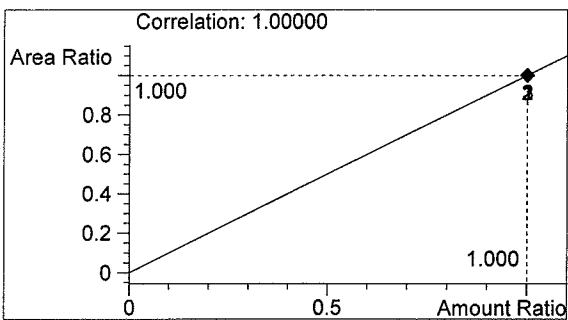


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 2:50:53 PM
 Instrument 5
 DB-ALC2


05002 QA #4
 Kari Gruendell

vial # 67

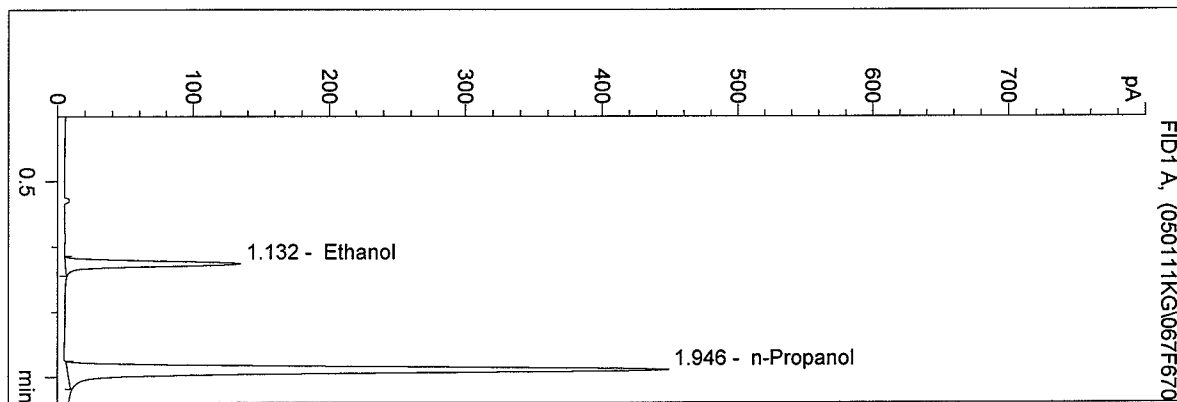


#	Compound	Area	RT
1	Ethanol	369	1.132
2	n-Propanol	1506	1.946

Totals:

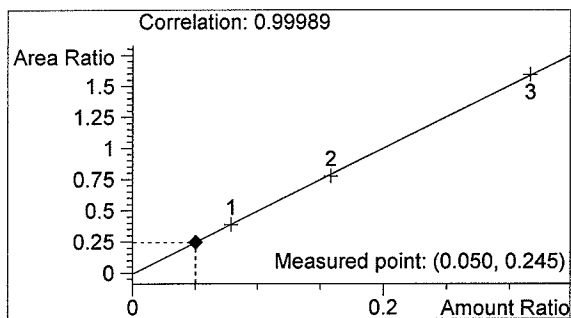

Ethanol 0.050 g/100ml

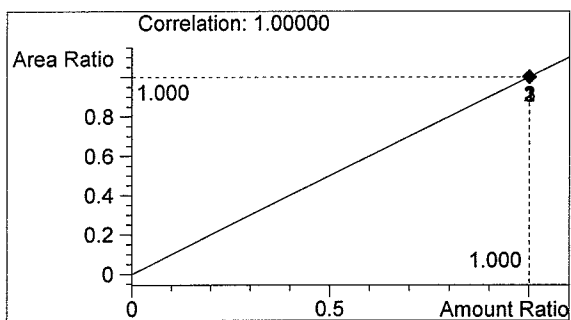


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 2:53:49 PM
 Instrument 5
 DB-ALC2


05002 QA #5
 Kari Gruendell

vial # 68

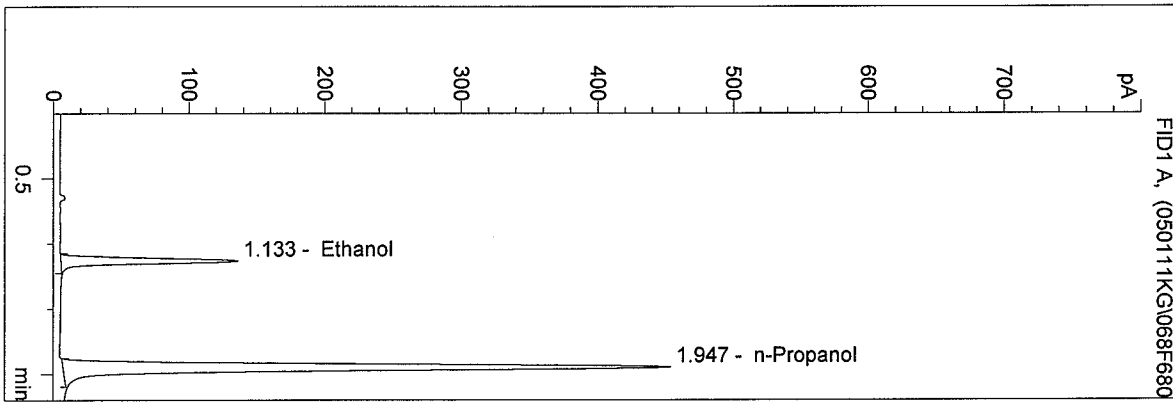


#	Compound	Area	RT
1	Ethanol	375	1.133
2	n-Propanol	1533	1.947

Totals:

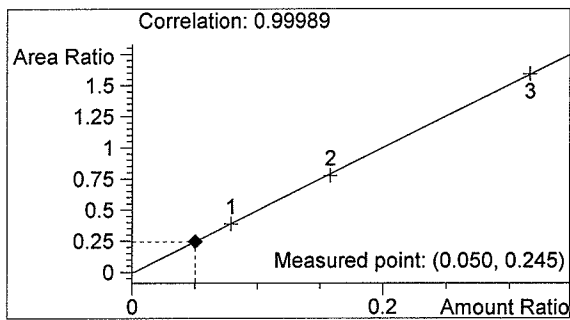

Ethanol 0.050 g/100ml

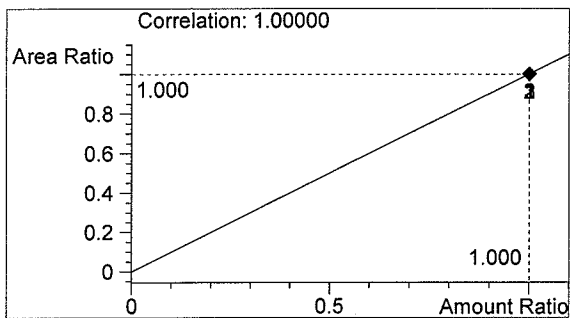


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 2:56:45 PM
 Instrument 5
 DB-ALC2


0.10 CONTROL
 Kari Gruendell

vial # 69

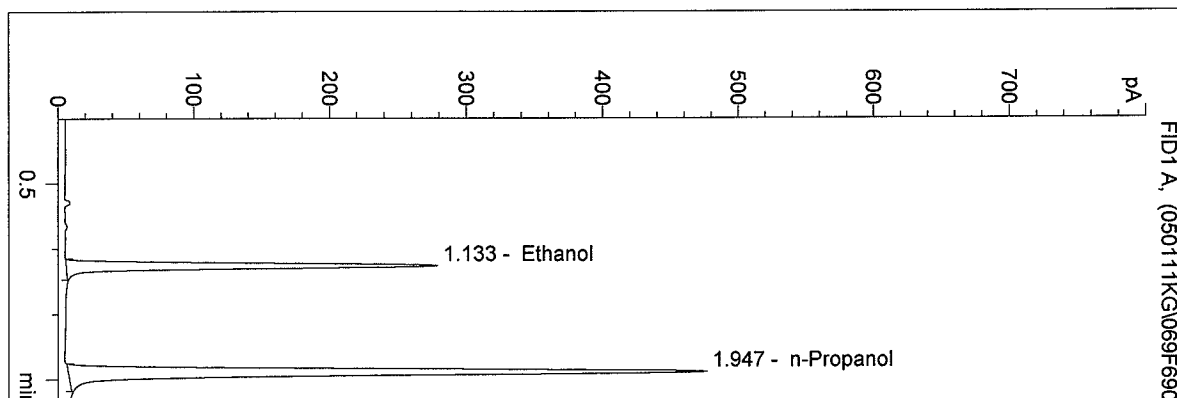


#	Compound	Area	RT
1	Ethanol	782	1.133
2	n-Propanol	1605	1.947

Totals:

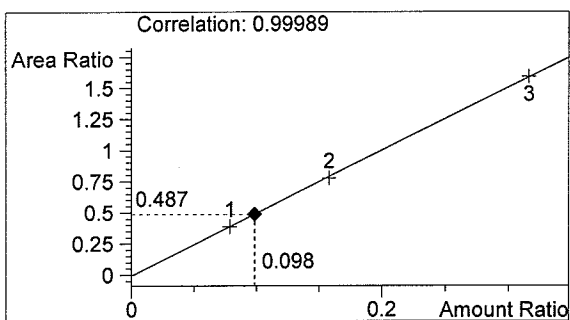

Ethanol 0.098 g/100ml

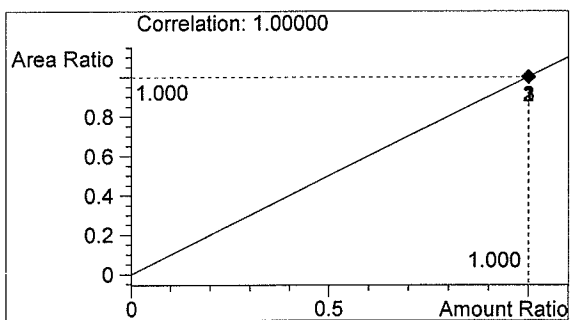


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 1/11/2005 3:00:00 PM
 Instrument 5
 DB-ALC2


BLANK
 Kari Gruendell

vial # 70

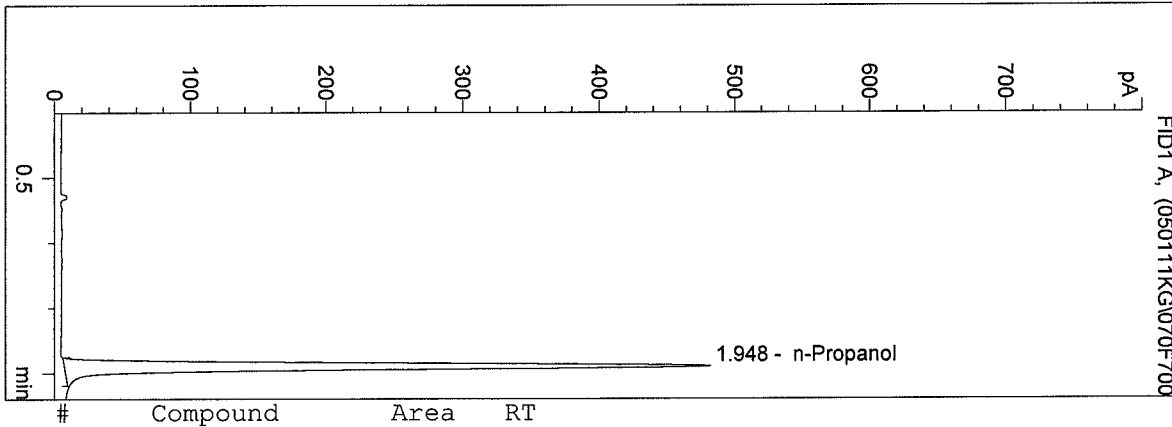


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1634	1.948

Totals:

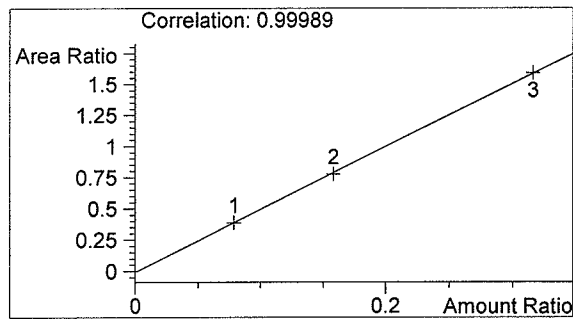

Ethanol 0.000 g/100ml

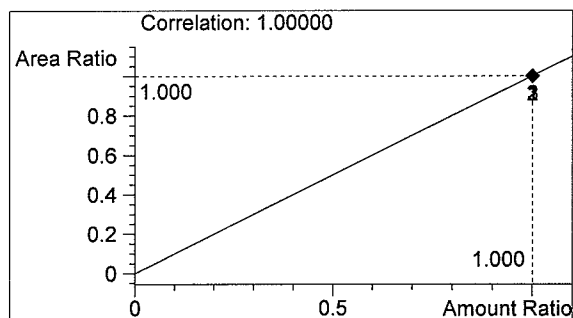

n-Propanol 1.000 g/100ml