


## Notice of Simulator Solution File Review

At the request of the State Toxicologist a review of the following simulator solution records has been accomplished. The following file consists of simulator solution analyses performed and completed by the State Toxicology Laboratory for a specific batch number. The file contains the simulator solution data entry form along with a file review record and the chromatograms generated by the Toxicology Laboratory during the analyses of the solutions. This file has been reviewed by Tpr. Ken Denton and Mr. Rod Gullberg for accuracy and completeness. Where computations regarding simulator solution values have been found to be incorrect, the corrected values have been written in by Mr. Rod Gullberg along with initials and date. The corrected values were then evaluated to ensure that the solution still conformed to those standards established by the State Toxicologist.


Where computation values changed for a specific batch number, the analysts employed by the State Toxicology Laboratory were asked to review the revisions, ensure the solution complied with the criteria established by the State Toxicologist and then re-sign their affidavit. Their signature will appear on their original affidavit along with a statement regarding their review of the results.

Where a dating error occurred that analyst will have made the correction on the original data form including their initials and date and then re-signed their original affidavit.

  
\_\_\_\_\_ 10/8/2007

Tpr. Ken Denton

Date

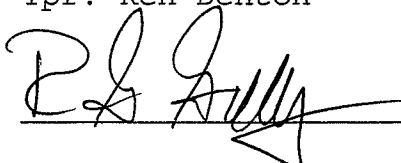  
\_\_\_\_\_ 10-8-07

Rod G. Gullberg

Date

Washington State Toxicology Laboratory  
Simulator Solution Data Entry Review Form

Reviewer KEN DELTON / ROD GULLBERG Date 10-4-07  
Location TOX LAB SEATTLE Batch Number 06024

Form Review Criteria

Preparation date precedes all analysis dates: Okay  Not Okay \_\_\_  
Data entry corresponds to all chromatograms: Okay  Not Okay \_\_\_  
All signatures present: Okay  Not Okay \_\_\_

Computations:

Avg. solution concentration: Correct  Not Correct \_\_\_  
Standard deviation: Correct  Not Correct \_\_\_  
Range: Correct  Not Correct \_\_\_  
Precision: Correct  Not Correct \_\_\_  
Equivalent vapor concent.: Correct  Not Correct \_\_\_  
External Control Information  
(lot # and future date): Correct  Not Correct \_\_\_

Complies with accuracy and precision requirements established by the  
State Toxicologist: Yes  No \_\_\_

Corrections Necessary:

Comments:

Reviewer Signature: [Signature] Date: 10-4-07  
Reviewer Signature: [Signature] Date: 10/4/2007

**WASHINGTON STATE TOXICOLOGY LABORATORY**  
**FORENSIC LABORATORY SERVICES BUREAU**  
**WASHINGTON STATE PATROL**  
 2203 AIRPORT WAY S, SUITE 360  
 SEATTLE, WASHINGTON 98134-2027  
 (206) 262-6100 FAX (206) 262-6145




Preparation and certification of **0.15** g/210L Quality Assurance solution  
 Batch number **06024** Date: 5/17/2006  
 Preparation: 42.3 mL of absolute ethyl alcohol diluted to 18 Liters with water  
 Concentration of ethanol (g/100mL) measured by gas chromatography:

	Anal 1	Anal 2	Anal 3	Anal 4	Anal 5	Anal 6	Anal 7	Anal 8	Anal 9	Anal 10	Anal 11	Anal 12	Anal 13	Anal 14	Anal 15	Anal 16
1	0.186	0.184	0.183													
2	0.190	0.191	0.184													
3	0.191	0.187	0.184													
4	0.188	0.187	0.184													
5	0.191	0.189	0.184													
Ctrl	0.102	0.102	0.101													

**External Control:**  
 Lot #: a035928-20 Exp date: 7/09  
 Target concentration: 0.10 g/100mL

**Statistics:**  
 Avg. solution concent.: 0.1869 g/100 mL  
 SD: 0.00297  
 Range (3xSD): 0.1780 to 0.1958  
 Precision CV (%): 1.5906 %

**Equivalent vapor concent.:** 0.1520 g/210L

Analyst	Name	Signature	Date
1	Edward Formoso		05/19/2006
2	Kelly Gross		05/23/2006
3	Brianne Akins		05/23/2006
4			
5			
6			
7			
8			
9			
10			
11			
12			
13			
14			
15			
16			

Prepared by: Edward Formoso according to the approved protocol



STATE OF WASHINGTON  
WASHINGTON STATE PATROL

WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360•Seattle, Washington 98134-2927•(206) 262-6100•FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION  
CERTIFICATION

I, Edward J. Formoso, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: BS degree in Chemistry and twenty-nine years of experience in the Washington State Toxicology Laboratory.

The quality assurance solution, Lot Number 06024, was prepared in the Washington State Toxicology Laboratory on 5/17/2006. I examined and tested this solution. The mean concentration of the alcohol was 0.1869 grams per 100ml.

Dated: 5/24/2006  
Seattle, WA

---

Edward J. Formoso  
Forensic Toxicologist

EJF/ks  
EFQA



STATE OF WASHINGTON  
WASHINGTON STATE PATROL

WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360•Seattle, Washington 98134-2927•(206) 262-6100•FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION  
CERTIFICATION

I, Kelly D. Gross, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: B.S. degree in Chemistry and fifteen years of forensic laboratory experience.

The quality assurance solution, Lot Number 06024, was prepared in the Washington State Toxicology Laboratory on 5/17/2006. I examined and tested this solution. The mean concentration of the alcohol was 0.1869 grams per 100ml.

Dated: 5/24/2006  
Seattle, WA

Kelly D. Gross  
Forensic Toxicologist

KDG/ks  
KDGQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.

10052007



STATE OF WASHINGTON  
WASHINGTON STATE PATROL

WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360•Seattle, Washington 98134-2927•(206) 262-6100•FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION  
CERTIFICATION

I, Brianne E. Akins, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: BS degree in Biology.

The quality assurance solution, Lot Number 06024, was prepared in the Washington State Toxicology Laboratory on 5/17/2006. I examined and tested this solution. The mean concentration of the alcohol was 0.1869 grams per 100ml.

Dated: 5/24/2006  
Seattle, WA

*Brianne E. Akins*

Brianne E. Akins  
Forensic Toxicologist

BEA/ks  
BAQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.


*Brianne E. Akins 10507*



D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/19/2006 2:45:05 PM  
 Instrument 5  
 DB-ALC2


06024  
 SIMULATOR SOLUTION

vial # 15

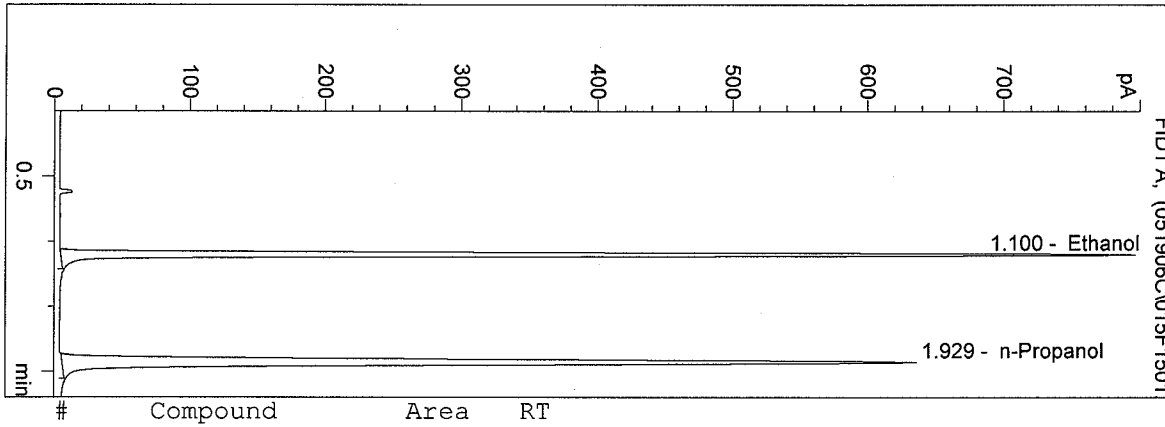


#	Compound	Area	RT
1	Ethanol	1579	1.100
2	n-Propanol	1838	1.929

Totals:

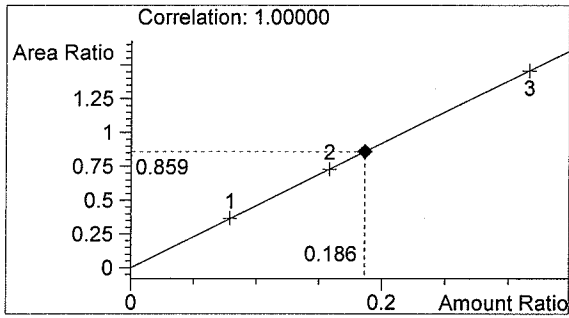

Ethanol 0.186 g/100ml

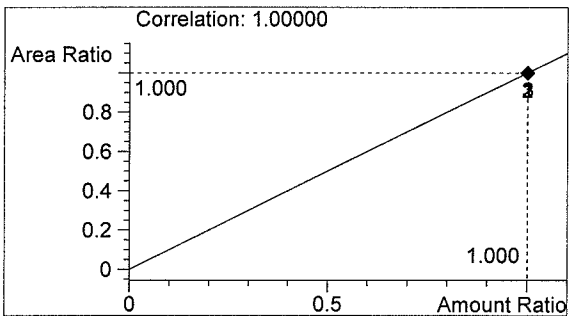


n-Propanol 1.000 g/100ml

EF  
 06024  
 RLL  
 10-8-07

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/19/2006 2:48:14 PM  
 Instrument 5  
 DB-ALC2


06024  
 SIMULATOR SOLUTION

vial # 16

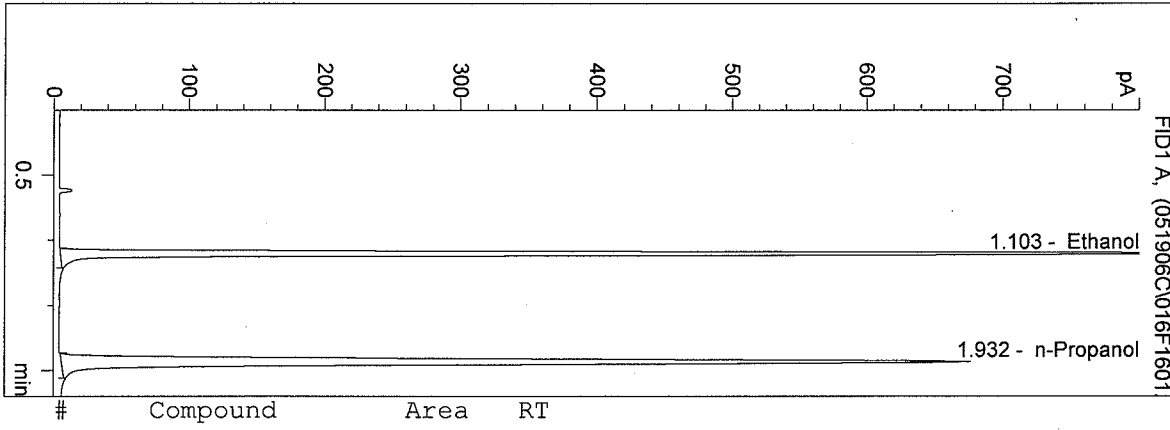


#	Compound	Area	RT
1	Ethanol	1718	1.103
2	n-Propanol	1957	1.932

Totals:



Ethanol 0.190 g/100ml




n-Propanol 1.000 g/100ml



D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/19/2006 2:51:23 PM  
 Instrument 5  
 DB-ALC2


06024  
 SIMULATOR SOLUTION

vial # 17

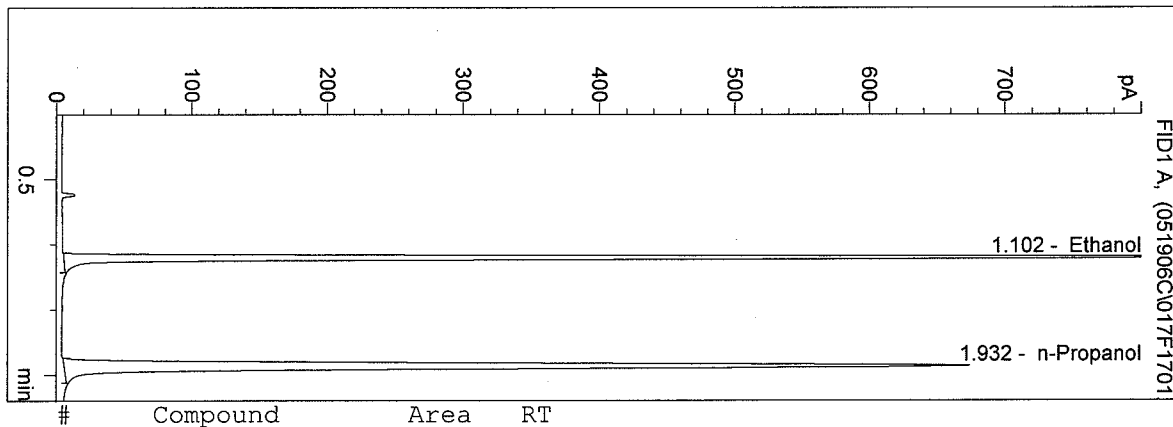


#	Compound	Area	RT
1	Ethanol	1718	1.102
2	n-Propanol	1954	1.932

Totals:

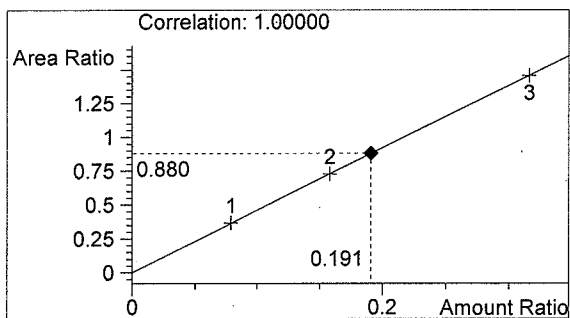

Ethanol 0.191 g/100ml

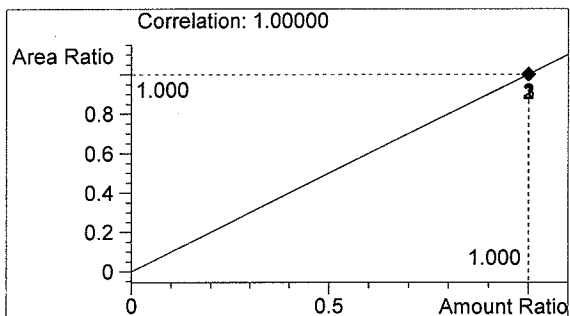


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/19/2006 2:54:39 PM  
 Instrument 5  
 DB-ALC2


06024  
 SIMULATOR SOLUTION

vial # 18

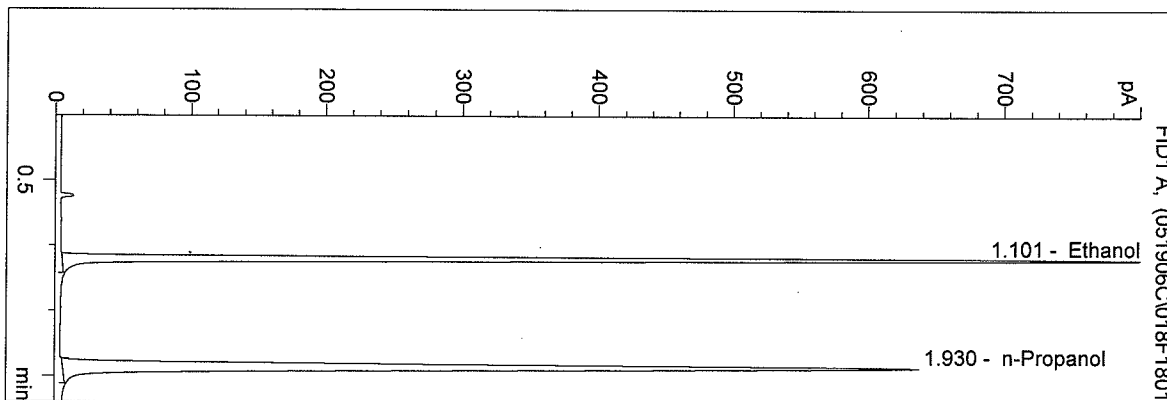


#	Compound	Area	RT
1	Ethanol	1596	1.101
2	n-Propanol	1845	1.930

Totals:

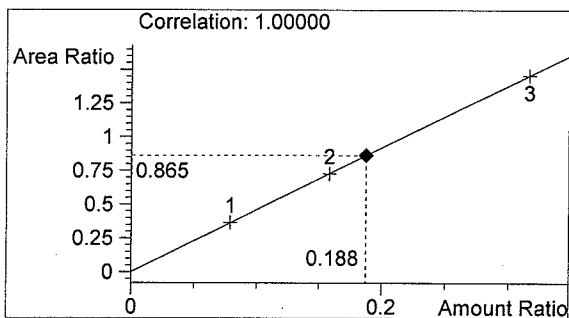

Ethanol 0.188 g/100ml

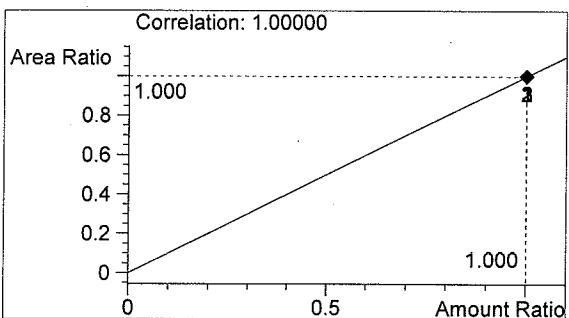


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/19/2006 2:57:57 PM  
 Instrument 5  
 DB-ALC2


06024  
 SIMULATOR SOLUTION

vial # 19

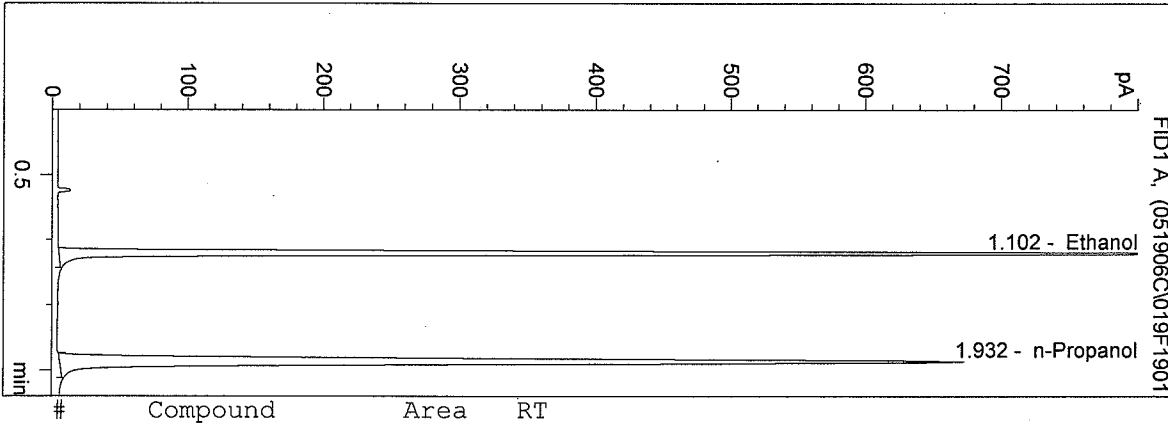


#	Compound	Area	RT
1	Ethanol	1711	1.102
2	n-Propanol	1948	1.932

Totals:

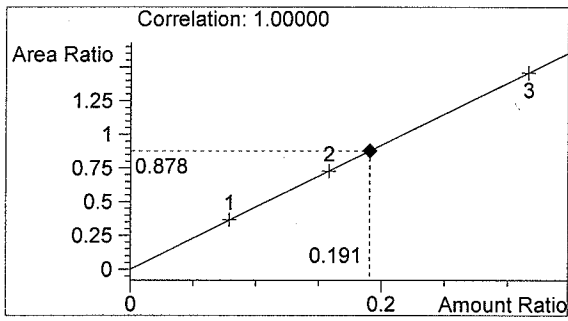

Ethanol 0.191 g/100ml




n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/19/2006 3:01:11 PM  
 Instrument 5  
 DB-ALC2


0.10 CONTROL  
 SIMULATOR SOLUTION

vial # 20

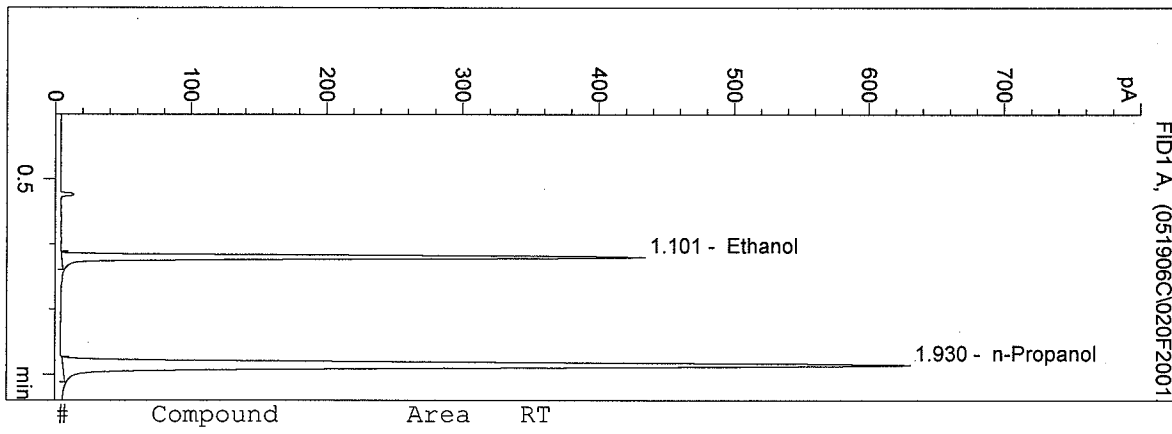


#	Compound	Area	RT
1	Ethanol	859	1.101
2	n-Propanol	1826	1.930

Totals:

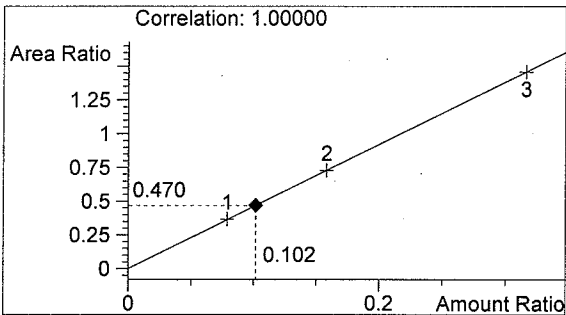

Ethanol 0.102 g/100ml

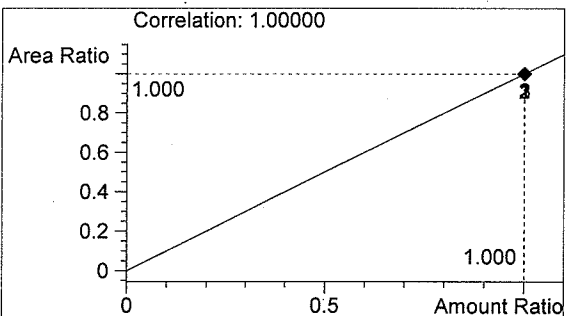


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:22:12 AM  
 Instrument 5  
 DB-ALC2


0.10 CTL-KDG  
 kgross

vial # 15

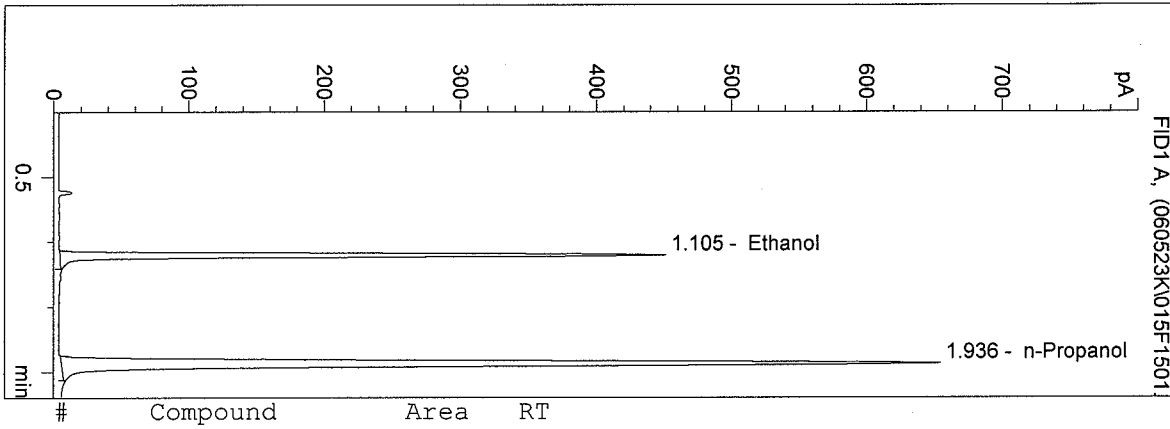


#	Compound	Area	RT
1	Ethanol	901	1.105
2	n-Propanol	1903	1.936

Totals:

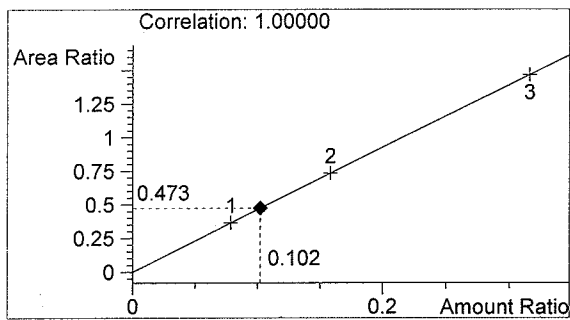

Ethanol 0.102 g/100ml

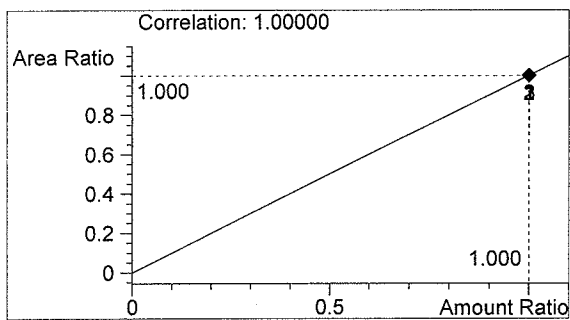


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:25:22 AM  
 Instrument 5  
 DB-ALC2


blank  
 kgross

vial # 16

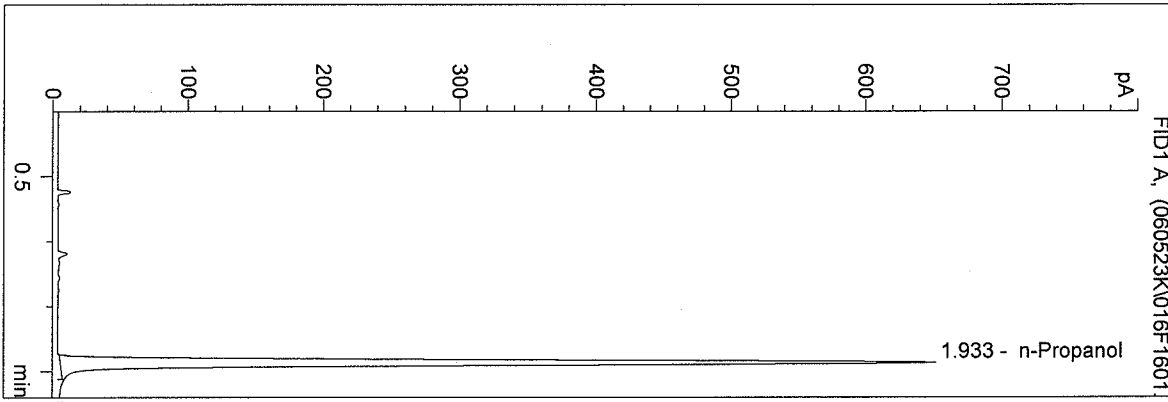


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1886	1.933

Totals:

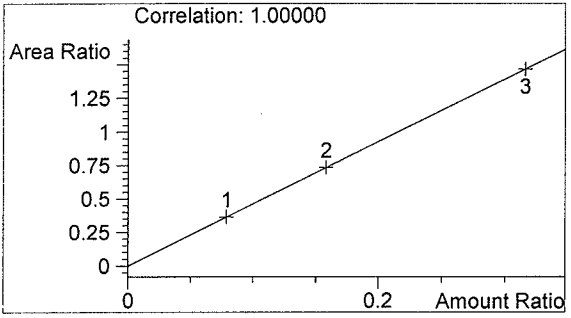

Ethanol 0.000 g/100ml

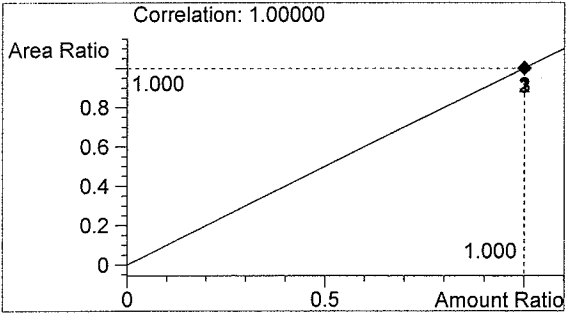


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:28:30 AM  
 Instrument 5  
 DB-ALC2


06024qa  
 kgross

vial # 17

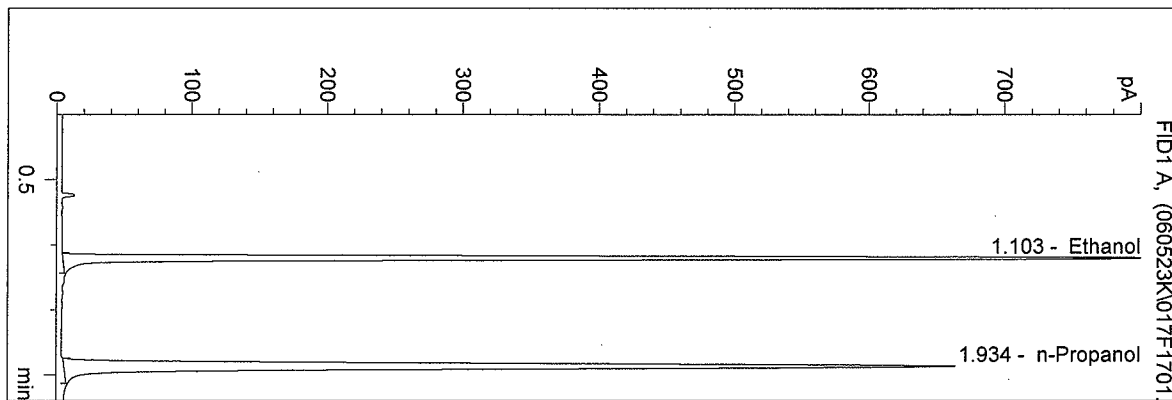


#	Compound	Area	RT
1	Ethanol	1649	1.103
2	n-Propanol	1930	1.934

Totals:

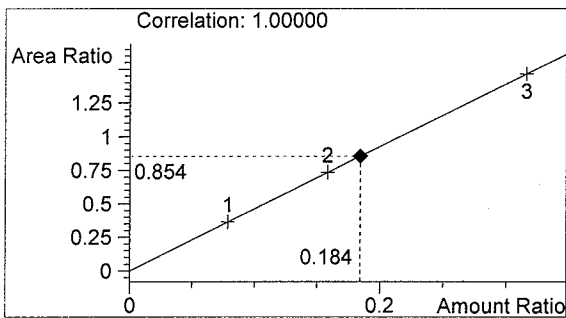

Ethanol 0.184 g/100ml

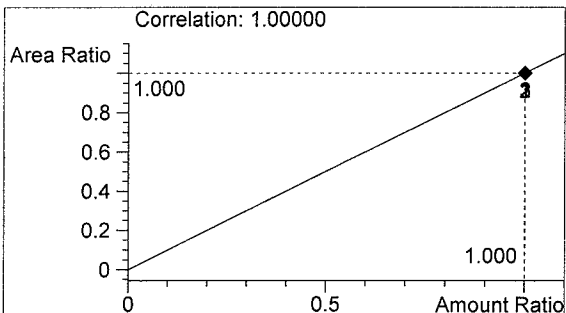


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:31:47 AM  
 Instrument 5  
 DB-ALC2


06024qa  
 kgross

vial # 18

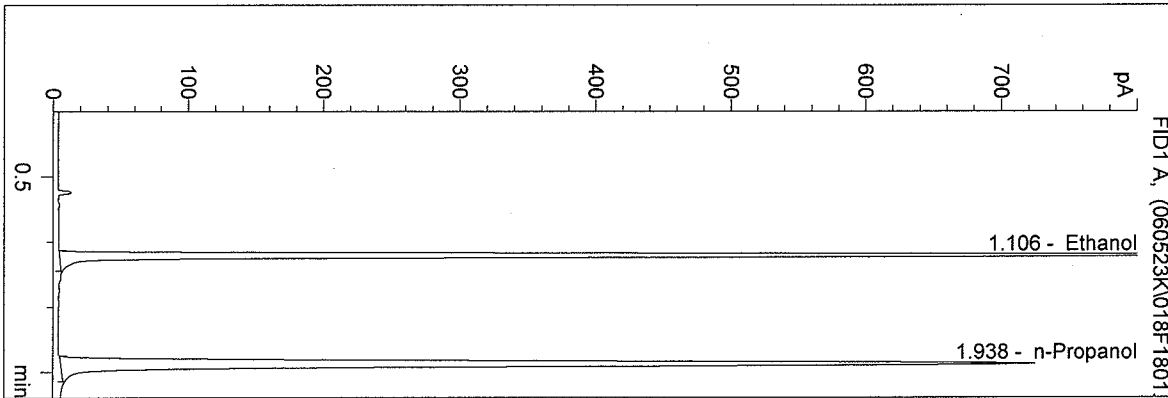


#	Compound	Area	RT
1	Ethanol	1857	1.106
2	n-Propanol	2103	1.938

Totals:

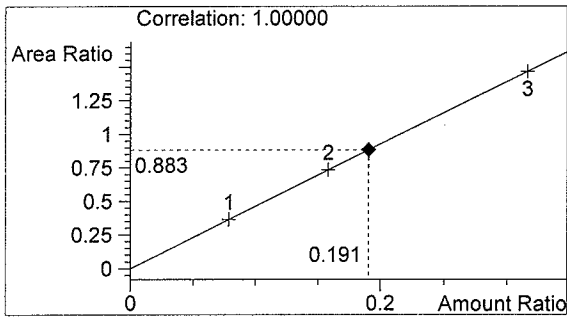

Ethanol 0.191 g/100ml

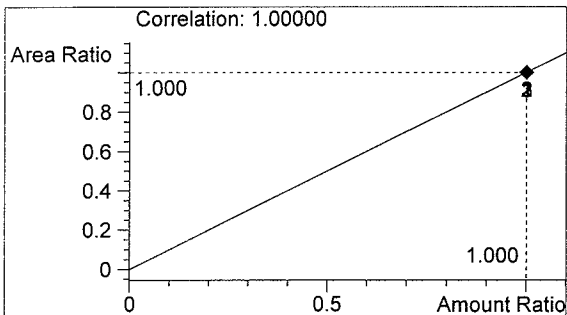


n-Propanol 1.000 g/100ml



D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:35:02 AM  
 Instrument 5  
 DB-ALC2


06024qa  
 kgross

vial # 19

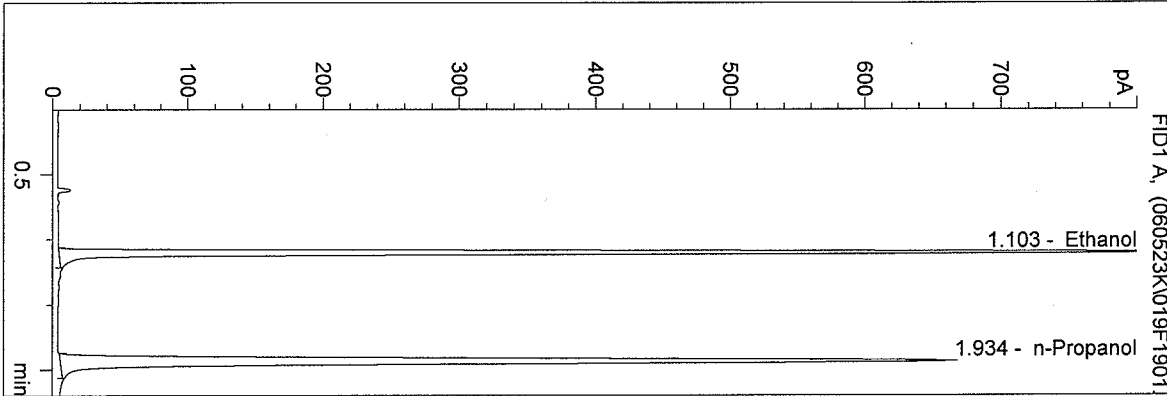


#	Compound	Area	RT
1	Ethanol	1677	1.103
2	n-Propanol	1940	1.934

Totals:

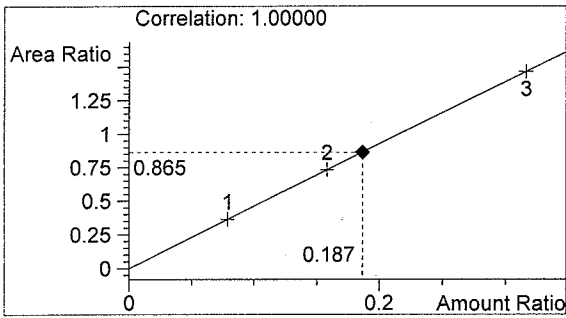

Ethanol 0.187 g/100ml

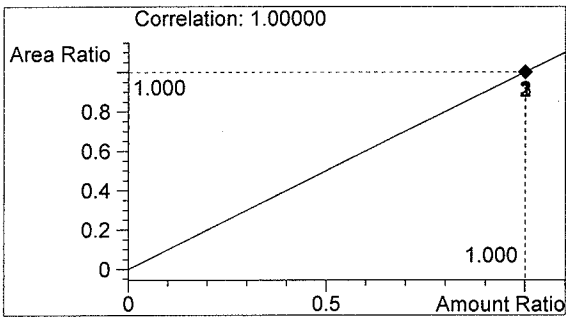


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:38:17 AM  
 Instrument 5  
 DB-ALC2


06024qa  
 kgross

vial # 20

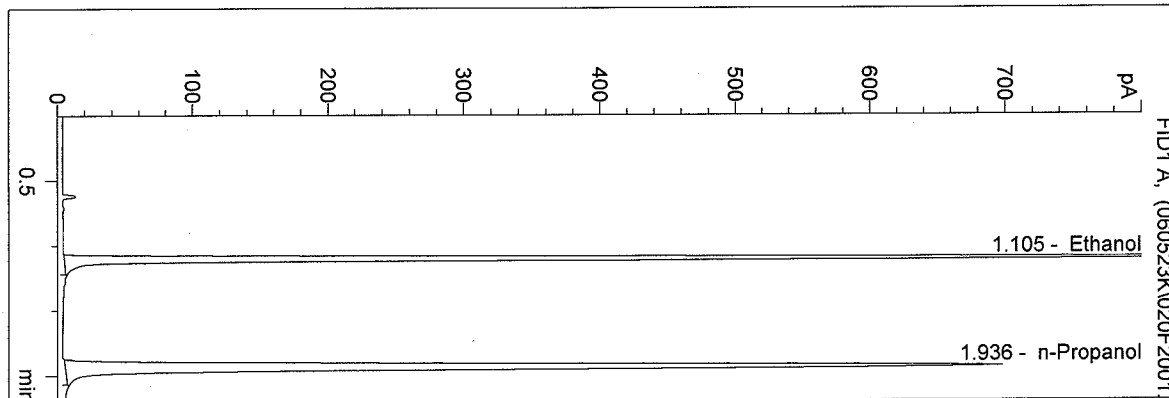


#	Compound	Area	RT
1	Ethanol	1760	1.105
2	n-Propanol	2029	1.936

Totals:



Ethanol 0.187 g/100ml

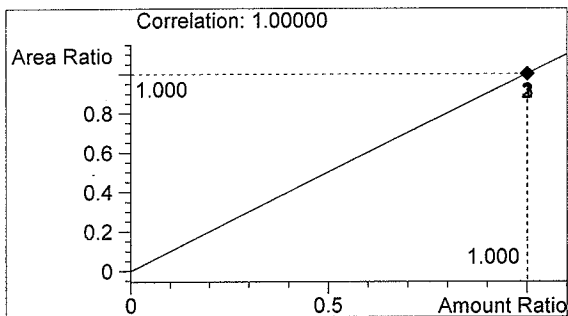


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 8:41:31 AM  
 Instrument 5  
 DB-ALC2


06024qa  
 kgross

vial # 21

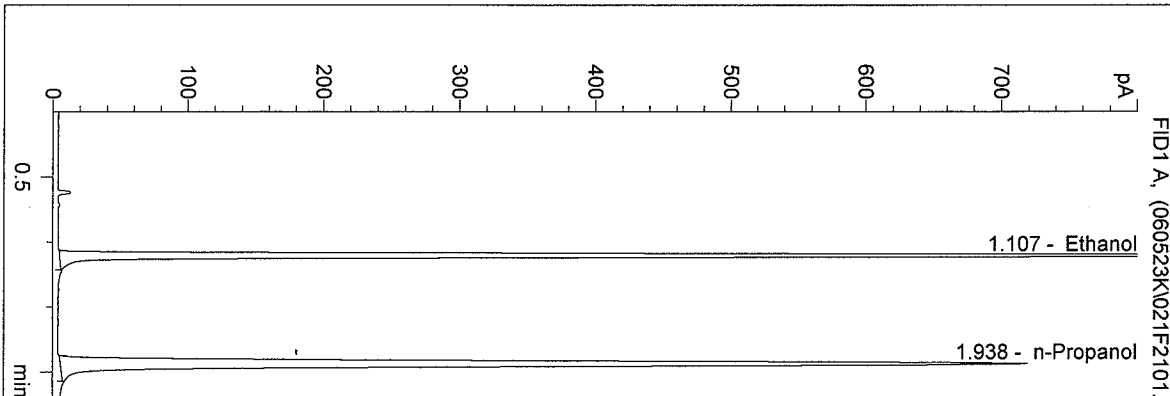


#	Compound	Area	RT
1	Ethanol	1830	1.107
2	n-Propanol	2091	1.938

Totals:

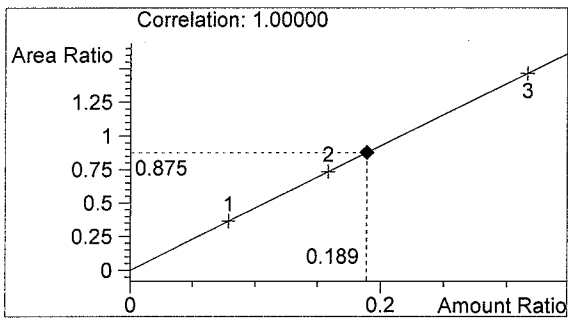

Ethanol 0.189 g/100ml

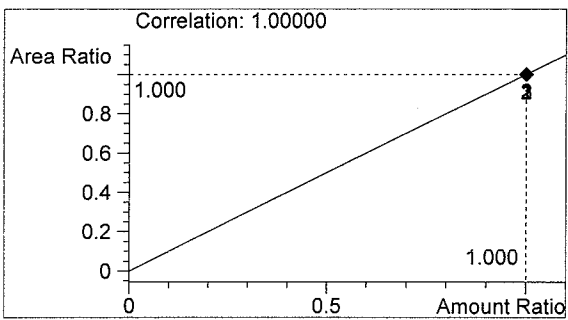

n-Propanol 1.000 g/100ml

## Sequence Parameters:

Operator: kgross  
 Data File Naming: Auto  
 Data Directory: D:\HPCHEM\1\DATA\  
 Data Subdirectory: 060523K  
 Part of Methods to run: According to Runtime Checklist  
 Barcode Reader: not used  
 Shutdown Cmd/Macro: none  
 Sequence Comment:

## Sequence Table (Front Injector):

## Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
====	=====	=====	=====	===	=====	=====	=====
1	Vial 1	0.10 CTL-KDG	BLDALCO2	1	Ctrl Samp		
2	Vial 2	BLANK	BLDALCO2	1	Sample		
3	Vial 3	06022qa	BLDALCO2	1	Sample		
4	Vial 4	06022qa	BLDALCO2	1	Sample		
5	Vial 5	06022qa	BLDALCO2	1	Sample		
6	Vial 6	06022qa	BLDALCO2	1	Sample		
7	Vial 7	06022qa	BLDALCO2	1	Sample		
8	Vial 8	0.10 CTL-KDG	BLDALCO2	1	Ctrl Samp		
9	Vial 9	BLANK	BLDALCO2	1	Sample		
10	Vial 10	06023qa	BLDALCO2	1	Ctrl Samp		
11	Vial 11	06023qa	BLDALCO2	1	Sample		
12	Vial 12	06023qa	BLDALCO2	1	Sample		
13	Vial 13	06023qa	BLDALCO2	1	Sample		
14	Vial 14	06023qa	BLDALCO2	1	Sample		
15	Vial 15	0.10 CTL-KDG	BLDALCO2	1	Ctrl Samp		
16	Vial 16	blank	BLDALCO2	1	Sample		
17	Vial 17	06024qa	BLDALCO2	1	Sample		
18	Vial 18	06024qa	BLDALCO2	1	Sample		
19	Vial 19	06024qa	BLDALCO2	1	Sample		
20	Vial 20	06024qa	BLDALCO2	1	Sample		
21	Vial 21	06024qa	BLDALCO2	1	Sample		

## Sequence Table (Back Injector):

No entries - empty table!

Sequence Parameters:

Operator: kgross  
Data File Naming: Auto  
Data Directory: D:\HPCHEM\1\DATA\  
Data Subdirectory: 060523K  
Part of Methods to run: According to Runtime Checklist  
Barcode Reader: not used  
Shutdown Cmd/Macro: none  
Sequence Comment:

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	0.10 CTL KDG	BLDALCO	1	Ctrl Samp		
2	Vial 2	BLANK	BLDALCO	1	Sample		
3	Vial 3	06020sim	BLDALCO	1	Sample		
4	Vial 4	06020sim	BLDALCO	1	Sample		
5	Vial 5	06020sim	BLDALCO	1	Sample		
6	Vial 6	06020sim	BLDALCO	1	Sample		
7	Vial 7	06020sim	BLDALCO	1	Sample		
8	Vial 8	0.10 CTL KDG	BLDALCO	1	Ctrl Samp		
9	Vial 9	BLANK	BLDALCO	1	Sample		
10	Vial 10	06021qa	BLDALCO	1	Sample		
11	Vial 11	06021qa	BLDALCO	1	Sample		
12	Vial 12	06021qa	BLDALCO	1	Sample		
13	Vial 13	06021qa	BLDALCO	1	Sample		
14	Vial 14	06021qa	BLDALCO	1	Sample		


Sequence Table (Back Injector):

No entries - empty table!

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:05:43 PM  
 Instrument 5  
 DB-ALC2


06024-a QA  
 Brianne E. Akins

vial # 6

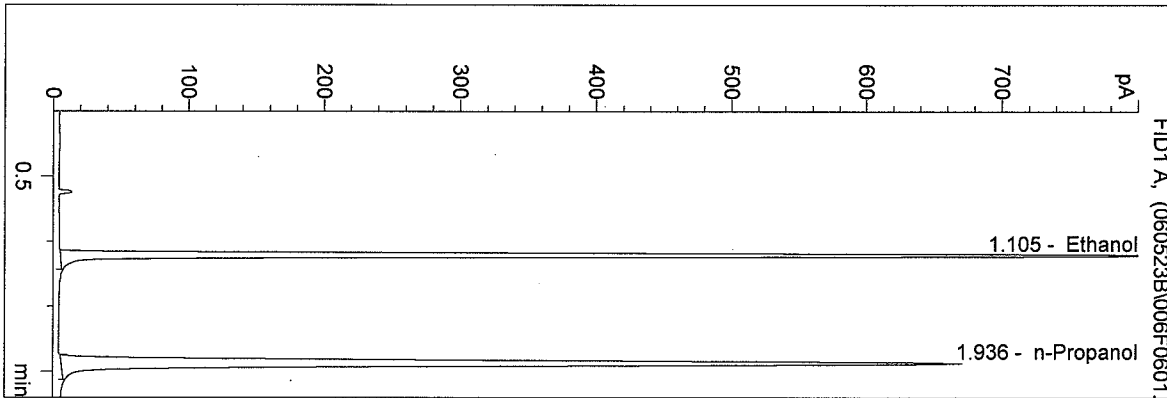


#	Compound	Area	RT
1	Ethanol	1682	1.105
2	n-Propanol	1941	1.936

Totals:

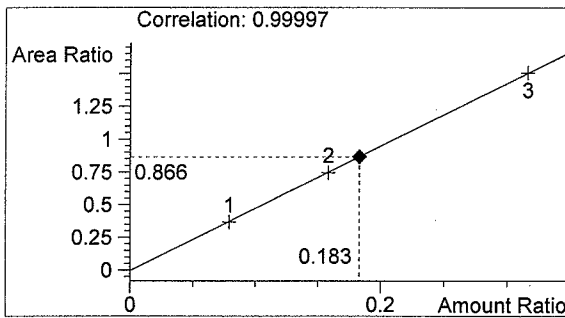

Ethanol 0.183 g/100ml

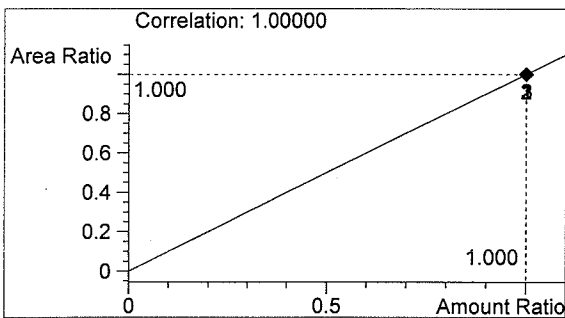


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:11:10 PM  
 Instrument 5  
 DB-ALC2


06024-b QA  
 Brianne E. Akins

vial # 7

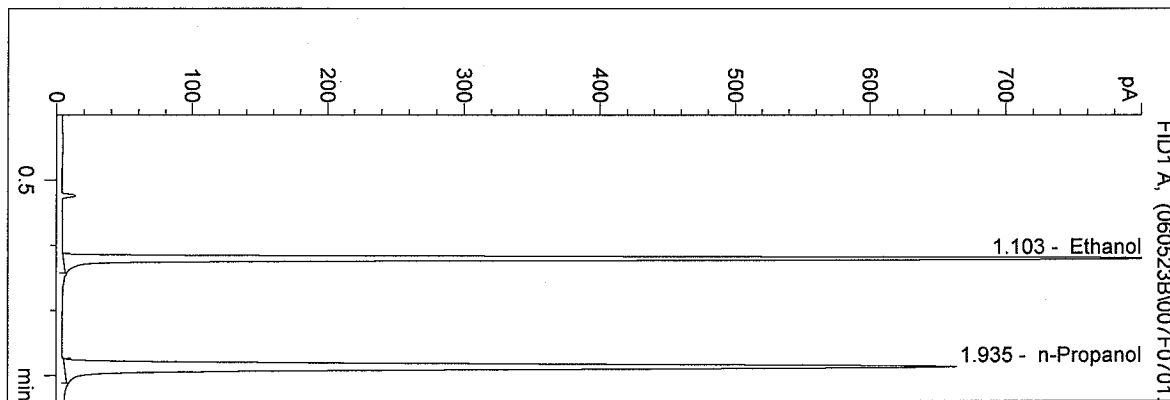


#	Compound	Area	RT
1	Ethanol	1675	1.103
2	n-Propanol	1924	1.935

Totals:

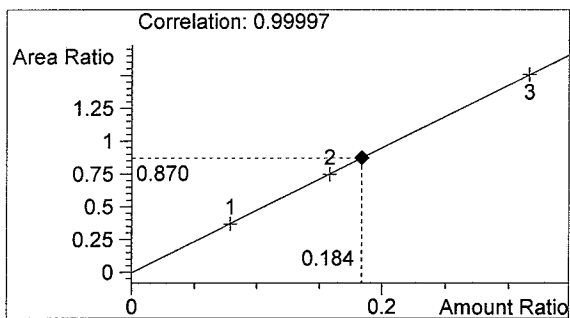

Ethanol 0.184 g/100ml

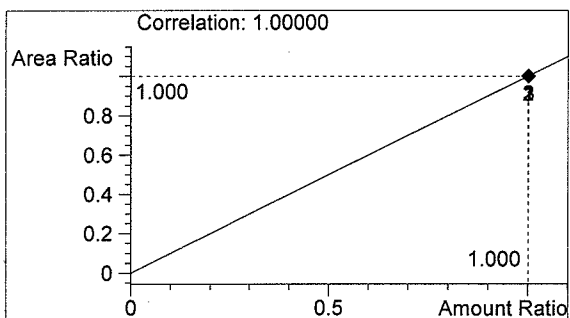


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:14:22 PM  
 Instrument 5  
 DB-ALC2


06024-c QA  
 Brianne E. Akins

vial # 8

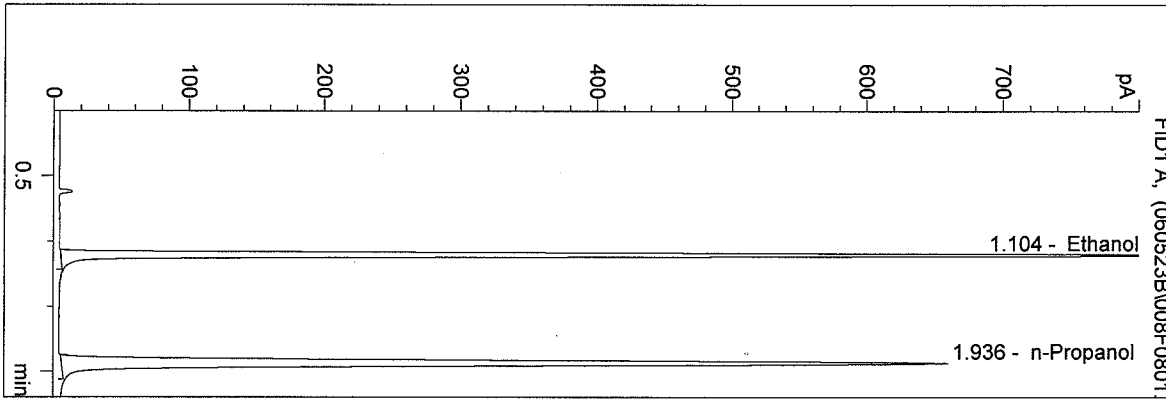


#	Compound	Area	RT
1	Ethanol	1666	1.104
2	n-Propanol	1908	1.936

Totals:



Ethanol 0.184 g/100ml




n-Propanol 1.000 g/100ml



D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:17:36 PM  
 Instrument 5  
 DB-ALC2


06024-d QA  
 Brianne E. Akins

vial # 9

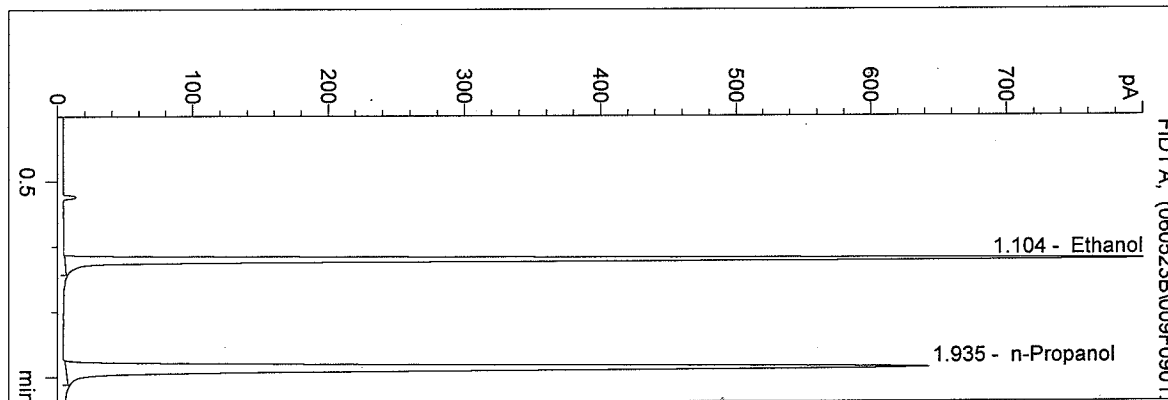


#	Compound	Area	RT
1	Ethanol	1624	1.104
2	n-Propanol	1860	1.935

Totals:



Ethanol 0.184 g/100ml




n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:20:51 PM  
 Instrument 5  
 DB-ALC2


06024-eQA  
 Brianne E. Akins

vial # 10

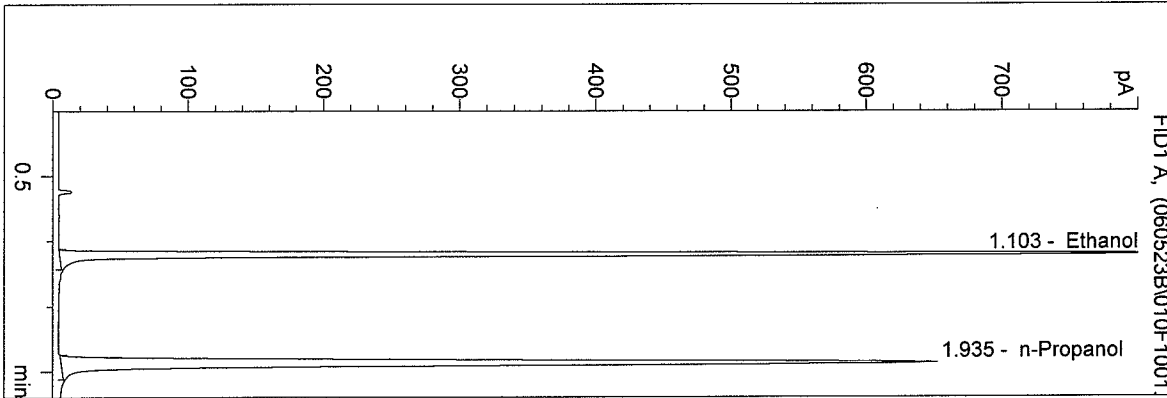


#	Compound	Area	RT
1	Ethanol	1643	1.103
2	n-Propanol	1885	1.935

Totals:



Ethanol 0.184 g/100ml




n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:24:04 PM  
 Instrument 5  
 DB-ALC2


0.10 CONTROL-ba  
 Brianne E. Akins

vial # 11

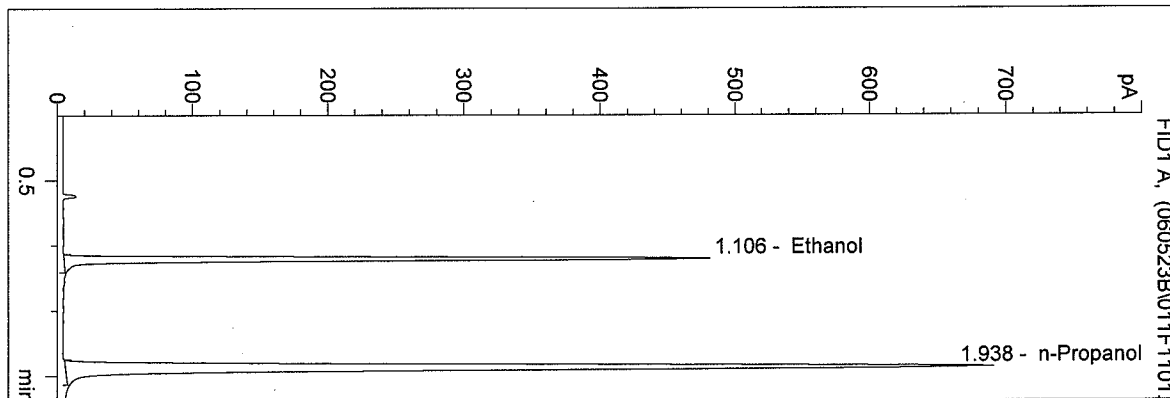


#	Compound	Area	RT
1	Ethanol	958	1.106
2	n-Propanol	2004	1.938

Totals:

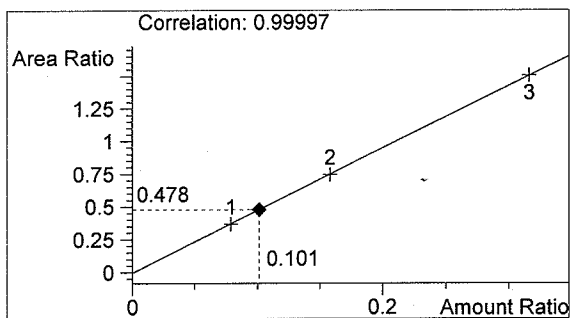


Ethanol 0.101 g/100ml

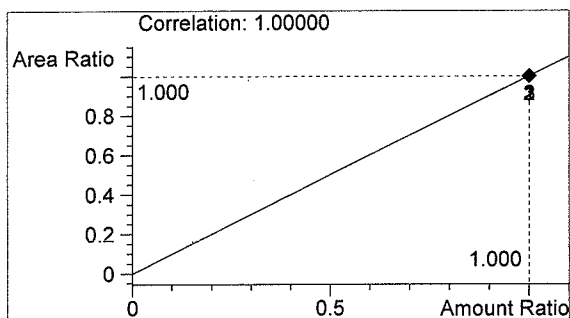

n-Propanol 1.000 g/100ml


D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:27:15 PM  
 Instrument 5  
 DB-ALC2

blank  
 Brianne E. Akins  
 vial # 12

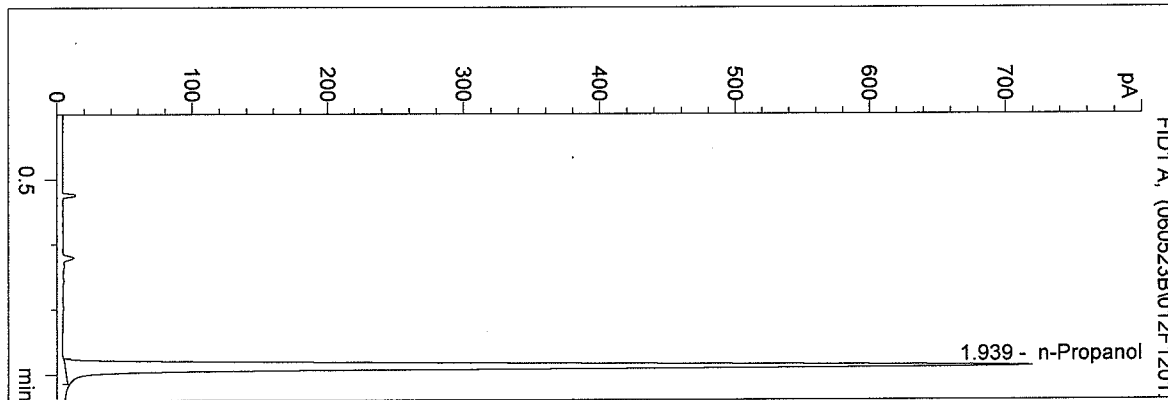


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	2095	1.939

Totals:



Ethanol 0.000 g/100ml




n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 2:49:35 PM  
 Instrument 5  
 DB-ALC2


BLANK  
 Brianne E. Akins

vial # 1

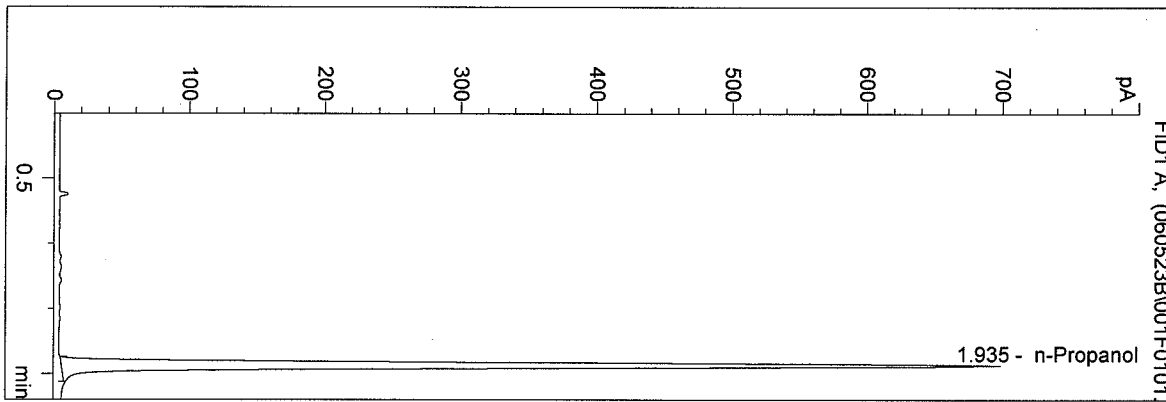


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	2017	1.935

Totals:

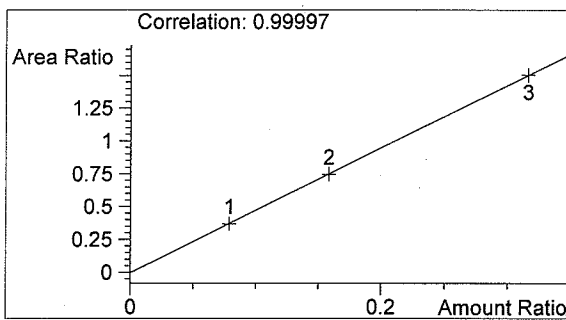

Ethanol 0.000 g/100ml

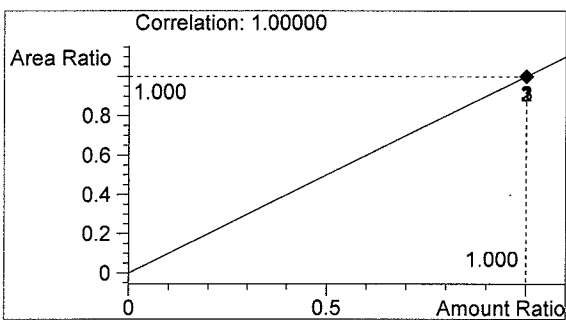


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/23/2006 2:49:02 PM  
 Instrument 4  
 DB-ALC1


BLANK  
 Brianne E. Akins

vial # 1

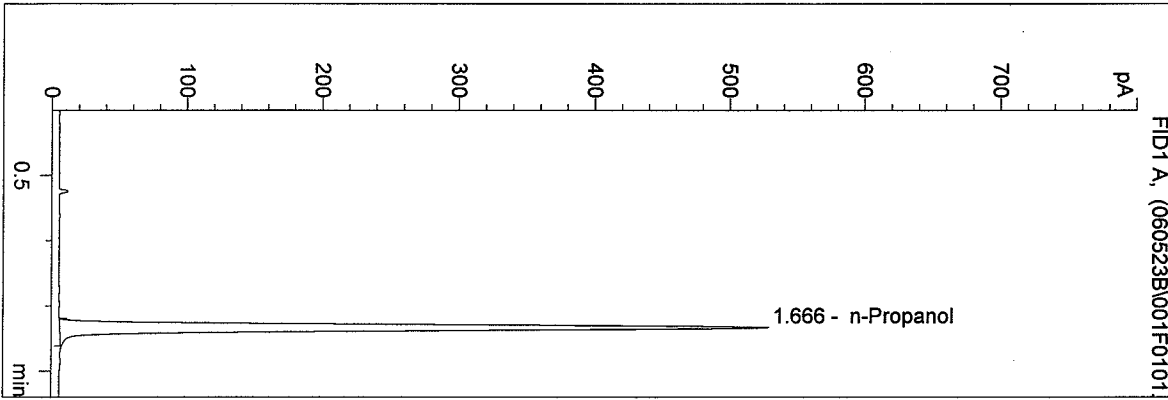


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1650	1.666

Totals:



Ethanol 0.000 g/100ml



n-Propanol 1.000 g/100ml

Sequence Parameters:

Operator: Brianne E. Akins  
 Data File Naming: Auto  
 Data Directory: D:\HPCHEM\1\DATA\  
 Data Subdirectory: 060523B  
 Part of Methods to run: According to Runtime Checklist  
 Barcode Reader: not used  
 Shutdown Cmd/Macro: none  
 Sequence Comment:

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	BLDALCO2	1	Sample		
2	Vial 2	0603669 realiquo	BLDALCO2	1	Sample		
3	Vial 3	0603668 realiquo	BLDALCO2	1	Sample		
4	Vial 4	blank	BLDALCO2	1	Sample		
5	Vial 5	blank	BLDALCO2	1	Sample		
6	Vial 6	06024-a QA	BLDALCO2	1	Sample		
7	Vial 7	06024-b QA	BLDALCO2	1	Sample		
8	Vial 8	06024-c QA	BLDALCO2	1	Sample		
9	Vial 9	06024-d QA	BLDALCO2	1	Sample		
10	Vial 10	06024-eQA	BLDALCO2	1	Sample		
11	Vial 11	0.10 CONTROL-ba	BLDALCO2	1	Ctrl Samp		
12	Vial 12	blank	BLDALCO2	1	Sample		

Sequence Table (Back Injector):

No entries - empty table!

Sequence Parameters:

Operator: Brianne E. Akins  
Data File Naming: Auto  
Data Directory: D:\HPCHEM\1\DATA\  
Data Subdirectory: 060523B  
Part of Methods to run: According to Runtime Checklist  
Barcode Reader: not used  
Shutdown Cmd/Macro: none  
Sequence Comment:

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	BLDALCO	1	Sample		
2	Vial 2	0603669 realiquo	BLDALCO	1	Sample		
3	Vial 3	0603668 realiquo	BLDALCO	1	Sample		
4	Vial 4	blank	BLDALCO	1	Sample		
5	Vial 5	blank	BLDALCO	1	Sample		
6	Vial 6	06023-a QA	BLDALCO	1	Sample		
7	Vial 7	06023-b QA	BLDALCO	1	Sample		
8	Vial 8	06023-c QA	BLDALCO	1	Sample		
9	Vial 9	06023-d QA	BLDALCO	1	Sample		
10	Vial 10	06023-e QA	BLDALCO	1	Sample		
11	Vial 11	0.10 CONTROL-ba	BLDALCO	1	Ctrl Samp		
12	Vial 12	blank	BLDALCO	1	Sample		

Sequence Table (Back Injector):


No entries - empty table!



D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/23/2006 3:02:02 PM  
 Instrument 4  
 DB-ALC1


blank  
 Brianne E. Akins

vial # 5

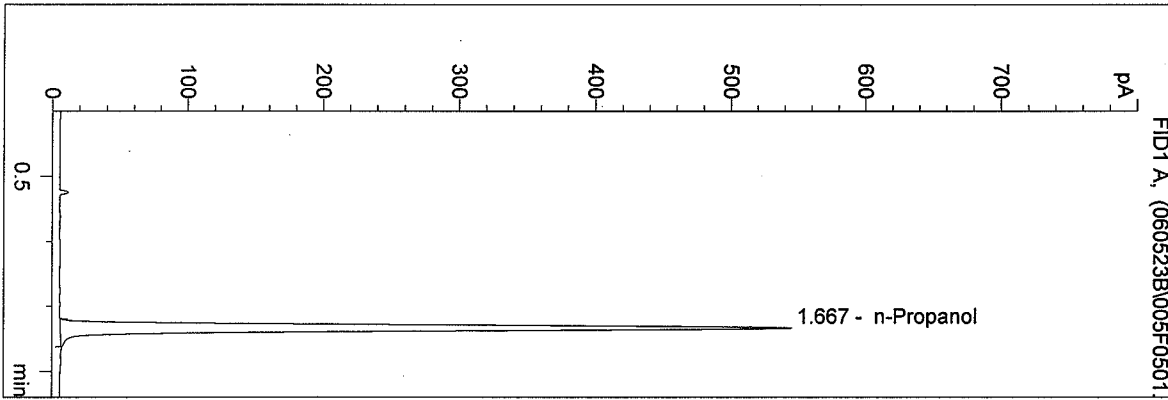


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1702	1.667

Totals:

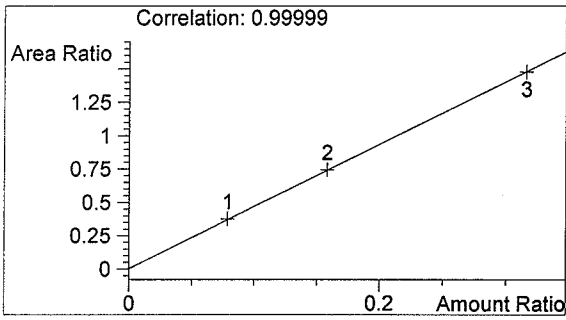

Ethanol 0.000 g/100ml

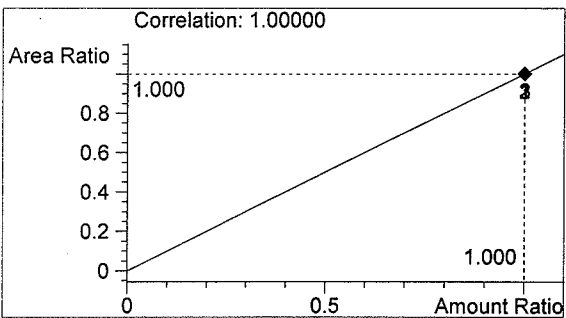


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M  
 5/23/2006 3:02:24 PM  
 Instrument 5  
 DB-ALC2


blank  
 Brianne E. Akins

vial # 5

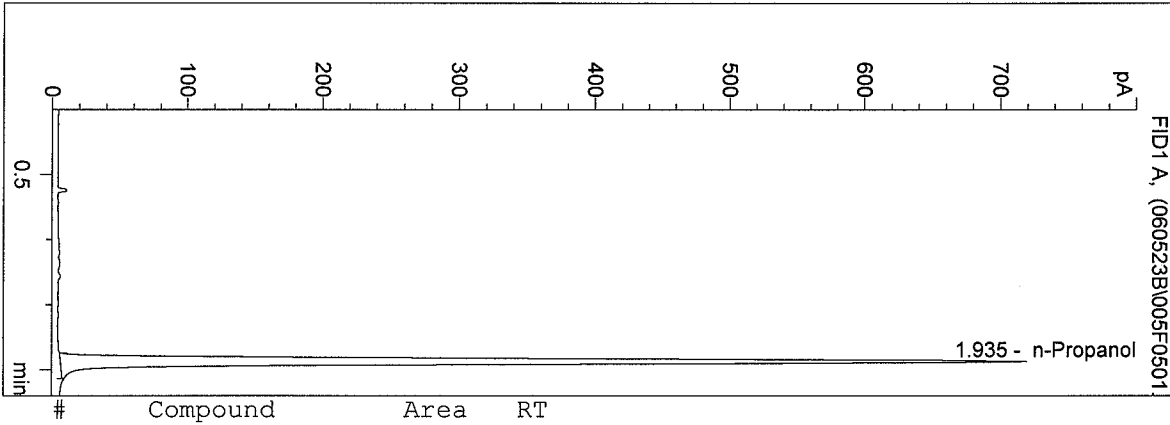


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	2079	1.935

Totals:

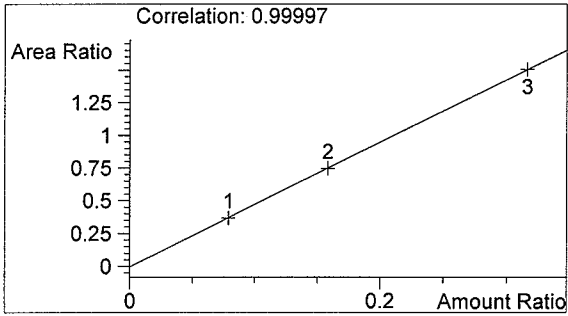

Ethanol 0.000 g/100ml

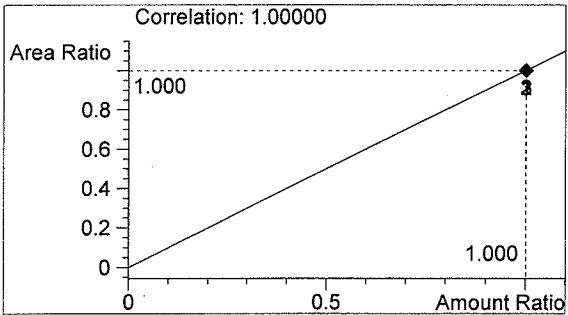


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/19/2006 1:50:19 PM  
 Instrument 4  
 DB-ALC1


BLANK  
 SIMULATOR SOLUTION

vial # 1

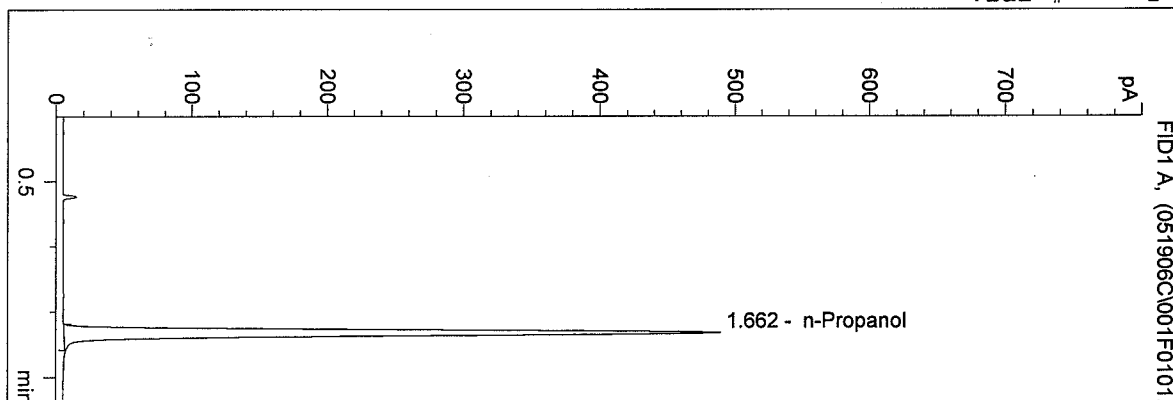


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1522	1.662

Totals:



Ethanol 0.000 g/100ml




n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/19/2006 1:53:34 PM  
 Instrument 4  
 DB-ALC1


0.079 CAL  
 SIMULATOR SOLUTION

vial # 2

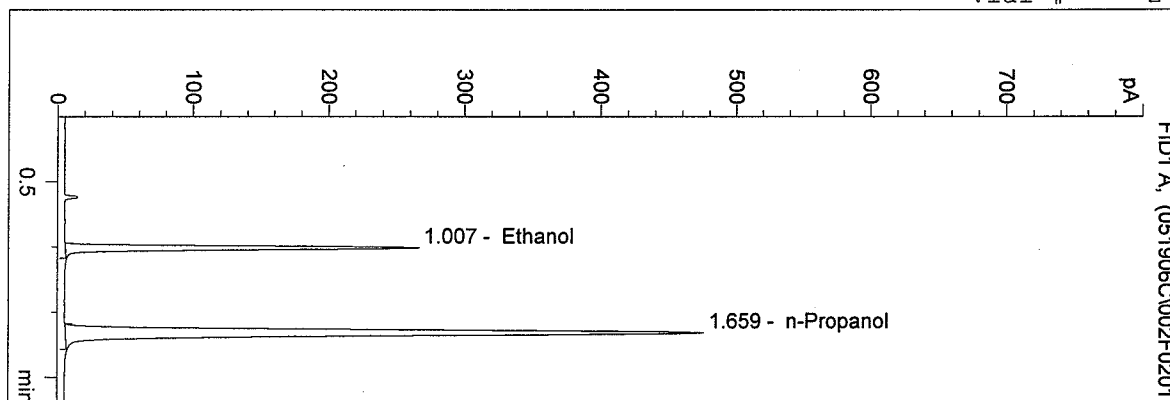


#	Compound	Area	RT
1	Ethanol	531	1.007
2	n-Propanol	1481	1.659

Totals:

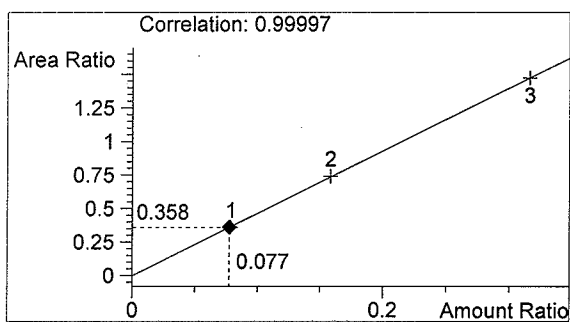

Ethanol 0.077 g/100ml

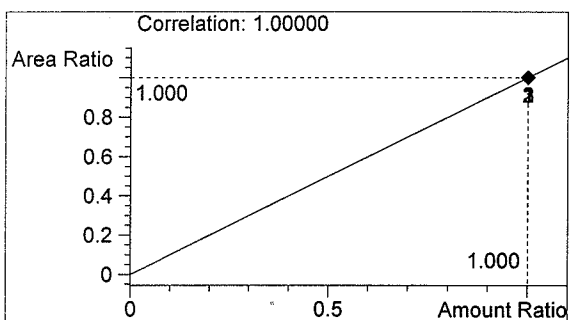


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/19/2006 1:56:48 PM  
 Instrument 4  
 DB-ALC1


0.158 CAL  
 SIMULATOR SOLUTION

vial # 3

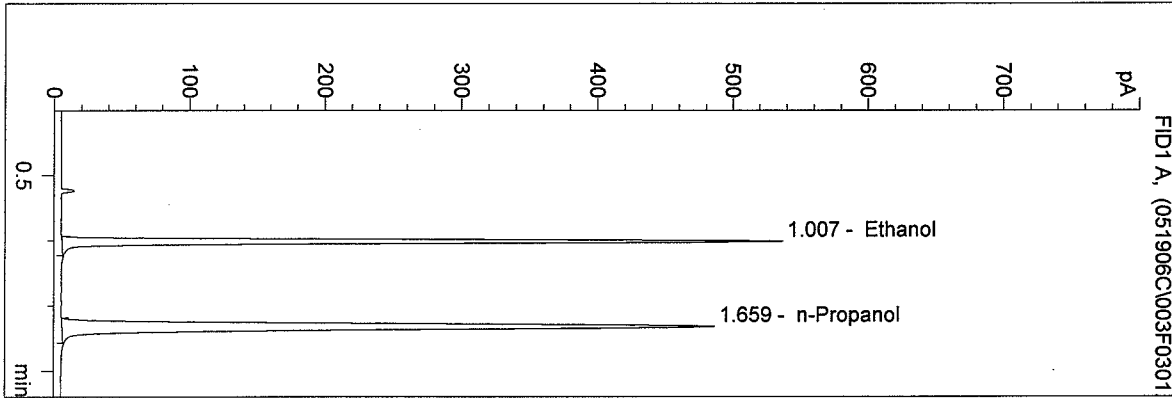


#	Compound	Area	RT
1	Ethanol	1087	1.007
2	n-Propanol	1514	1.659

Totals:

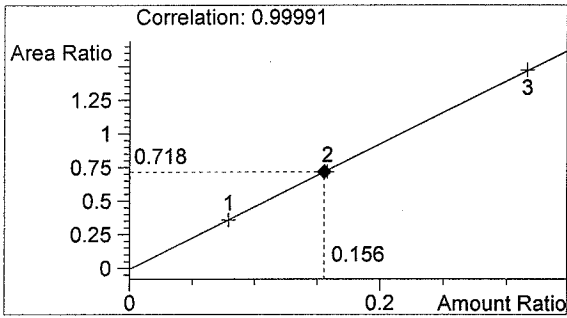

Ethanol 0.156 g/100ml

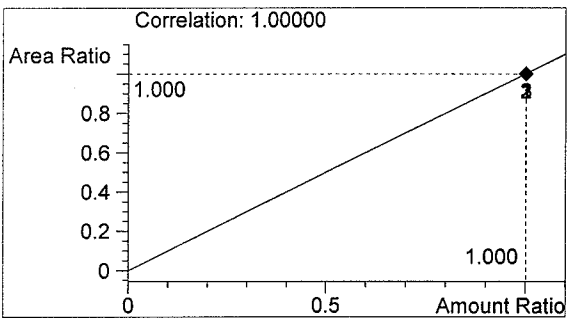


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/19/2006 1:59:59 PM  
 Instrument 4  
 DB-ALC1


0.316 CAL  
 SIMULATOR SOLUTION

vial # 4

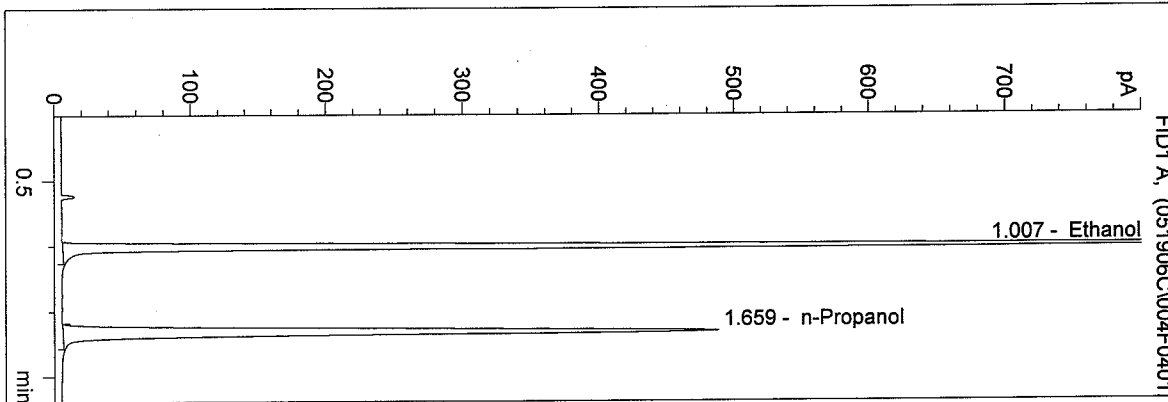


#	Compound	Area	RT
1	Ethanol	2179	1.007
2	n-Propanol	1520	1.659

Totals:



Ethanol 0.316 g/100ml




n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M  
 5/19/2006 2:03:10 PM  
 Instrument 4  
 DB-ALC1


BLANK  
 SIMULATOR SOLUTION

vial # 5

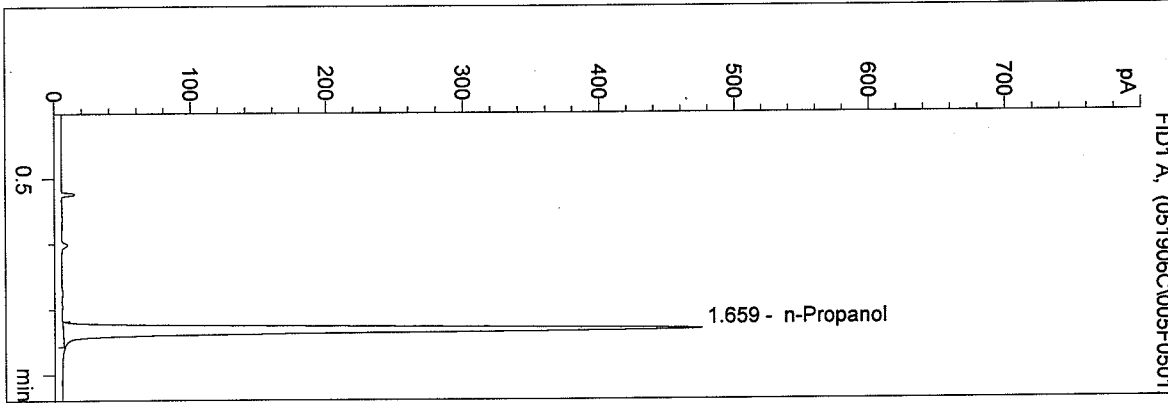


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1480	1.659

Totals:

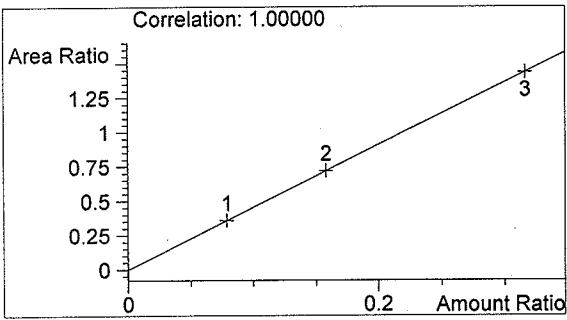

Ethanol 0.000 g/100ml

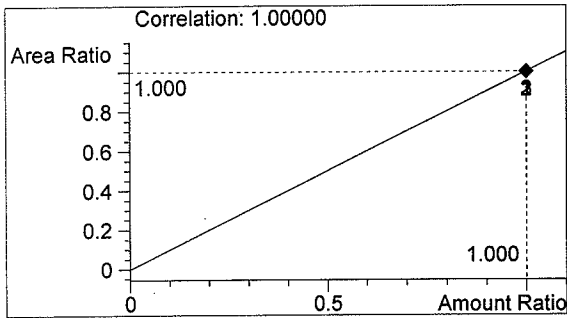

n-Propanol 1.000 g/100ml