


Notice of Simulator Solution File Review

At the request of the State Toxicologist a review of the following simulator solution records has been accomplished. The following file consists of simulator solution analyses performed and completed by the State Toxicology Laboratory for a specific batch number. The file contains the simulator solution data entry form along with a file review record and the chromatograms generated by the Toxicology Laboratory during the analyses of the solutions. This file has been reviewed by Tpr. Ken Denton and Mr. Rod Gullberg for accuracy and completeness. Where computations regarding simulator solution values have been found to be incorrect, the corrected values have been written in by Mr. Rod Gullberg along with initials and date. The corrected values were then evaluated to ensure that the solution still conformed to those standards established by the State Toxicologist.


Where computation values changed for a specific batch number, the analysts employed by the State Toxicology Laboratory were asked to review the revisions, ensure the solution complied with the criteria established by the State Toxicologist and then re-sign their affidavit. Their signature will appear on their original affidavit along with a statement regarding their review of the results.

Where a dating error occurred that analyst will have made the correction on the original data form including their initials and date and then re-signed their original affidavit.

 _____ 10/10/2007

Tpr. Ken Denton

Date

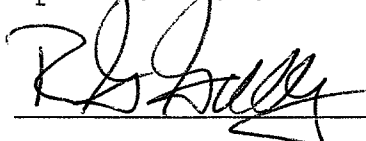 _____ 10-10-07

Rod G. Gullberg

Date

Washington State Toxicology Laboratory

Simulator Solution Data Entry Review Form

Reviewer KEN DENTON / RON GULLBERG Date 10-1-07
Location TOX LAB SEATTLE Batch Number 06050

Form Review Criteria

Preparation date precedes all analysis dates: Okay Not Okay ___
Data entry corresponds to all chromatograms: Okay Not Okay ___
All signatures present: Okay Not Okay ___


Computations:

Avg. solution concentration: Correct Not Correct ___
Standard deviation: Correct Not Correct ___
Range: Correct Not Correct ___
Precision: Correct Not Correct ___
Equivalent vapor concent.: Correct Not Correct ___
External Control Information
(lot # and future date): Correct Not Correct ___

Complies with accuracy and precision requirements established by the
State Toxicologist: Yes No ___

Corrections Necessary:

Comments:

Reviewer Signature:  Date: 10-1-07
Reviewer Signature:  Date: 10/1/2007

WASHINGTON STATE TOXICOLOGY LABORATORY
 FORENSIC LABORATORY SERVICES BUREAU
 WASHINGTON STATE PATROL
 2203 AIRPORT WAY S, SUITE 360
 SEATTLE, WASHINGTON 98134-2027
 (206) 262-6100 FAX (206) 262-6145

Preparation and certification of **0.04** g/210L Quality Assurance solution
 Batch number **06050** Date: 12/14/2006
 Preparation: 11.1 mL of absolute ethyl alcohol diluted to 18 Liters with water
 Concentration of ethanol (g/100mL) measured by gas chromatography:

	Anal 1	Anal 2	Anal 3	Anal 4	Anal 5	Anal 6	Anal 7	Anal 8	Anal 9	Anal 10	Anal 11	Anal 12	Anal 13	Anal 14	Anal 15	Anal 16
1	0.049	0.049	0.049													
2	0.049	0.048	0.048													
3	0.049	0.049	0.048													
4	0.049	0.048	0.048													
5	0.049	0.048	0.048													
Ctrl	0.099	0.098	0.099													

External Control:

Lot #: A041837 Exp date: 4/2010

Target concentration: 0.10 g/100mL

Statistics:




Avg. solution concent.: 0.0485 g/100 mL

SD: 0.00052

Range (3xSD): 0.0470 to 0.0500

Precision CV (%): 1.0647 %

Equivalent vapor concent.: 0.0394 g/210L

Analyst	Name	Signature	Date
1	Naziha Nuwayhid, PhD		12/19/2006
2	Justin L Kroy		12/19/2006
3	Brian Capron		12/21/2006
4			
5			
6			
7			
8			
9			
10			
11			
12			
13			
14			
15			
16			

Prepared by: Naziha Nuwayhid, PhD according to the approved protocol

CHRISTINE O. GREGOIRE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2927 • (206) 262-6100 • FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION
CERTIFICATION


I, Naziha Nuwayhid, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: Bachelor and Masters degrees in Biology, Ph.D. degree in Basic Medical Science, ten years experience in clinical laboratory sciences, one year in clinical toxicology and six years in forensic toxicology. I am also board certified by the American Board of Clinical Chemistry.

The quality assurance solution, Lot Number 06050, was prepared in the Washington State Toxicology Laboratory on 12/14/2006. I examined and tested this solution. The mean concentration of the alcohol was 0.0485 grams per 100ml.


Dated: 01/08/2007
Seattle, WA


Naziha Nuwayhid, Ph.D.
Forensic Toxicologist

NN/km
NNQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.

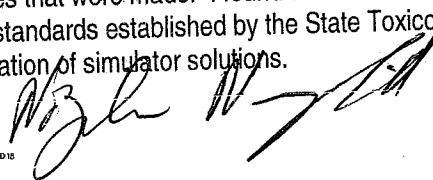

 10/9/07



CHRISTINE O. GREGOIRE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY
2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2927 • (206) 262-6100 • FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION
CERTIFICATION


I, Justin L. Knoy, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: BS degree in Biology, and MS degree in Forensic Science.


The quality assurance solution, Lot Number 06050, was prepared in the Washington State Toxicology Laboratory on 12/14/2006. I examined and tested this solution. The mean concentration of the alcohol was 0.0485 grams per 100ml.

Dated: 01/08/2007
Seattle, WA

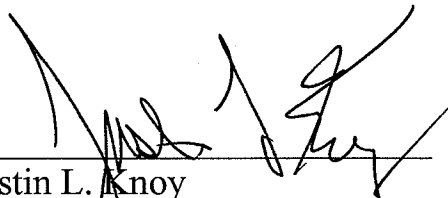
Justin L. Knoy
Forensic Toxicologist

JLK/km
JKQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.

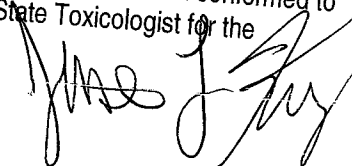 10/5/07



CHRISTINE O. GREGOIRE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2927 • (206) 262-6100 • FAX (206) 262-6145

DATAMASTER QUALITY ASSURANCE SOLUTION
CERTIFICATION


I, Brian Capron, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and a part of my responsibilities includes preparing and testing the alcohol solutions for the DataMaster breath test instrument.

I possess the following qualifications: BS degree in Biology and nine years of experience in forensic toxicology.

The quality assurance solution, Lot Number 06050, was prepared in the Washington State Toxicology Laboratory on 12/14/2006. I examined and tested this solution. The mean concentration of the alcohol was 0.0485 grams per 100ml.

Dated: 01/08/07
Seattle, WA


Brian Capron
Forensic Toxicologist

BC/km
BCQA

A review of solution batch records was recently completed. After this review, I checked the file for this solution and reviewed all changes that were made. I found that the solution still conformed to those standards established by the State Toxicologist for the certification of simulator solutions.

 10.9.07

Sequence Parameters:

Operator: N Nuwayhid, PhD
 Data File Naming: Auto
 Data Directory: D:\HPCHEM\1\DATA\
 Data Subdirectory: 061219NN
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none
 Sequence Comment:

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	BLDALCO2	1	Sample		
2	Vial 2	0.079 CALIBRATOR	BLDALCO2	1	Calib		
3	Vial 3	0.158 CALIBRATOR	BLDALCO2	1	Calib		
4	Vial 4	0.316 CALIBRATOR	BLDALCO2	1	Calib		
5	Vial 5	BLANK	BLDALCO2	1	Sample		
6	Vial 6	0.100 CTL	BLDALCO2	1	Ctrl Samp		
7	Vial 7	06050 QA-1	BLDALCO2	1	Sample		
8	Vial 8	06050 QA-2	BLDALCO2	1	Sample		
9	Vial 9	06050 QA-3	BLDALCO2	1	Sample		
10	Vial 10	06050 QA-4	BLDALCO2	1	Sample		
11	Vial 11	06050 QA-5	BLDALCO2	1	Sample		
12	Vial 12	0.100 CTL	BLDALCO2	1	Ctrl Samp		
13	Vial 13	BLANK	BLDALCO2	1	Sample		
14	Vial 14	06051 QA-1	BLDALCO2	1	Sample		
15	Vial 15	06051 QA-2	BLDALCO2	1	Sample		
16	Vial 16	06051 QA-3	BLDALCO2	1	Sample		
17	Vial 17	06051 QA-4	BLDALCO2	1	Sample		
18	Vial 18	06051 QA-5	BLDALCO2	1	Sample		
19	Vial 19	0.100 CTL	BLDALCO2	1	Ctrl Samp		
20	Vial 20	BLANK	BLDALCO2	1	Sample		
21	Vial 21	06052 QA-1	BLDALCO2	1	Sample		
22	Vial 22	06052 QA-2	BLDALCO2	1	Sample		
23	Vial 23	06052 QA-3	BLDALCO2	1	Sample		
24	Vial 24	06052 QA-4	BLDALCO2	1	Sample		
25	Vial 25	06052 QA-5	BLDALCO2	1	Sample		
26	Vial 26	0.100 CTL	BLDALCO2	1	Ctrl Samp		
27	Vial 27	BLANK	BLDALCO2	1	Sample		
28	Vial 28	06053 QA-1	BLDALCO2	1	Sample		
29	Vial 29	06053 QA-2	BLDALCO2	1	Sample		
30	Vial 30	06053 QA-3	BLDALCO2	1	Sample		
31	Vial 31	06053 QA-4	BLDALCO2	1	Sample		
32	Vial 32	06053 QA-5	BLDALCO2	1	Sample		
33	Vial 33	0.100 CTL	BLDALCO2	1	Ctrl Samp		
34	Vial 34	BLANK	BLDALCO2	1	Sample		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CALIBRATOR	BLDALCO2	1	Replace		Average		
3	Vial 3	0.158 CALIBRATOR	BLDALCO2	2	Replace		Average		
4	Vial 4	0.316 CALIBRATOR	BLDALCO2	3	Replace		Average		


Sequence Table (Back Injector):

No entries - empty table!

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:18:45 AM
 Instrument 5
 DB-ALC2


BLANK
 N Nuwayhid, PhD

vial # 1

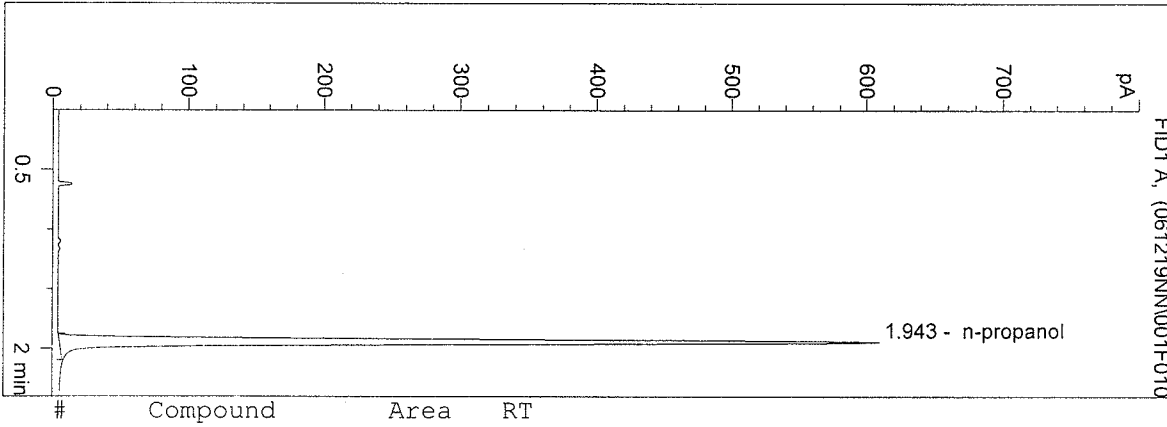


#	Compound	Area	RT
1	ethanol	0	0.000
2	n-propanol	1778	1.943

Totals:

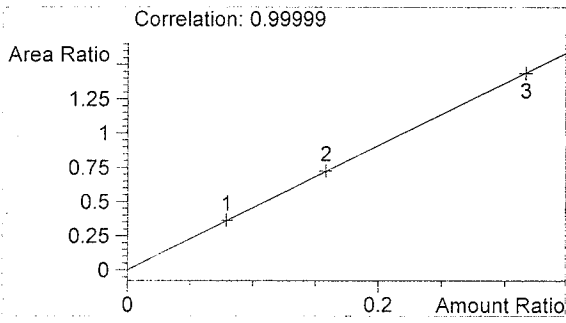

ethanol 0.000 g/100ml

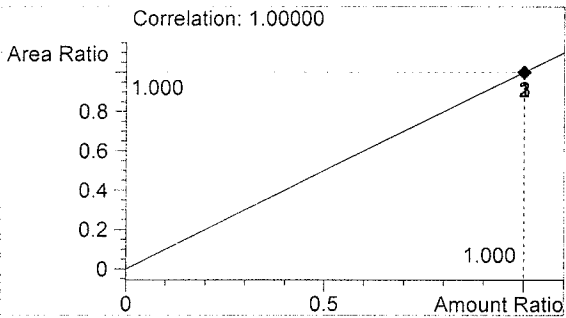


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:22:04 AM
 Instrument 5
 DB-ALC2


0.079 CALIBRATOR
 N Nuwayhid, PhD

vial # 2

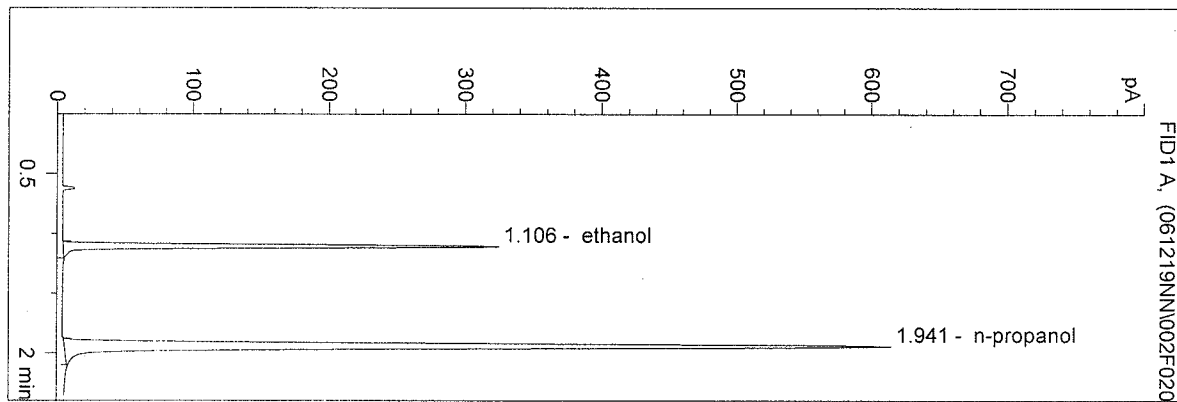


#	Compound	Area	RT
1	ethanol	645	1.106
2	n-propanol	1787	1.941

Totals:

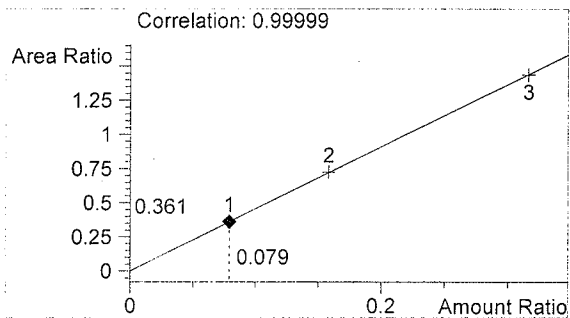

ethanol 0.079 g/100ml

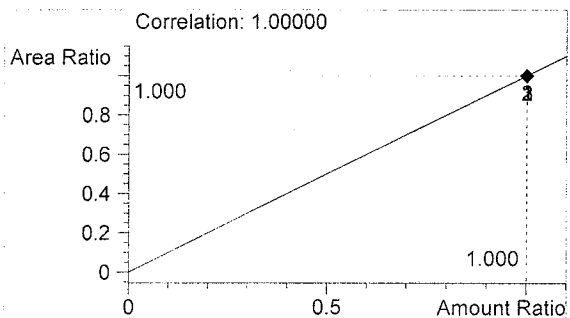


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:25:36 AM
 Instrument 5
 DB-ALC2


0.158 CALIBRATOR
 N Nuwayhid, PhD

vial # 3

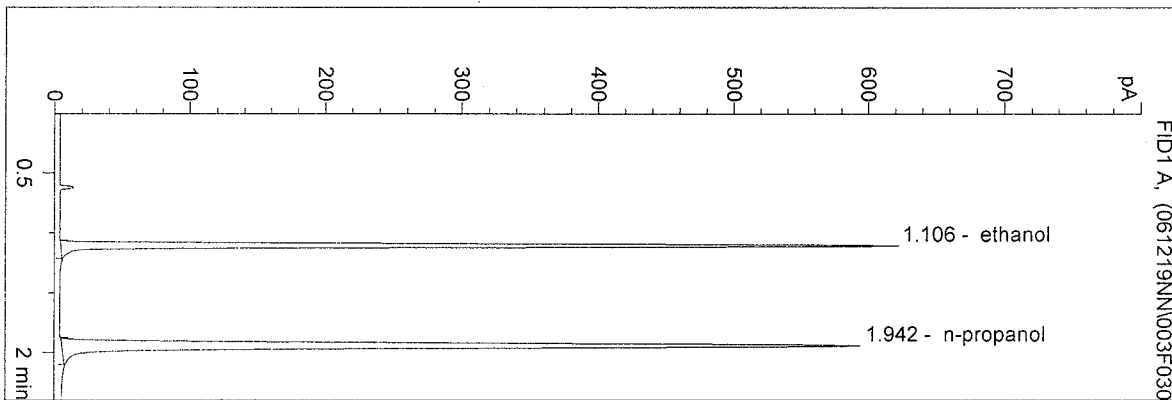


#	Compound	Area	RT
1	ethanol	1272	1.106
2	n-propanol	1736	1.942

Totals:

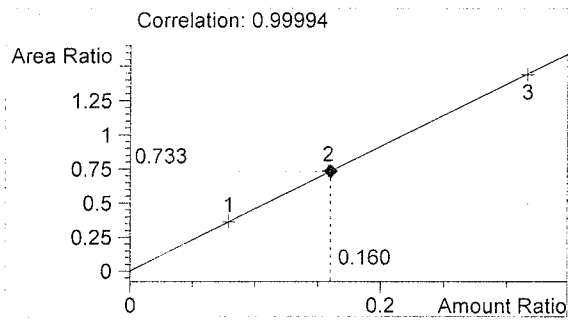

ethanol 0.160 g/100ml

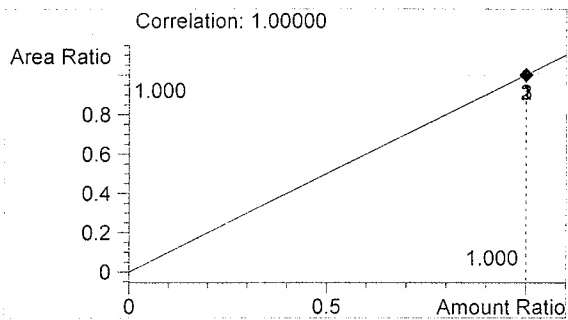


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:30:42 AM
 Instrument 5
 DB-ALC2


0.316 CALIBRATOR
 N Nuwayhid, PhD

vial # 4

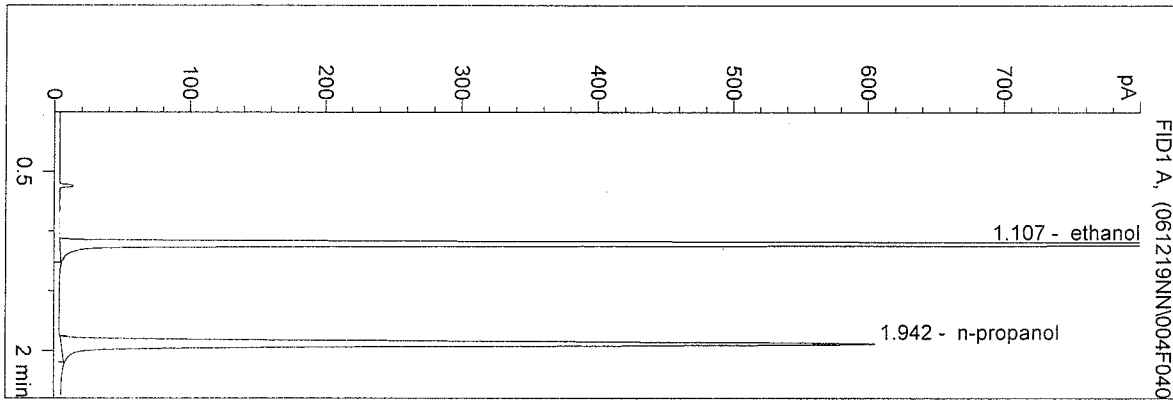


#	Compound	Area	RT
1	ethanol	2571	1.107
2	n-propanol	1766	1.942

Totals:

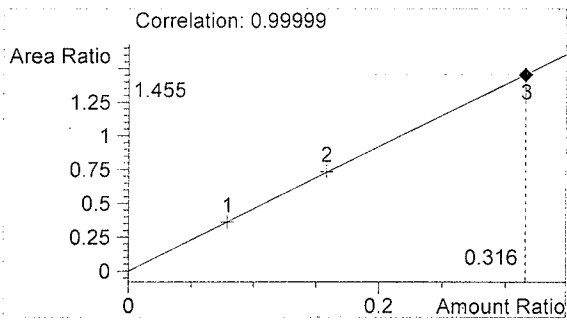

ethanol 0.316 g/100ml

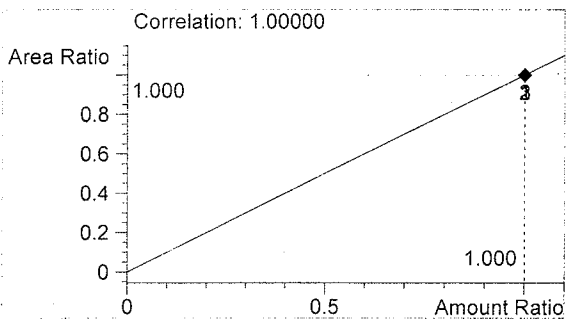


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:34:07 AM
 Instrument 5
 DB-ALC2


BLANK
 N Nuwayhid, PhD

vial # 5

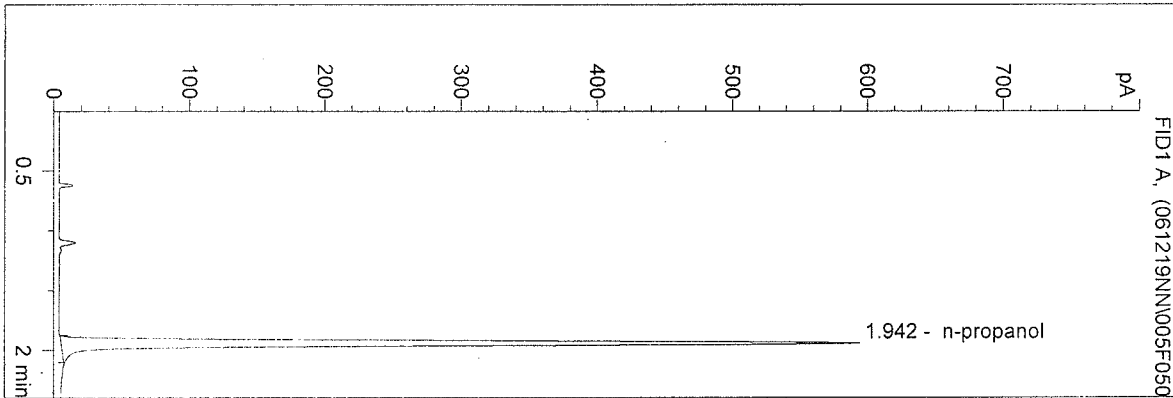


#	Compound	Area	RT
1	ethanol	0	0.000
2	n-propanol	1738	1.942

Totals:

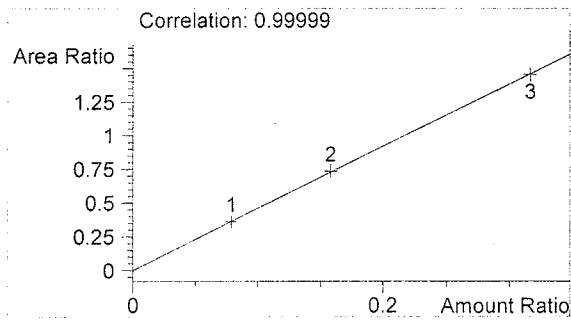

ethanol 0.000 g/100ml

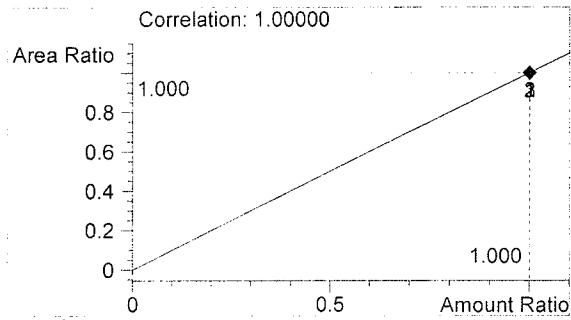


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:37:31 AM
 Instrument 5
 DB-ALC2


0.100 CTL
 N Nuwayhid, PhD

vial # 6

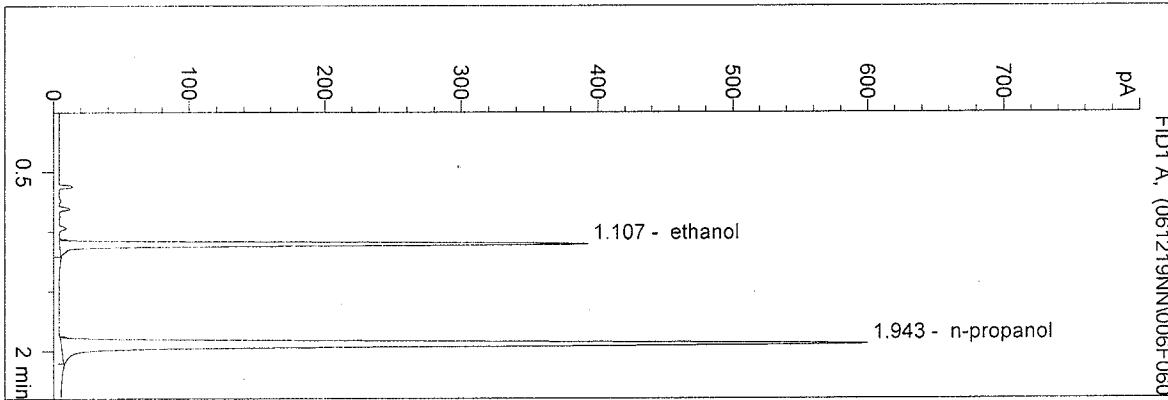


#	Compound	Area	RT
1	ethanol	804	1.107
2	n-propanol	1753	1.943

Totals:

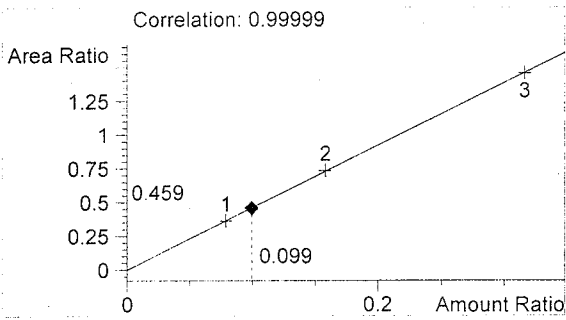

ethanol 0.099 g/100ml

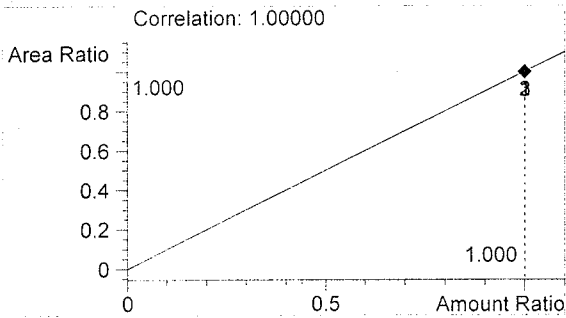


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:42:35 AM
 Instrument 5
 DB-ALC2


06050 QA-1
 N Nuwayhid, PhD

vial # 7

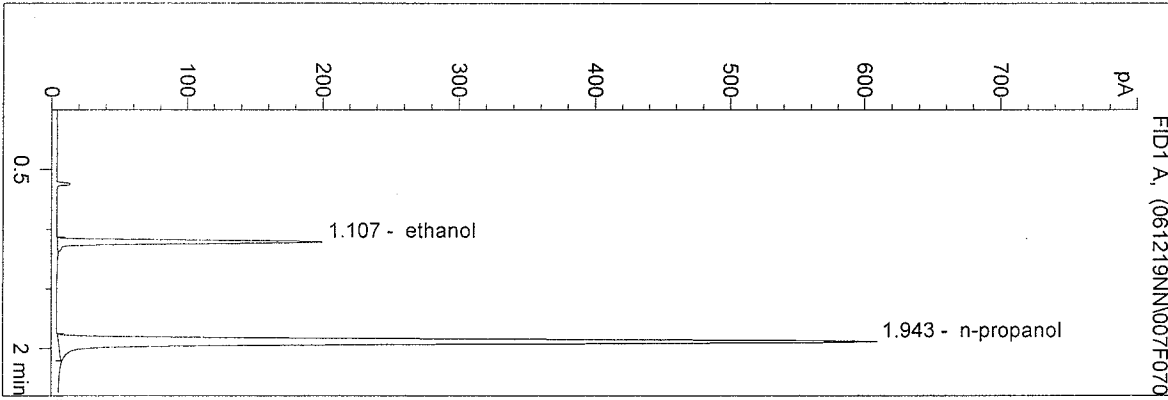


#	Compound	Area	RT
1	ethanol	406	1.107
2	n-propanol	1783	1.943

Totals:

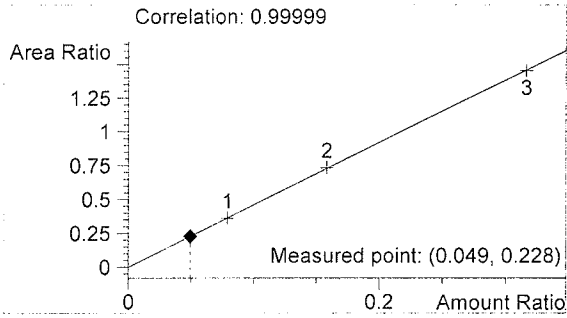

ethanol 0.049 g/100ml

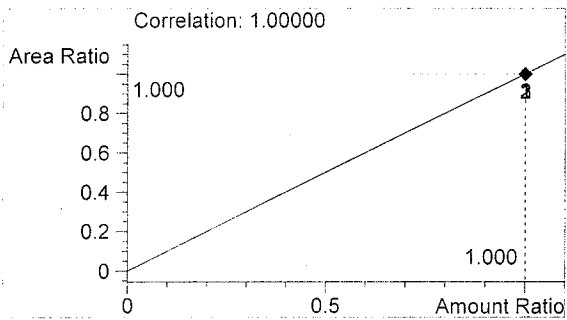


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:45:59 AM
 Instrument 5
 DB-ALC2


06050 QA-2
 N Nuwayhid, PhD

vial # 8

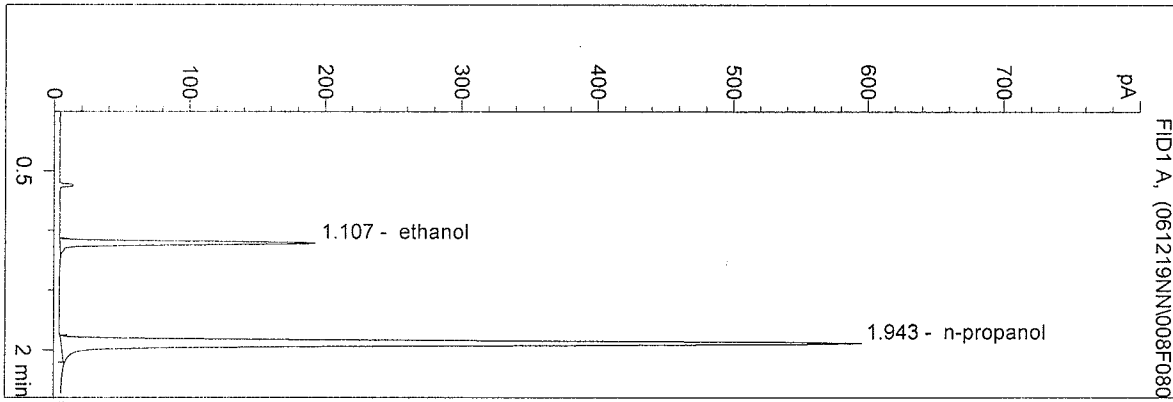


#	Compound	Area	RT
1	ethanol	393	1.107
2	n-propanol	1745	1.943

Totals:

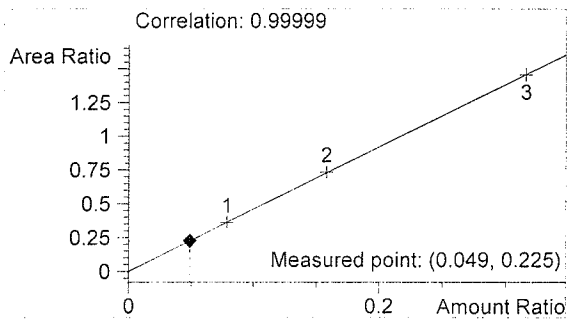

ethanol 0.049 g/100ml

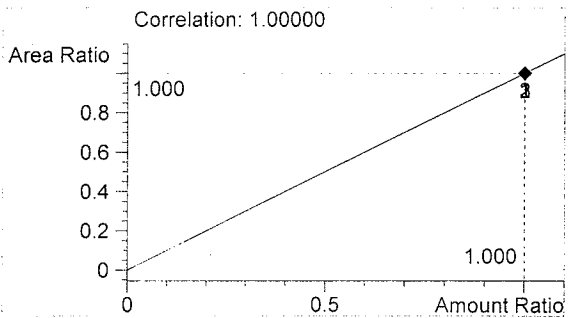


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:49:32 AM
 Instrument 5
 DB-ALC2


06050 QA-3
 N Nuwayhid, PhD

vial # 9

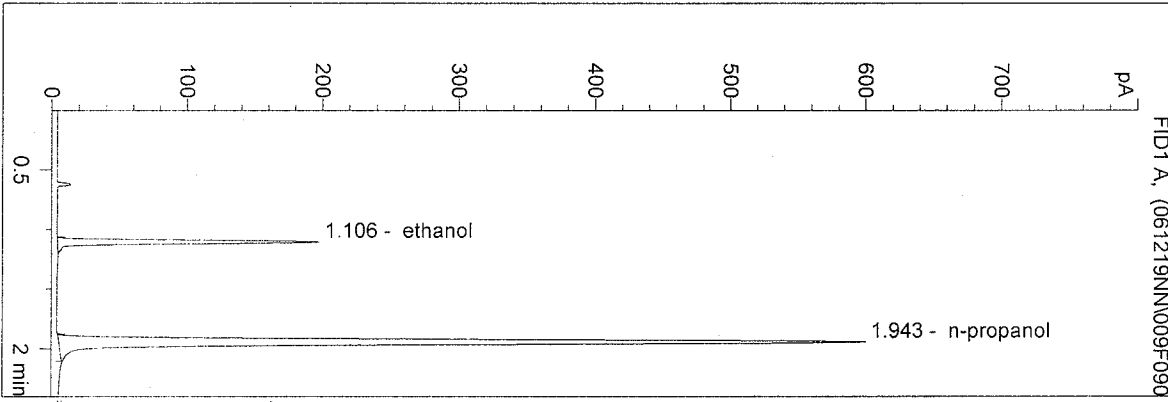


#	Compound	Area	RT
1	ethanol	401	1.106
2	n-propanol	1762	1.943

Totals:

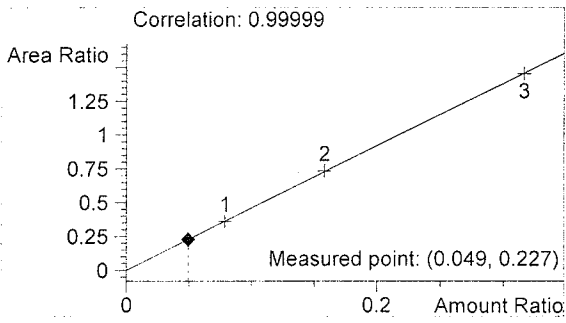

ethanol 0.049 g/100ml

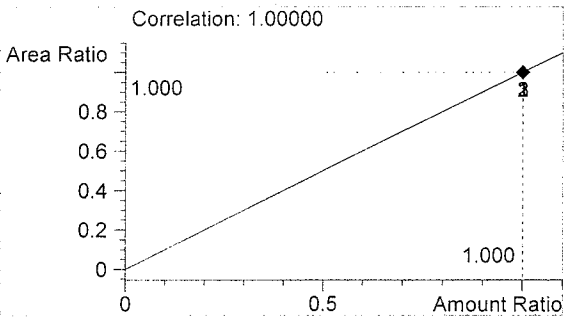


n-propanol 1.000 g/100ml


D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:54:26 AM
 Instrument 5
 DB-ALC2

06050 QA-4
 N Nuwayhid, PhD


vial # 10

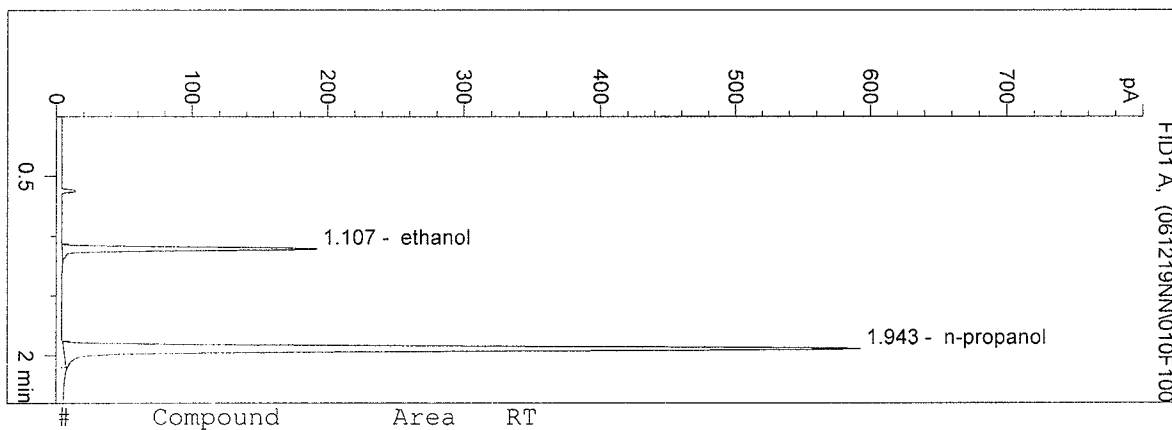

Totals:

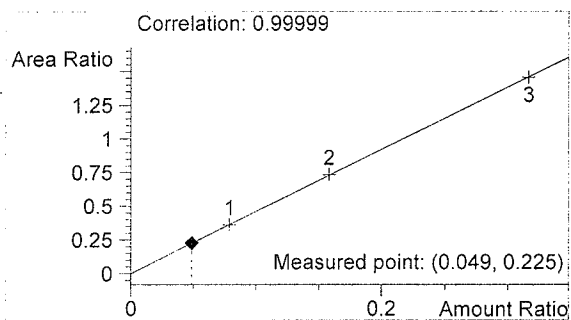

ethanol 0.049 g/100ml

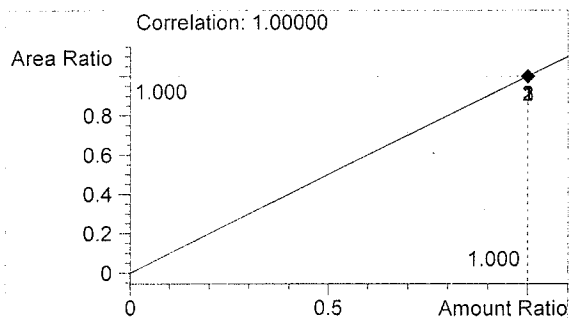


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 10:57:50 AM
 Instrument 5
 DB-ALC2


06050 QA-5
 N Nuwayhid, PhD

vial # 11

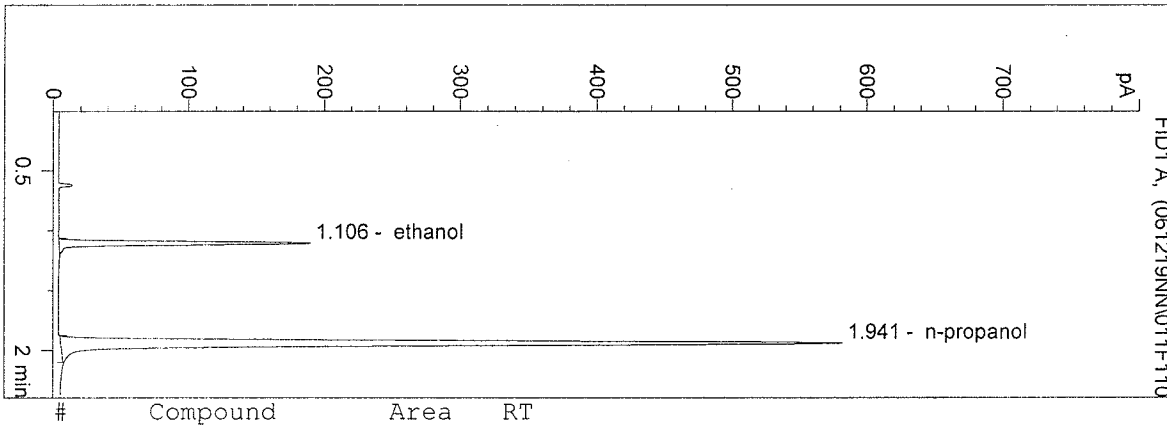


#	Compound	Area	RT
1	ethanol	380	1.106
2	n-propanol	1698	1.941

Totals:

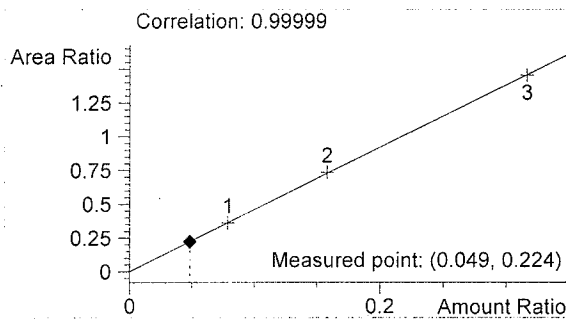

ethanol 0.049 g/100ml

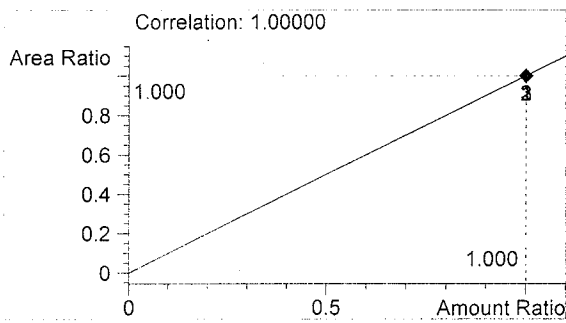


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 11:01:29 AM
 Instrument 5
 DB-ALC2


0.100 CTL
 N Nuwayhid, PhD

vial # 12

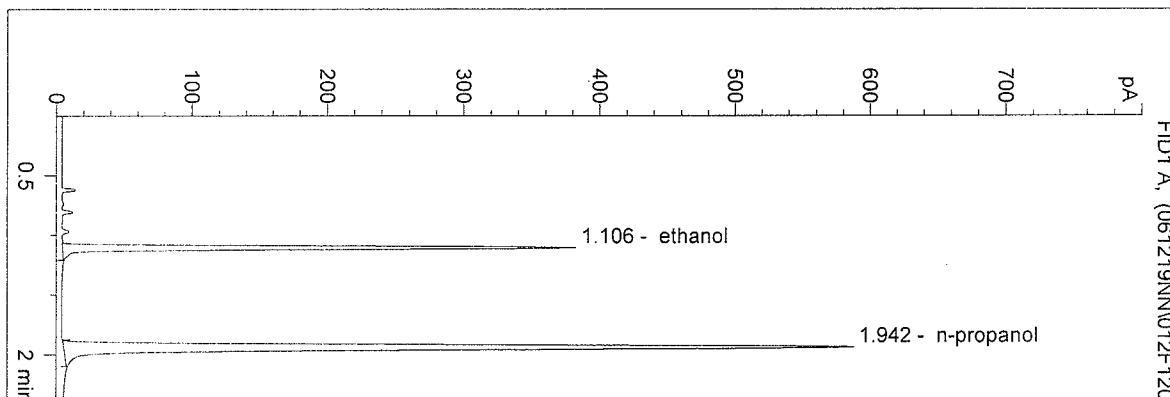


#	Compound	Area	RT
1	ethanol	781	1.106
2	n-propanol	1719	1.942

Totals:

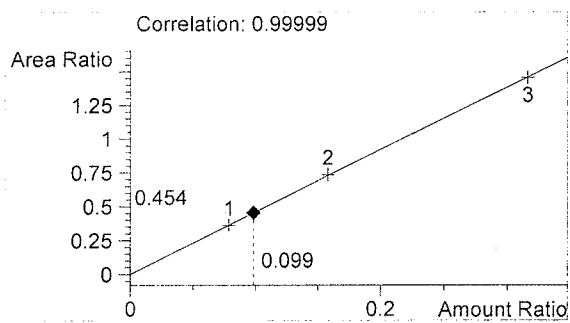

ethanol 0.099 g/100ml

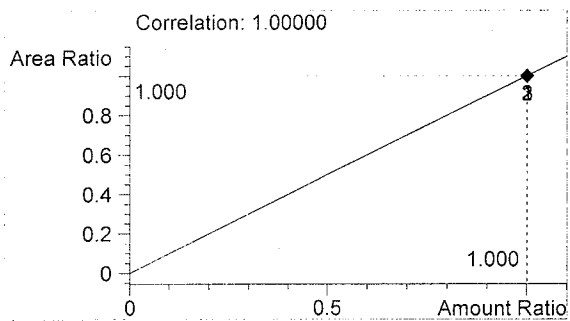


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/19/2006 11:06:25 AM
 Instrument 5
 DB-ALC2


BLANK
 N Nuwayhid, PhD

vial # 13

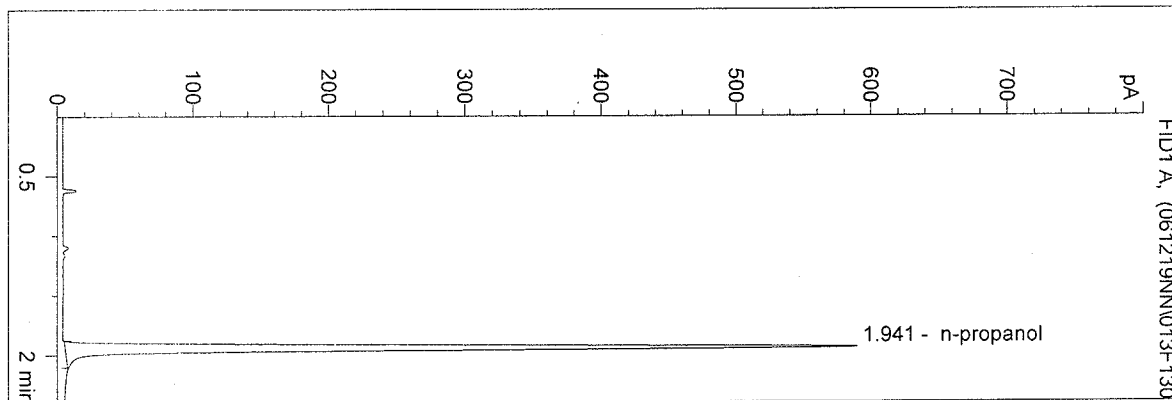


#	Compound	Area	RT
1	ethanol	0	0.000
2	n-propanol	1720	1.941

Totals:

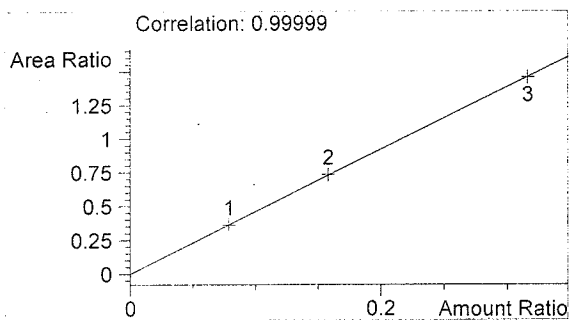

ethanol 0.000 g/100ml

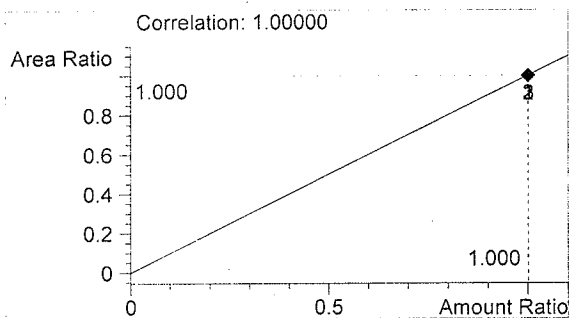


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:03:58 PM
 Instrument 4
 DB-ALC1


06050-1
 Justin Knoy

vial # 63

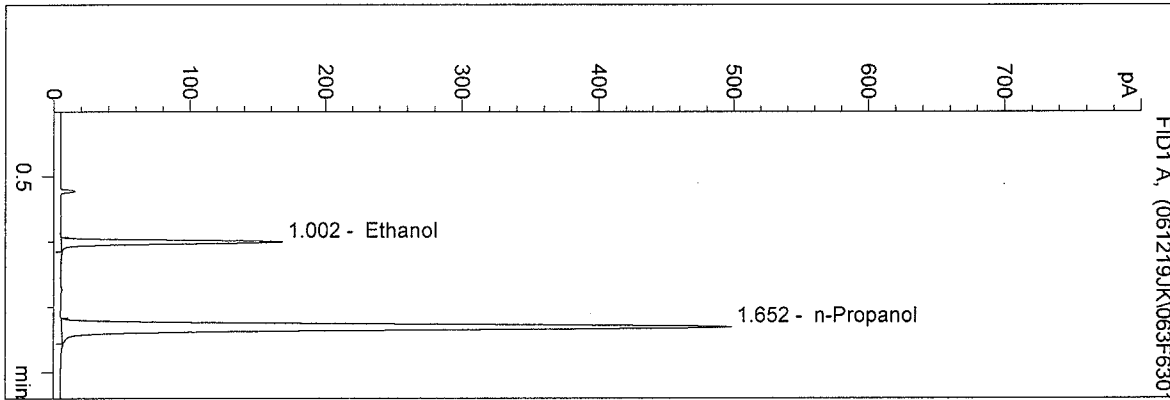


#	Compound	Area	RT
1	Ethanol	323	1.002
2	n-Propanol	1538	1.652

Totals:

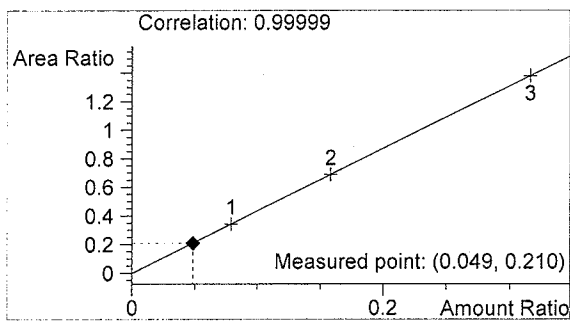

Ethanol 0.049 g/100ml

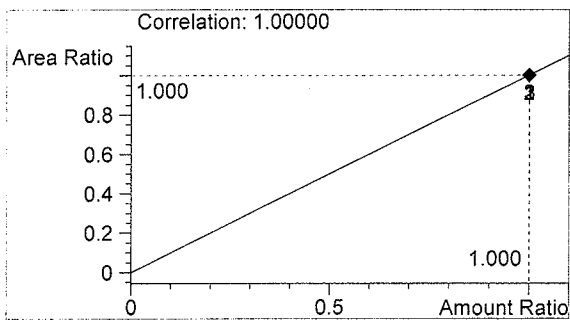


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:07:17 PM
 Instrument 4
 DB-ALC1


06050-2
 Justin Knoy

vial # 64

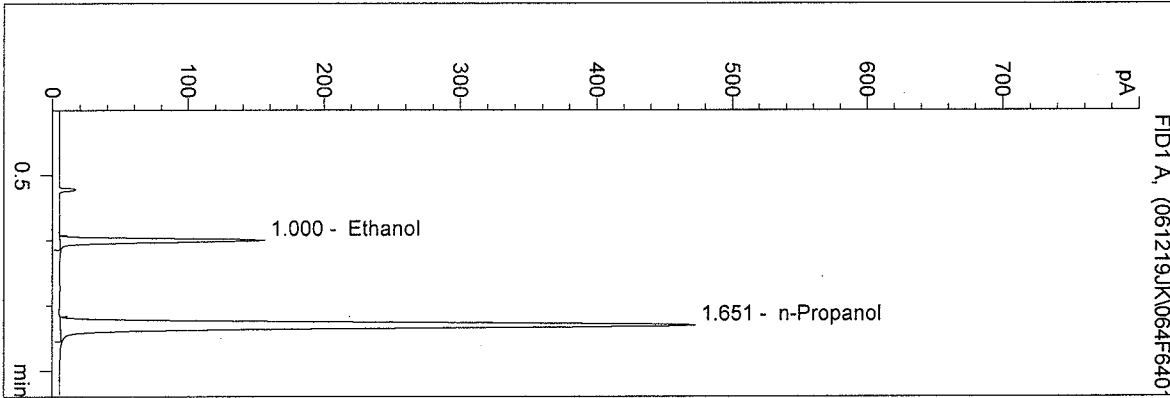


#	Compound	Area	RT
1	Ethanol	307	1.000
2	n-Propanol	1469	1.651

Totals:

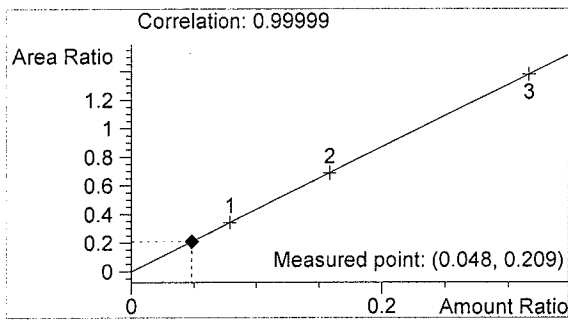

Ethanol 0.048 g/100ml

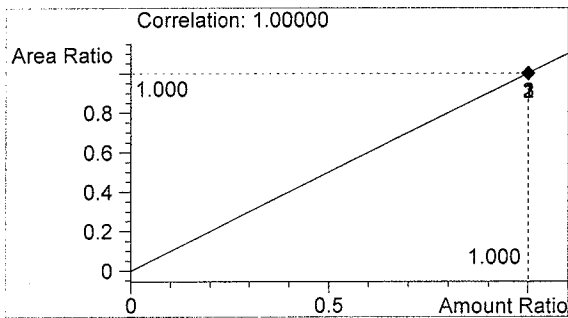


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:15:48 PM
 Instrument 4
 DB-ALC1


06050-3
 Justin Knoy

vial # 65

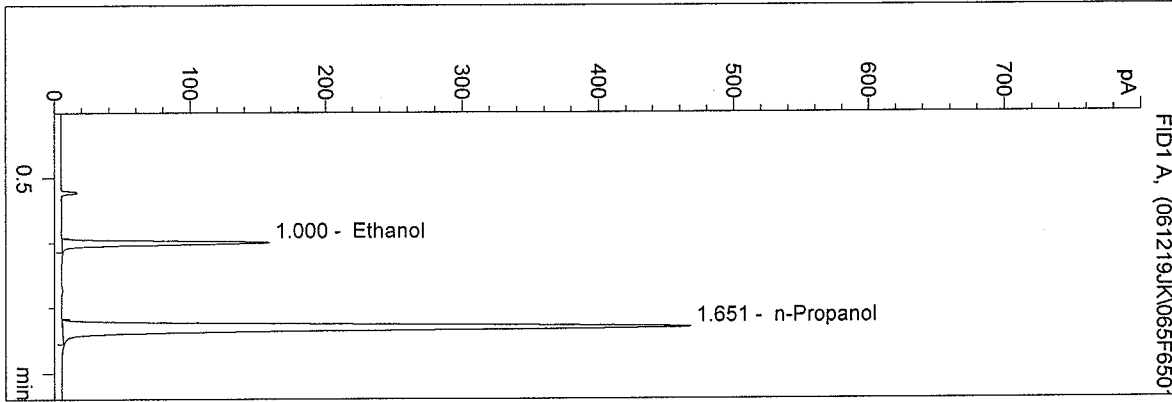


#	Compound	Area	RT
1	Ethanol	310	1.000
2	n-Propanol	1452	1.651

Totals:

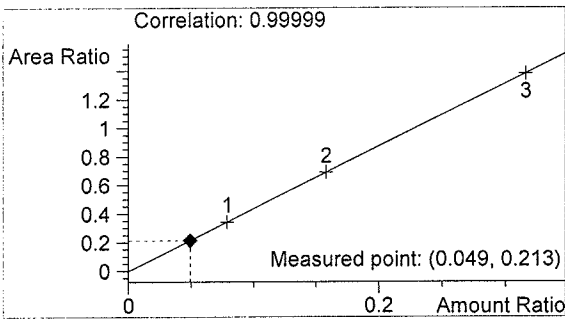

Ethanol 0.049 g/100ml

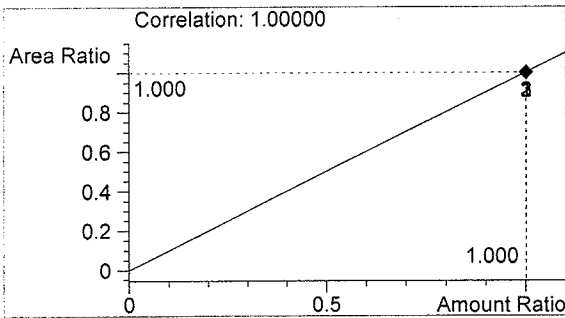


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:19:13 PM
 Instrument 4
 DB-ALC1


06050-4
 Justin Knoy

vial # 66

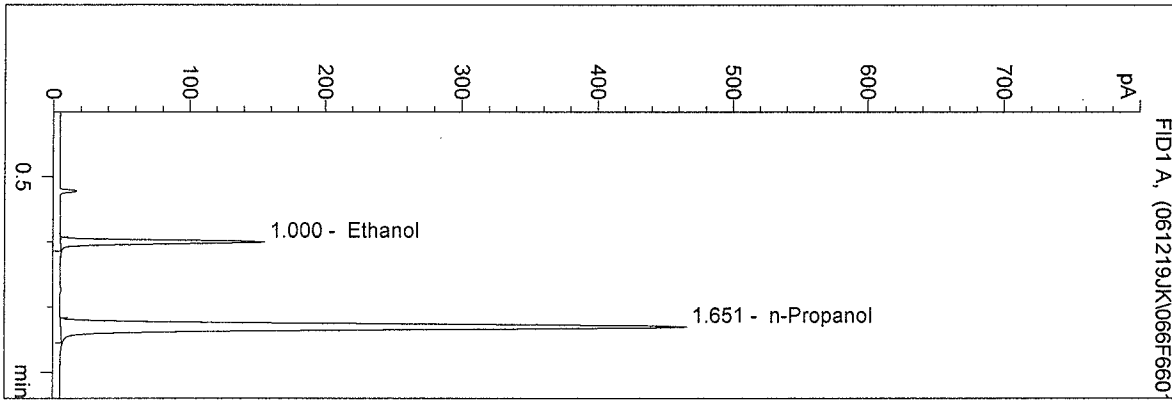


#	Compound	Area	RT
1	Ethanol	302	1.000
2	n-Propanol	1443	1.651

Totals:

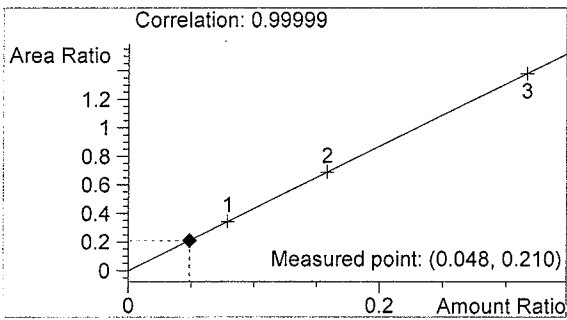

Ethanol 0.048 g/100ml

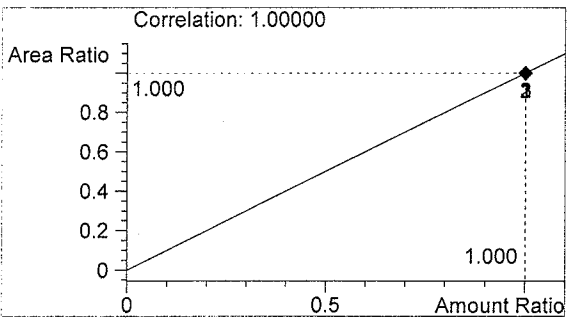


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:22:29 PM
 Instrument 4
 DB-ALC1


06050-5
 Justin Knoy

vial # 67

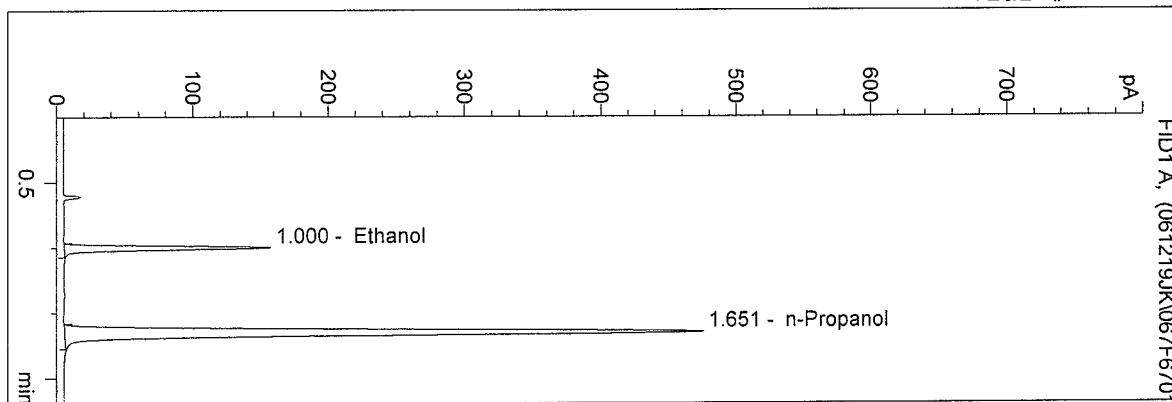


#	Compound	Area	RT
1	Ethanol	309	1.000
2	n-Propanol	1476	1.651

Totals:

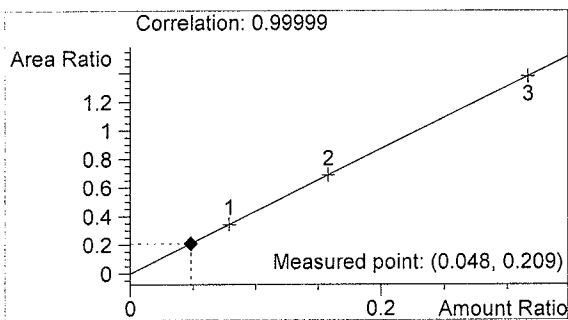

Ethanol 0.048 g/100ml

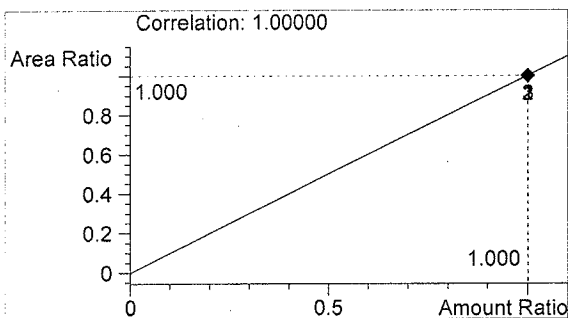


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:25:44 PM
 Instrument 4
 DB-ALC1


0.10 CTRL JK
 Justin Knoy

vial # 68

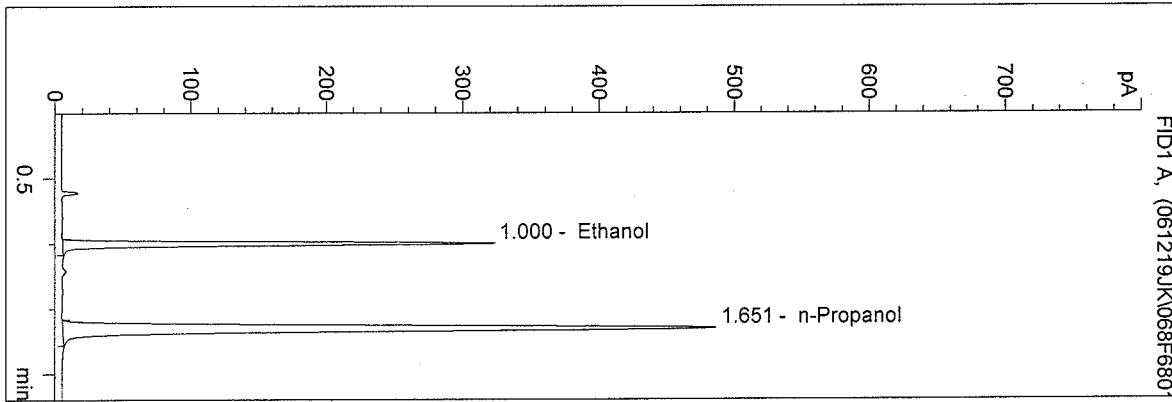


#	Compound	Area	RT
1	Ethanol	643	1.000
2	n-Propanol	1510	1.651

Totals:

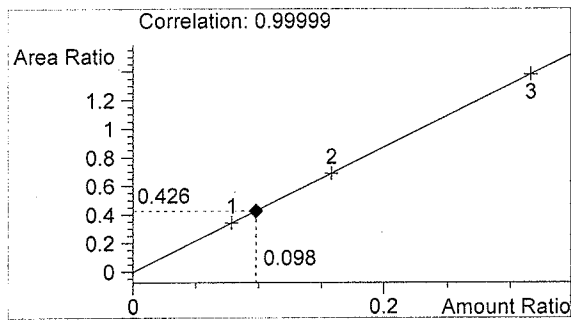

Ethanol 0.098 g/100ml

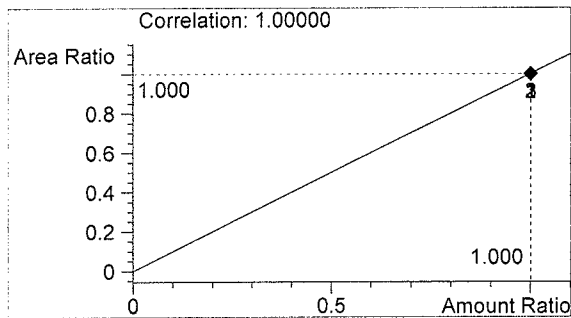


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO.M
 12/19/2006 8:28:57 PM
 Instrument 4
 DB-ALC1


blank
 Justin Knoy

vial # 69

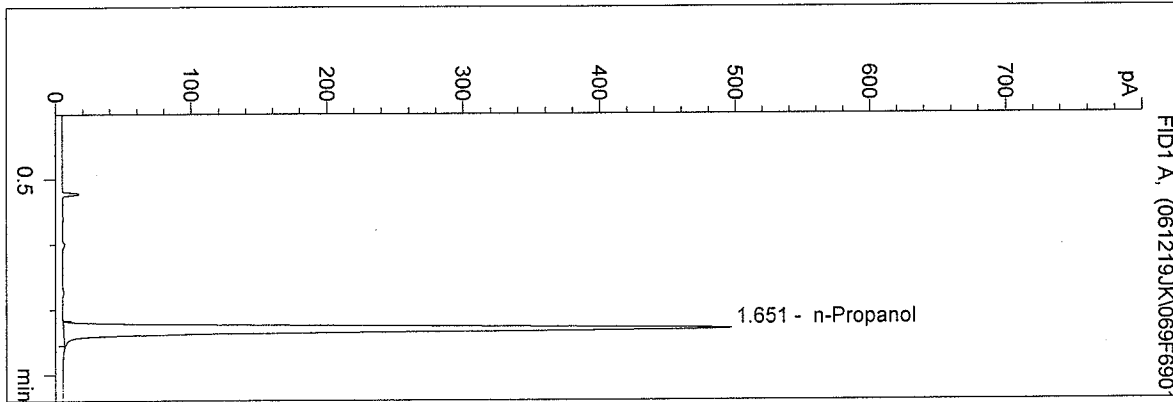


#	Compound	Area	RT
1	Ethanol	0	0.000
2	n-Propanol	1542	1.651

Totals:

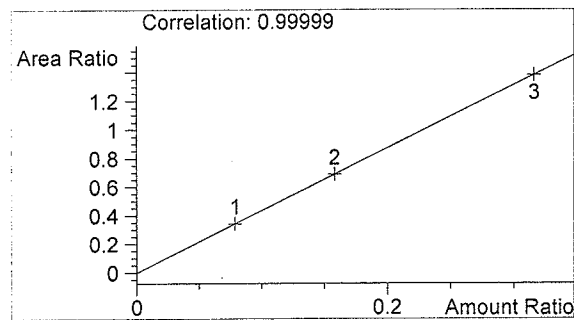

Ethanol 0.000 g/100ml

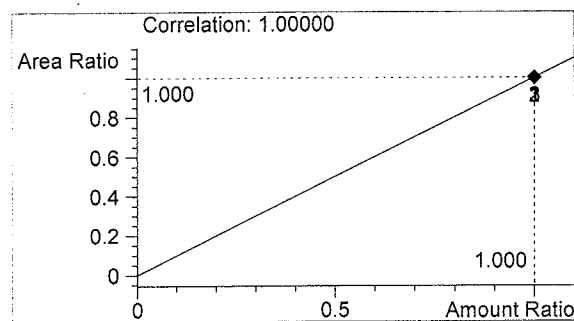


n-Propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:28:29 AM
 Instrument 5
 DB-ALC2


06050
 bcapron

vial # 21

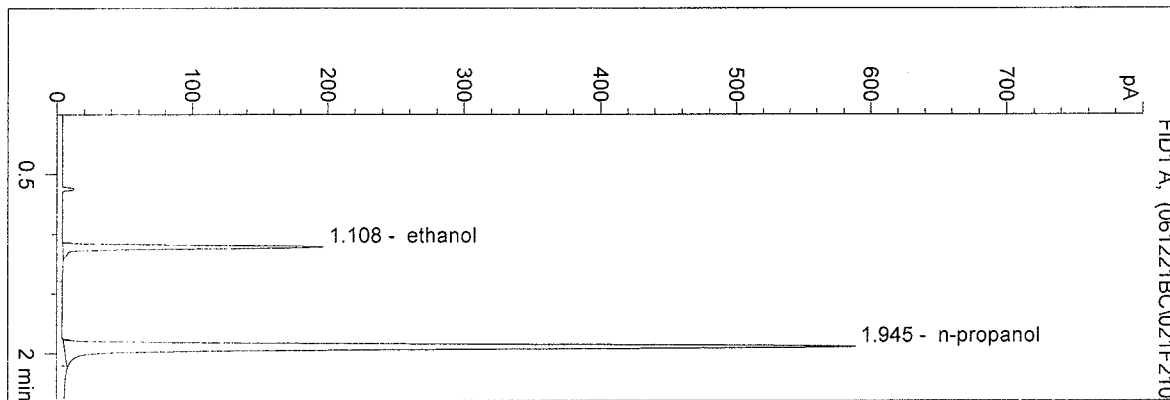


#	Compound	Area	RT
1	ethanol	401	1.108
2	n-propanol	1722	1.945

Totals:

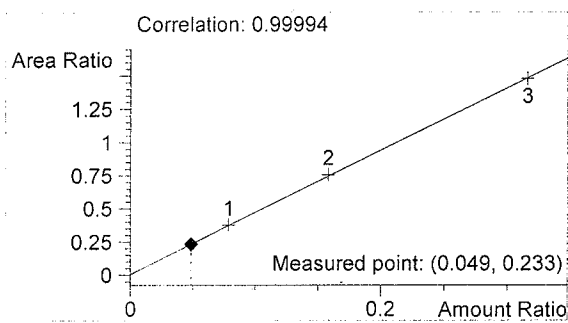

ethanol 0.049 g/100ml

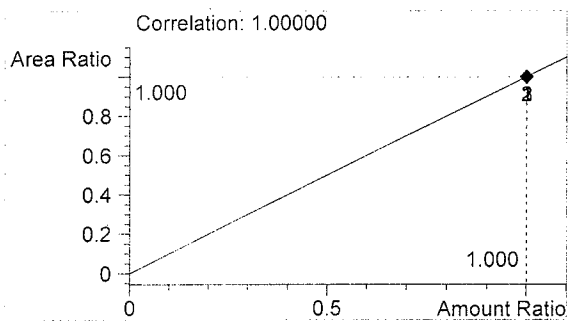


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:33:33 AM
 Instrument 5
 DB-ALC2


06050
 bcapron

vial # 22

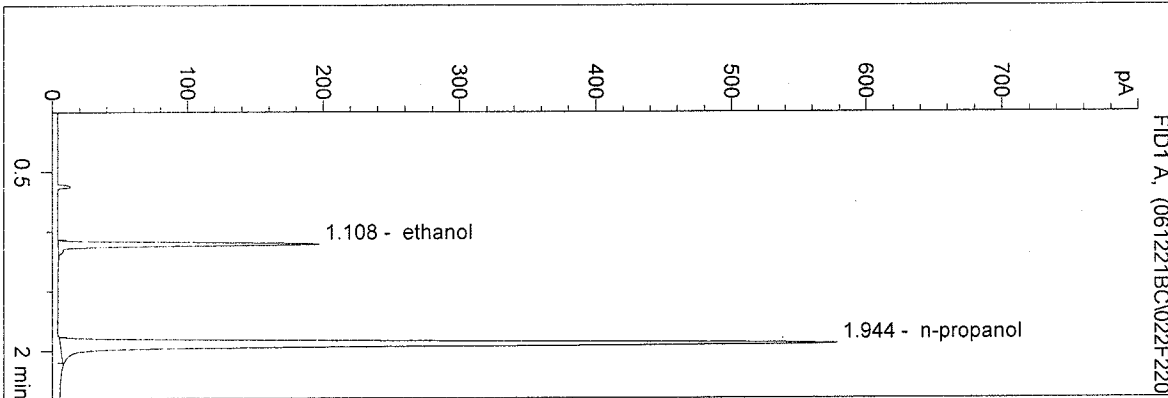


#	Compound	Area	RT
1	ethanol	390	1.108
2	n-propanol	1685	1.944

Totals:

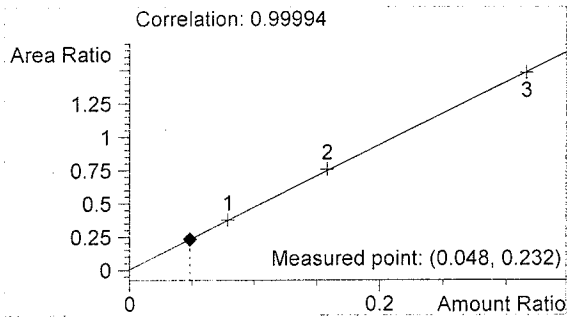

ethanol 0.048 g/100ml

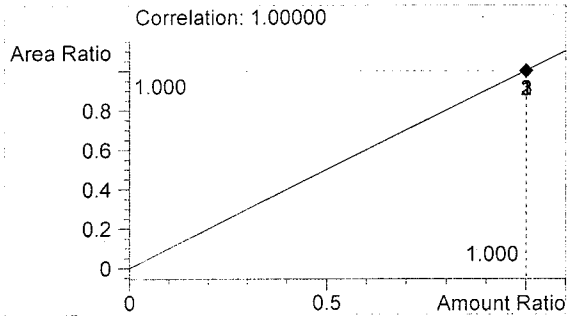


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:37:10 AM
 Instrument 5
 DB-ALC2


06050
 bcapron

vial # 23

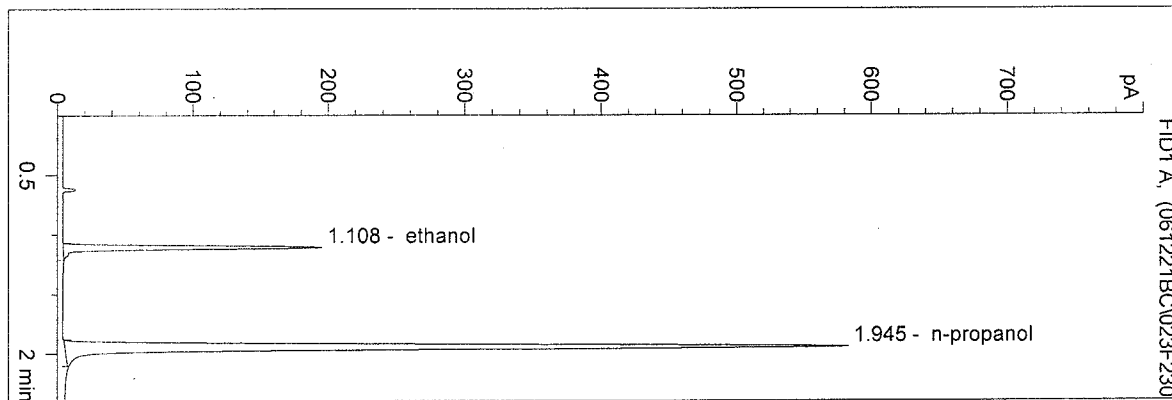


#	Compound	Area	RT
1	ethanol	394	1.108
2	n-propanol	1700	1.945

Totals:

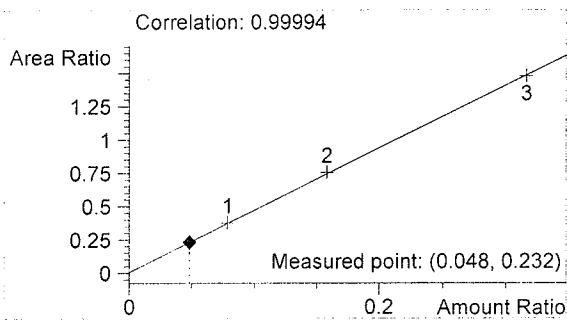

ethanol 0.048 g/100ml

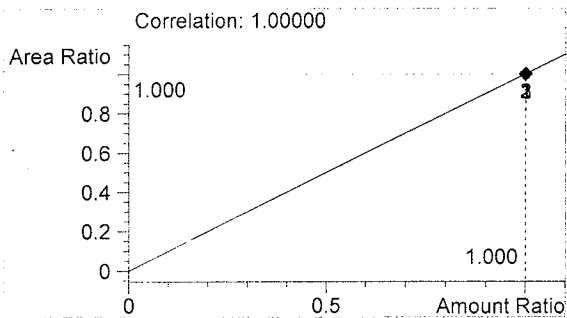


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:40:30 AM
 Instrument 5
 DB-ALC2


06050
 bcapron

vial # 24

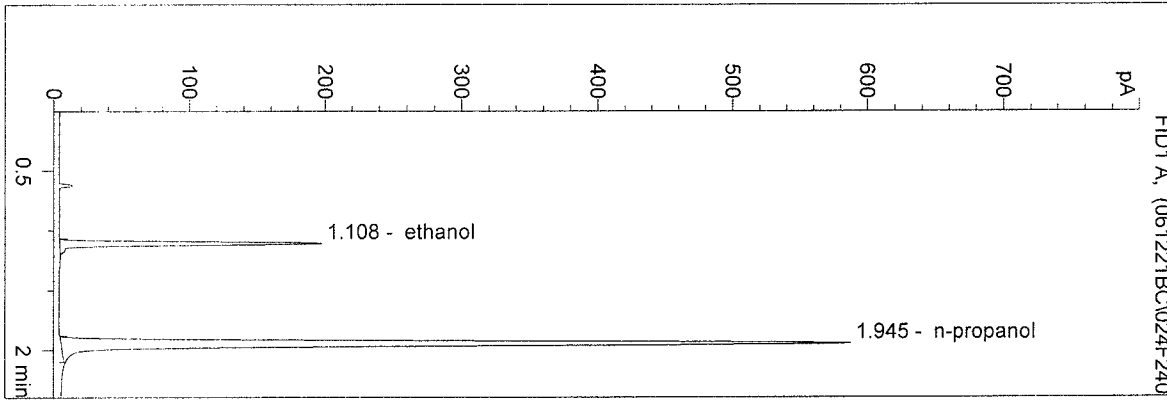


#	Compound	Area	RT
1	ethanol	397	1.108
2	n-propanol	1711	1.945

Totals:

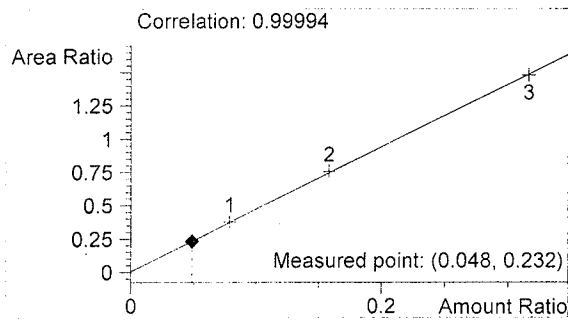

ethanol 0.048 g/100ml

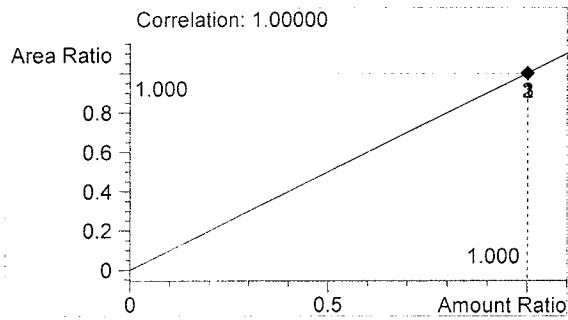


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:45:38 AM
 Instrument 5
 DB-ALC2


06050
 bcapron

vial # 25

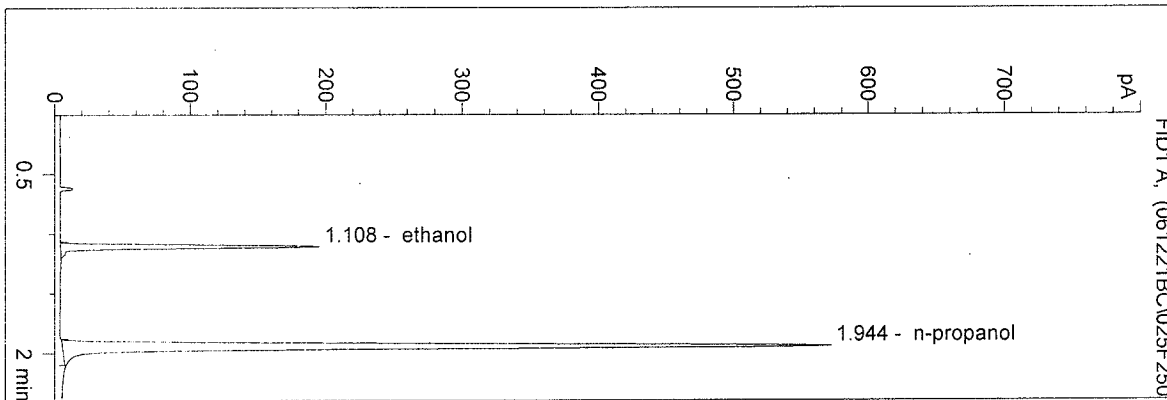


#	Compound	Area	RT
1	ethanol	386	1.108
2	n-propanol	1667	1.944

Totals:

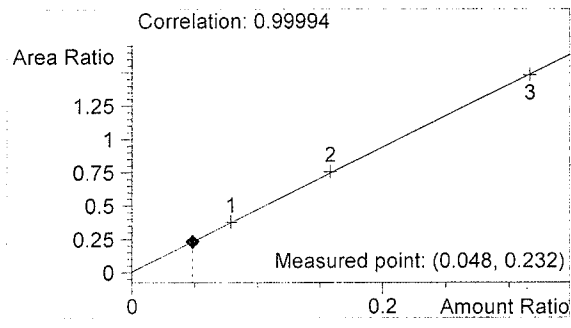

ethanol 0.048 g/100ml

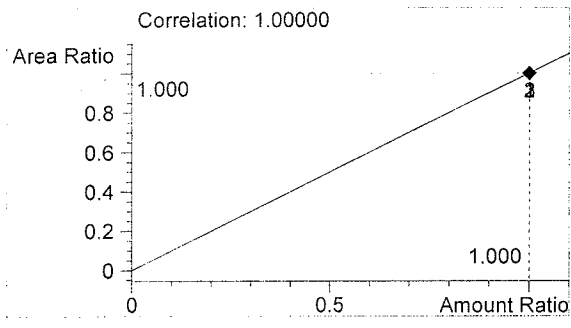


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:49:12 AM
 Instrument 5
 DB-ALC2


0.10 control bc
 bcapron

vial # 26

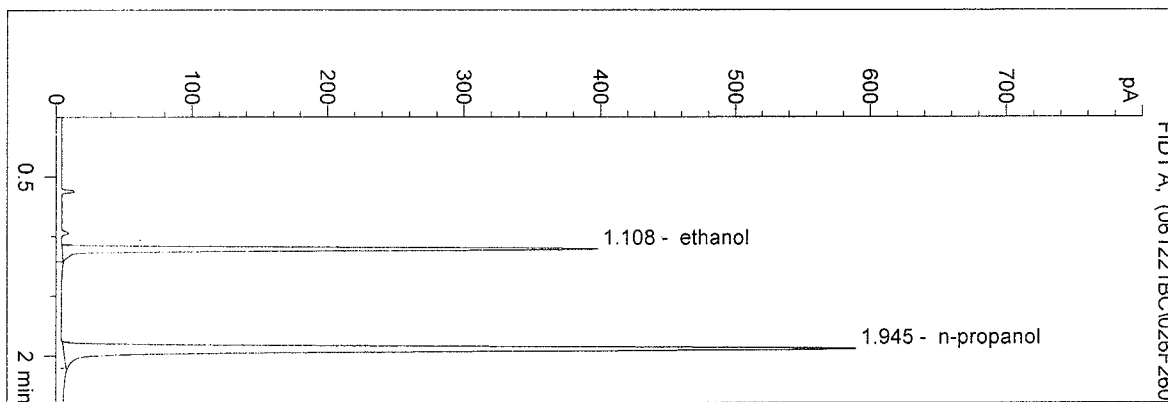


#	Compound	Area	RT
1	ethanol	808	1.108
2	n-propanol	1720	1.945

Totals:

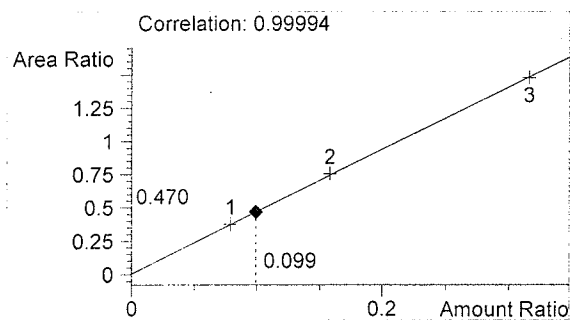

ethanol 0.099 g/100ml

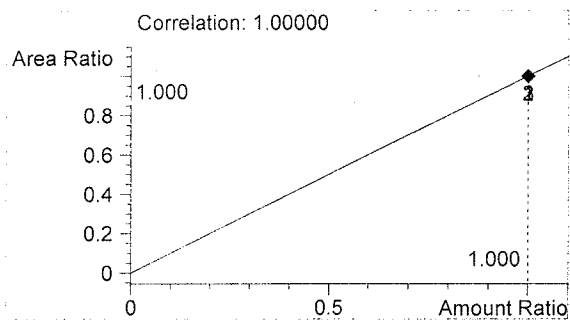


n-propanol 1.000 g/100ml

D:\HPCHEM\1\METHODS\BLDALCO2.M
 12/21/2006 8:52:27 AM
 Instrument 5
 DB-ALC2


blank
 bcapron

vial # 27

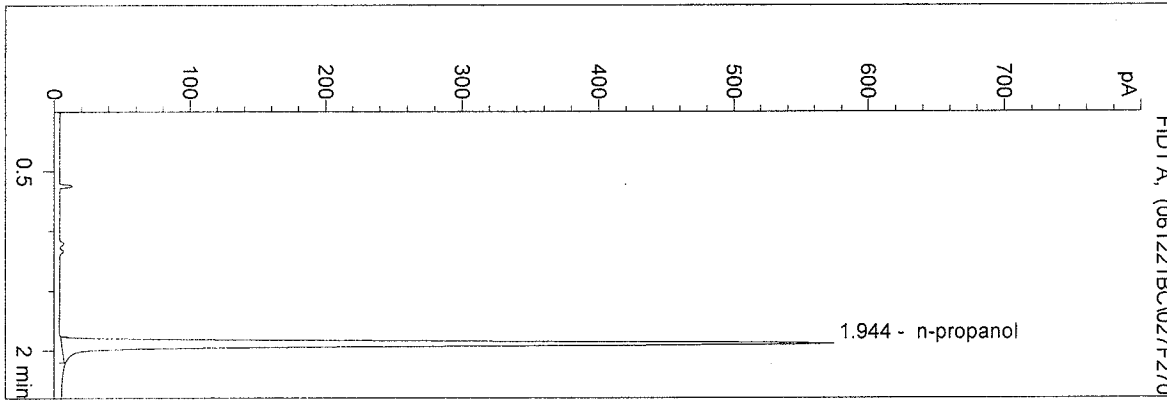


#	Compound	Area	RT
1	ethanol	0	0.000
2	n-propanol	1676	1.944

Totals:

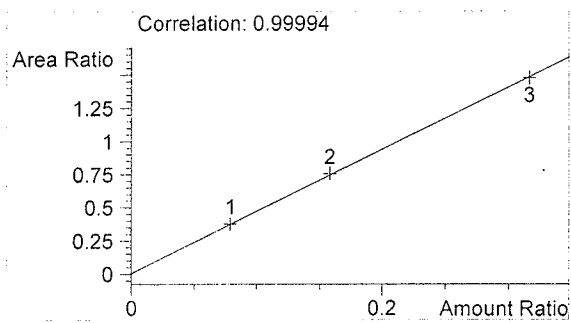

ethanol 0.000 g/100ml

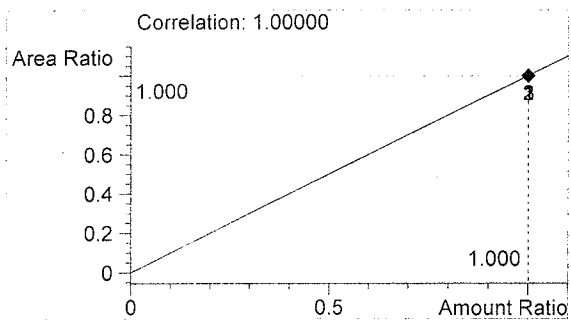

n-propanol 1.000 g/100ml