



QUALITY ASSURANCE PROCEDURE SOLUTION TEST REPORT

BATCH REPORT: 15008

CUSTOMER INFORMATION

Washington State Patrol – Breath Test Program
811 East Roanoke SEATTLE, WA 98102

TESTING PROCEDURE USED: TLD Technical Manual, Chapter 4.0 Certification of Simulator Solutions;
Headspace-Gas Chromatography.

TESTING ITEM INFORMATION

TARGET VAPOR CONCENTRATION: 0.20 g/210L
DATE PREPARED: 01/13/2015
BATCH UNITS: g/100mL

IDENTITY: QAP Solution
PREPARED BY: Elizabeth Wehner

| | EW | DN | NN |
|---|-------|-------|-------|
| 1 | 0.255 | 0.249 | 0.255 |
| 2 | 0.254 | 0.251 | 0.256 |
| 3 | 0.255 | 0.252 | 0.254 |
| 4 | 0.255 | 0.255 | 0.256 |
| 5 | 0.257 | 0.254 | 0.254 |
| C | 0.103 | 0.102 | 0.103 |

ETHANOL CONTROL INFORMATION

LOT NUMBER: FN08051301 EXPIRATION: 10/2018 CONCENTRATION: 0.10 g/100mL

RESULTS OF TESTING

AVERAGE SOLUTION CONCENTRATION: 0.2541 g/100mL PRECISION CV (%): 0.81
STANDARD DEVIATION: 0.00207 NUMBER OF TESTS: 15

EQUIVALENT VAPOR CONCENTRATION: **0.2066 g/210L**
EXPANDED UNCERTAINTY: ± 0.0046 (k=2, 95.45% confidence interval)




WASHINGTON STATE PATROL – TOXICOLOGY LABORATORY DIVISION



Lisa Noble Forensic Scientist Supervisor

2/4/15

DATE REPORT ISSUED

| THIS TESTING WAS PERFORMED BY: | | | |
|--------------------------------|------------------|--|-------------|
| ANALYST | NAME | SIGNATURE | DATE TESTED |
| EW | Elizabeth Wehner |  | 01/13/2015 |
| DN | David Nguyen |  | 01/14/2015 |
| NN | Naziha Nuwayhid |  | 01/14/2015 |

Washington State Patrol - Toxicology Laboratory Division
QAP Test Report Calculation Record

QAP Solution Batch #: 15008

Date Prepared: 1/13/2015

| Analyst: | EW | DN | NN |
|--------------|-----------|-----------|-----------|
| Date Tested: | 1/13/2015 | 1/14/2015 | 1/14/2015 |
| Instrument: | HSGC #3 | HSGC #3 | HSGC #3 |
| 1 | 0.255 | 0.249 | 0.255 |
| 2 | 0.254 | 0.251 | 0.256 |
| 3 | 0.255 | 0.252 | 0.254 |
| 4 | 0.255 | 0.255 | 0.256 |
| 5 | 0.257 | 0.254 | 0.254 |
| C | 0.103 | 0.102 | 0.103 |

| CV^2_{COA} | $CV^2_{QAP\ Solution}$ | $CV^2_{Control}$ | $CV^2_{Part\ Coef}$ |
|--------------|------------------------|------------------|---------------------|
| 0.0000084100 | 0.0000044043 | 0.0000105414 | 0.0001016326 |

Ethanol Control Lot #: FN08051301
Control Uncertainty (%): 0.29

Average Solution Concentration: 0.2541 g/100mL
Standard Deviation: 0.00207 g/100mL
Precision CV (%): 0.81
Equivalent Vapor Concentration: 0.2066 g/210L
Combined Standard Uncertainty (\pm): 0.0023 g/210L
Expanded Uncertainty (\pm): 0.0046 coverage factor (k) =2 (95.45% level of confidence)

Calculations performed by: Lira Noble Anahobe 1/27/15
Name Signature Date

Calculations verified by: Amanda M. Black [Signature] 2-3-2015 Method: Hand calculation
Name Signature Date

Tech. review performed by: Lira Noble Anahobe 1/27/15
Name Signature Date

fn

SIMULATOR SOLUTION DATA ENTRY REVIEW

Reviewer/s: Amanda M. Black

Date: 2-3-2015

Location: WSP-FLSB Seattle, WA

Solution Batch Number: 15008

| | YES | NO | N/A |
|---|-------------------------------------|--------------------------|--------------------------|
| Analysis dates do not precede preparation date: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Declarations signed and properly dated: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Data entry corresponds to all chromatograms: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| All signatures present on Test Report: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Average solution concentration correct: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Standard deviation correct: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| CV (%) correct: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Equivalent vapor concentration correct: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| All chromatograms and sequences included in file: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Ethanol control information present: (lot # present & used within expiration) | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |
| Complies with accuracy and precision requirements established by the State Toxicologist: | <input checked="" type="checkbox"/> | <input type="checkbox"/> | <input type="checkbox"/> |

Comments:

Reviewer Signature: 

Date: 2-3-2015



SOLUTION CERTIFICATE REVIEW

Please check that the data on your chromatograms is the data entered into the Test Report, that the date to the right of your name is the date that you tested the solution, and then sign the Test Report.

Please initial and date below to affirm that you have:

- 1) Checked your data
- 2) Checked the date to the right of your name on the Test Report
- 3) Signed the Test Report

| | Initials | Date |
|-------------------------------|----------|----------|
| Amanda Chandler | | |
| Andrew Gingras | | |
| Asa Louis | | |
| Brittany Thomas | | |
| Christie Mitchell-Mata | | |
| Christopher Johnston | | |
| David Nguyen | DN | 1/28/15 |
| Dawn Sklerov | | |
| Elizabeth Wehner | EW | 01/28/15 |
| Justin Knoy | | |
| Katie Harris | | |
| Lyndsey Lowe | | |
| Naziha Nuwayhid | NN | 1.28.15 |
| Rebecca Flaherty | | |

Batch # 15008 1/27/15

[Faint signature]

[Handwritten signature]

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2927 • (206) 262-6100 • FAX (206) 262-6145

**0.20 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 15008**

I, Elizabeth Wehner, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Biochemistry.

The quality assurance procedure (QAP) solution, Lot Number 15008, was prepared in the Washington State Toxicology Laboratory on 1/13/2015. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 1/13/2016.

Seattle, WA

Elizabeth Wehner 01/28/15

Elizabeth Wehner

Date

Forensic Scientist



JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2927 • (206) 262-6100 • FAX (206) 262-6145

**0.20 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 15008**


I, David Nguyen, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Chemistry.

The quality assurance procedure (QAP) solution, Lot Number 15008, was prepared in the Washington State Toxicology Laboratory on 1/13/2015. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 1/13/2016.

Seattle, WA

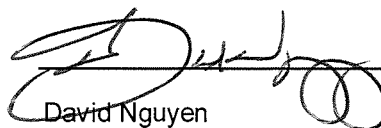 - 1/29/15
Date

David Nguyen
Forensic Scientist

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2927 • (206) 262-6100 • FAX (206) 262-6145

**0.20 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 15008**


I, Naziha Nuwayhid, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: Bachelor and Masters Degrees in Biology, Ph.D. degree in Basic Medical Science, ten years experience in clinical laboratory sciences, one year in clinical toxicology and more than ten years in forensic toxicology. I am also board certified by the American Board of Clinical Chemistry.

The quality assurance procedure (QAP) solution, Lot Number 15008, was prepared in the Washington State Toxicology Laboratory on 1/13/2015. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 1/13/2016.

Seattle, WA

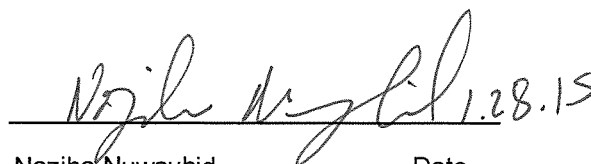

Naziha Nuwayhid Date

Forensic Scientist



FILE A COPY IN THE BATCH FILE FOR EACH SOLUTION LISTED ON THE WORKSHEET

Preparation Date: 01/13/15 Expiration Date: 01/13/16 Initials of Preparer: EW

Lot # of 200-proof Ethanol used in preparation: 2D60231

Date the 200-proof Ethanol bottle was opened: 12/03/14

After opening, each bottle of 200-proof Ethanol is approved for use for 6 months unless an extension is approved by the State Toxicologist. This timeframe applies to the 200-proof Ethanol only, not to simulator solutions which have a 1 year expiration.

Environmental conditions verified as acceptable:

| Simulator Solution | Volume of Ethanol (mL) | Volume of Deionized Water (L) | | Batch Number |
|--------------------|------------------------|-------------------------------|-------------------------------------|-------------------|
| QAP 0.04 | 11.2 | 18 | <input checked="" type="checkbox"/> | <u>15004</u> |
| QAP 0.08 | 22.4 | 18 | <input checked="" type="checkbox"/> | <u>15005</u> |
| QAP 0.10 | 28.1 | 18 | <input checked="" type="checkbox"/> | <u>15006</u> |
| QAP 0.15 | 42.1 | 18 | <input checked="" type="checkbox"/> | <u>15007</u> |
| QAP 0.20 | 56.1 | 18 | <input checked="" type="checkbox"/> | <u>15008</u> |
| ESS | 66.5 | 52 | <input type="checkbox"/> | <u> </u> |

Stir bar is rotating

Stirred for minimum 30 minutes; 2 hours for ESS

Spigot purged

Aliquot taken

Batch labeled, packaged and sealed

01/13/15
Date

If different ethanol lot numbers are used in the preparation of solutions, record them and the corresponding solution batch numbers in the comments section.

Comments:

Elizabeth Wehner
Analyst Signature

01/13/15
Date *EW*

Sequence Parameters:

Operator: Elizabeth Wehner
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\2\DATA\
 Data Subdirectory: 150113EW
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

CAL 1: 0.079 g/100mL - LOT# E0814-01 - EXP 02/19/2015
 CAL 2: 0.158 g/100mL - LOT# E0814-02 - EXP 02/19/2015
 CAL 3: 0.316 g/100mL - LOT# E0814-03 - EXP 02/19/2015

 CTRL 1: 0.04 g/100mL - LOT# FN05011301 - EXP 05/2018
 CTRL 2: 0.10 g/100mL - LOT# FN08051301 - EXP 10/2018
 CTRL 3: 0.20 g/100mL - LOT# FN03211401 - EXP 06/2019

n-PROPANOL ISTD - LOT# P1114 - EXP 02/20/2015

Vials# 1-9 are filed with 15004

Sequence Table (Front Injector):

Method and Injection Info Part:

| Line | Location | SampleName | Method | Inj | SampleType | InjVolume | DataFile |
|------|----------|-----------------|---------|-----|------------|-----------|----------|
| 1 | Vial 1 | BLANK | SIMALC3 | 1 | Sample | | |
| 2 | Vial 2 | CAL 1 (0.079) | SIMALC3 | 1 | Calib | | |
| 3 | Vial 3 | CAL 2 (0.158) | SIMALC3 | 1 | Calib | | |
| 4 | Vial 4 | CAL 3 (0.316) | SIMALC3 | 1 | Calib | | |
| 5 | Vial 5 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 6 | Vial 6 | CTRL 1 (0.04) | SIMALC3 | 1 | Ctrl Samp | | |
| 7 | Vial 7 | CTRL 2 (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 8 | Vial 8 | CTRL 3 (0.20) | SIMALC3 | 1 | Ctrl Samp | | |
| 9 | Vial 9 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 10 | Vial 10 | 15004 #1 | SIMALC3 | 1 | Sample | | |
| 11 | Vial 11 | 15004 #2 | SIMALC3 | 1 | Sample | | |
| 12 | Vial 12 | 15004 #3 | SIMALC3 | 1 | Sample | | |
| 13 | Vial 13 | 15004 #4 | SIMALC3 | 1 | Sample | | |
| 14 | Vial 14 | 15004 #5 | SIMALC3 | 1 | Sample | | |
| 15 | Vial 15 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 16 | Vial 16 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 17 | Vial 17 | 15005 #1 | SIMALC3 | 1 | Sample | | |
| 18 | Vial 18 | 15005 #2 | SIMALC3 | 1 | Sample | | |
| 19 | Vial 19 | 15005 #3 | SIMALC3 | 1 | Sample | | |
| 20 | Vial 20 | 15005 #4 | SIMALC3 | 1 | Sample | | |
| 21 | Vial 21 | 15005 #5 | SIMALC3 | 1 | Sample | | |
| 22 | Vial 22 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 23 | Vial 23 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 24 | Vial 24 | 15006 #1 | SIMALC3 | 1 | Sample | | |

15008

fn/2/15

fr

EW

| Line | Location | SampleName | Method | Inj | SampleType | InjVolume | DataFile |
|------|----------|-----------------|---------|-----|------------|-----------|----------|
| 25 | Vial 25 | 15006 #2 | SIMALC3 | 1 | Sample | | |
| 26 | Vial 26 | 15006 #3 | SIMALC3 | 1 | Sample | | |
| 27 | Vial 27 | 15006 #4 | SIMALC3 | 1 | Sample | | |
| 28 | Vial 28 | 15006 #5 | SIMALC3 | 1 | Sample | | |
| 29 | Vial 29 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 30 | Vial 30 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 31 | Vial 31 | 15007 #1 | SIMALC3 | 1 | Sample | | |
| 32 | Vial 32 | 15007 #2 | SIMALC3 | 1 | Sample | | |
| 33 | Vial 33 | 15007 #3 | SIMALC3 | 1 | Sample | | |
| 34 | Vial 34 | 15007 #4 | SIMALC3 | 1 | Sample | | |
| 35 | Vial 35 | 15007 #5 | SIMALC3 | 1 | Sample | | |
| 36 | Vial 36 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 37 | Vial 37 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 38 | Vial 38 | 15008 #1 | SIMALC3 | 1 | Sample | | |
| 39 | Vial 39 | 15008 #2 | SIMALC3 | 1 | Sample | | |
| 40 | Vial 40 | 15008 #3 | SIMALC3 | 1 | Sample | | |
| 41 | Vial 41 | 15008 #4 | SIMALC3 | 1 | Sample | | |
| 42 | Vial 42 | 15008 #5 | SIMALC3 | 1 | Sample | | |
| 43 | Vial 43 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 44 | Vial 44 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |

Calibration Part:

| Line | Location | SampleName | Method | CalLev | Update | RF | Update | RT | Interval |
|------|----------|---------------|---------|--------|---------|----|---------|----|----------|
| 2 | Vial 2 | CAL 1 (0.079) | SIMALC3 | 1 | Replace | | Replace | | |
| 3 | Vial 3 | CAL 2 (0.158) | SIMALC3 | 2 | Replace | | Replace | | |
| 4 | Vial 4 | CAL 3 (0.316) | SIMALC3 | 3 | Replace | | Replace | | |

Sequence Table (Back Injector):

No entries - empty table!

15008
Jan/27/15

fr

EW

Inj. Date: 1/13/2015 1:03:27 PM

Sample Name: 15008 #1

Instrument: HSGC#3


Operator: Elizabeth Wehner

Column: DB-ALC2


Location: Vial 38

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

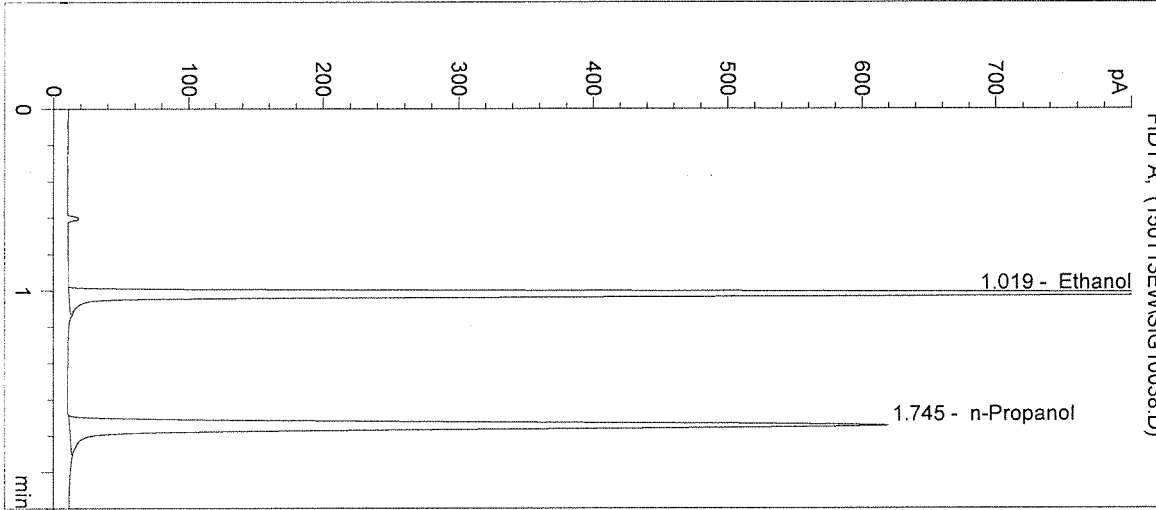

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1906 | 1.019 |
| 2 | n-Propanol | 1626 | 1.745 |

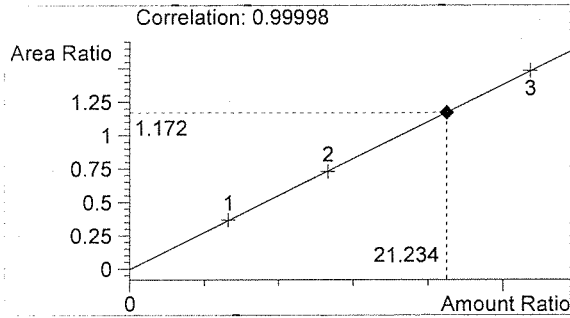

Ethanol 0.255 g/100mL

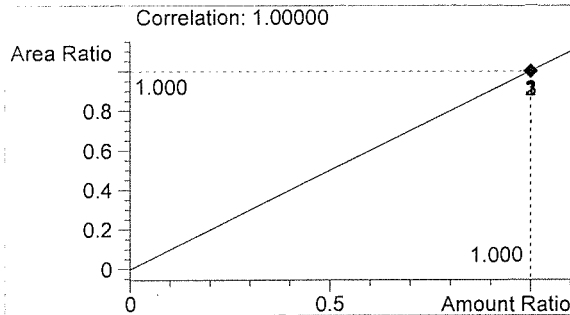

n-Propanol 0.012 g/100mL

EW

EW

Inj. Date: 1/13/2015 1:06:39 PM

Sample Name: 15008 #2

Instrument: HSGC#3


Operator: Elizabeth Wehner

Column: DB-ALC2


Location: Vial 39

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

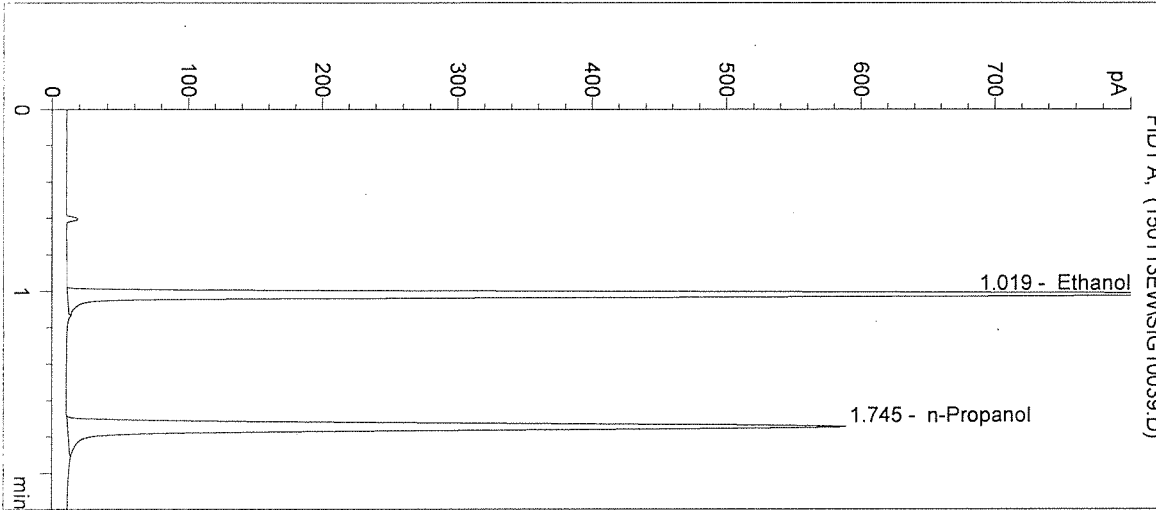

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1801 | 1.019 |
| 2 | n-Propanol | 1542 | 1.745 |

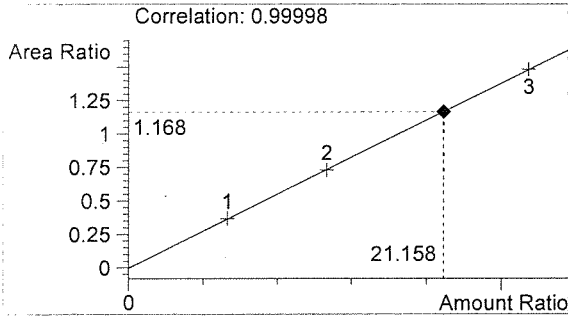

Ethanol 0.254 g/100mL

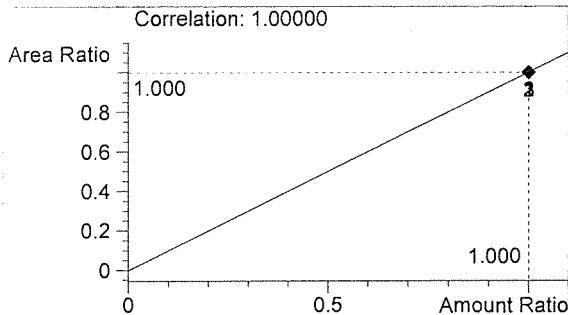

n-Propanol 0.012 g/100mL

Jr

EW

Inj. Date: 1/13/2015 1:09:53 PM

Sample Name: 15008 #3

Instrument: HSGC#3


Operator: Elizabeth Wehner

Column: DB-ALC2


Location: Vial 40

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

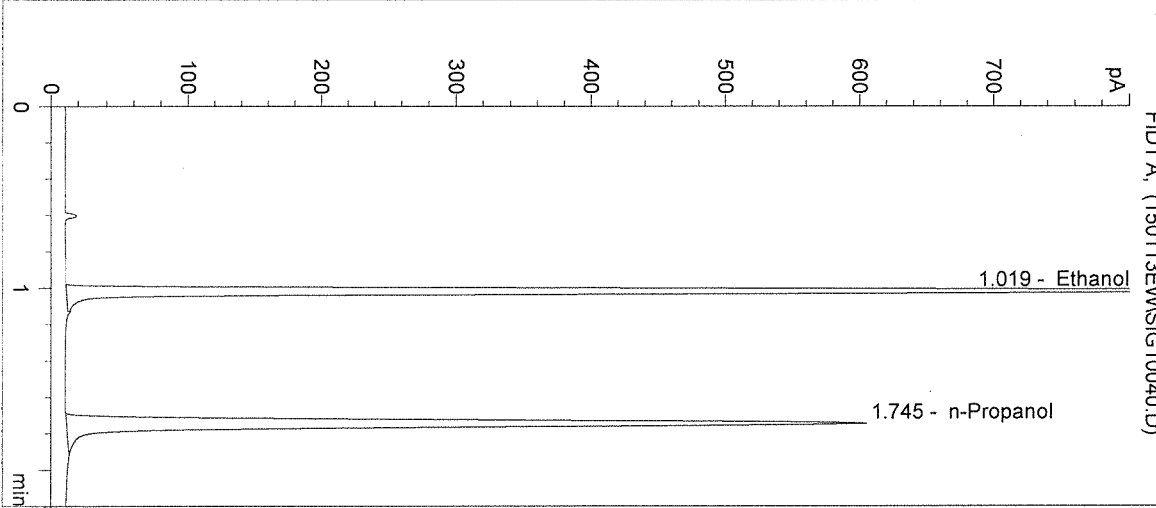

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1860 | 1.019 |
| 2 | n-Propanol | 1585 | 1.745 |

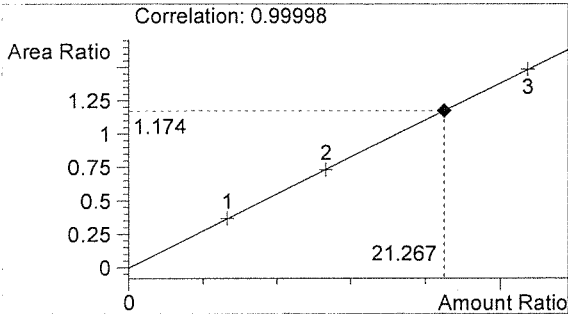

Ethanol 0.255 g/100mL

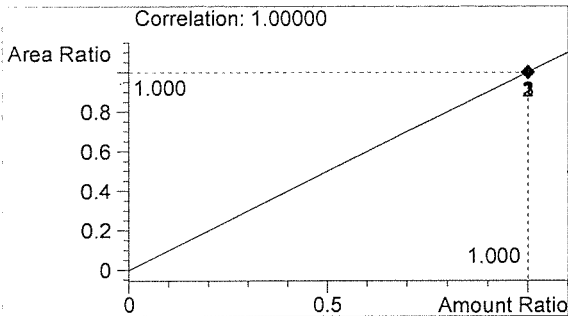

n-Propanol 0.012 g/100mL

f

EW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/13/2015 1:13:07 PM

Sample Name: 15008 #4

Instrument: HSGC#3


Operator: Elizabeth Wehner

Column: DB-ALC2


Location: Vial 41

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

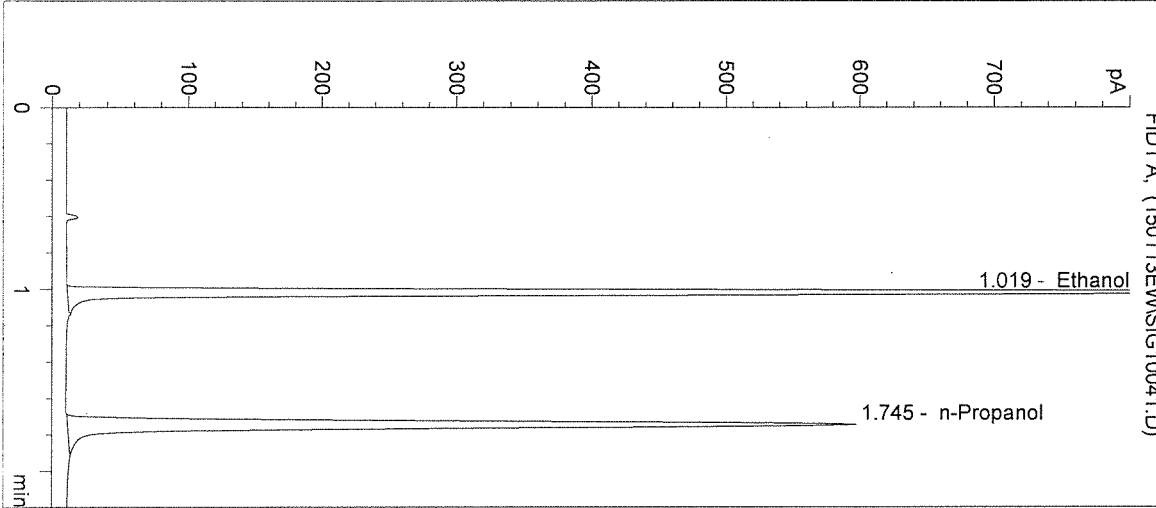

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1841 | 1.019 |
| 2 | n-Propanol | 1570 | 1.745 |

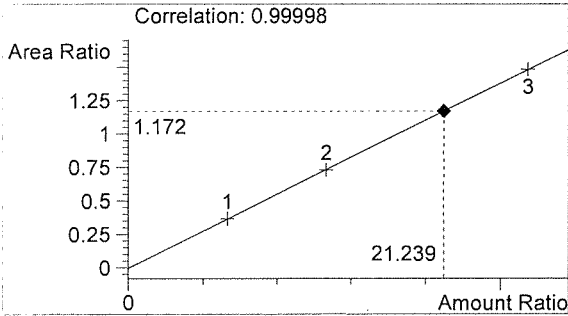

Ethanol 0.255 g/100mL

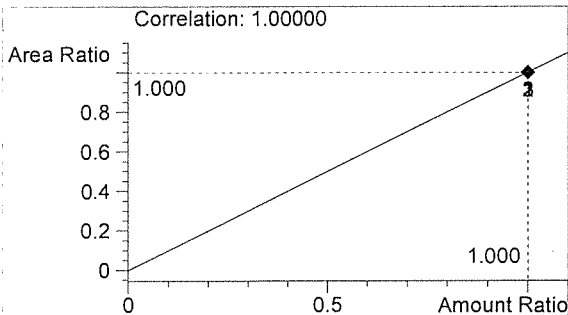

n-Propanol 0.012 g/100mL

EW

EW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/13/2015 1:16:20 PM

Sample Name: 15008 #5

Instrument: HSGC#3


Operator: Elizabeth Wehner

Column: DB-ALC2


Location: Vial 42

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

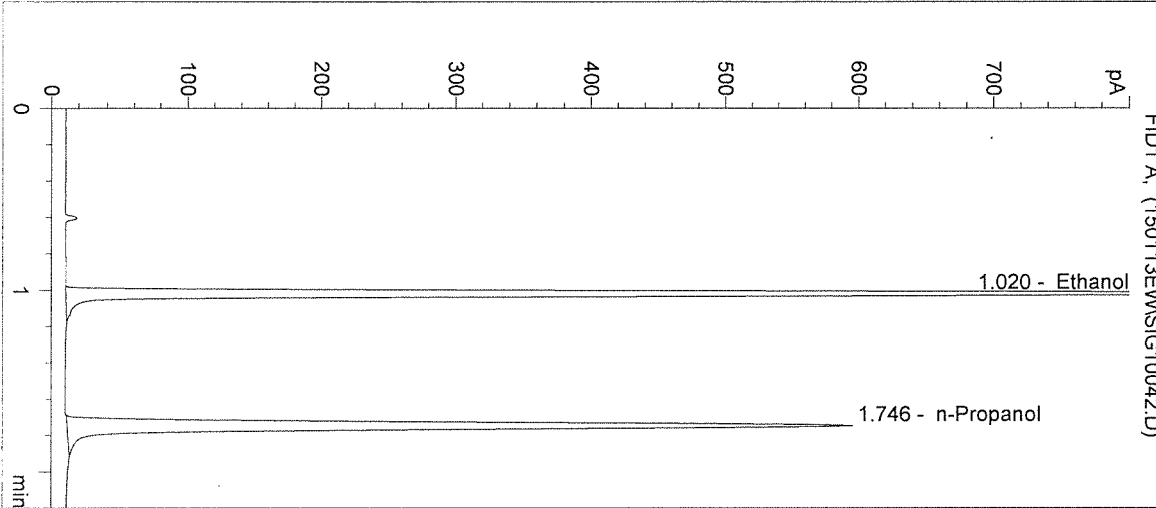

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1849 | 1.020 |
| 2 | n-Propanol | 1562 | 1.746 |

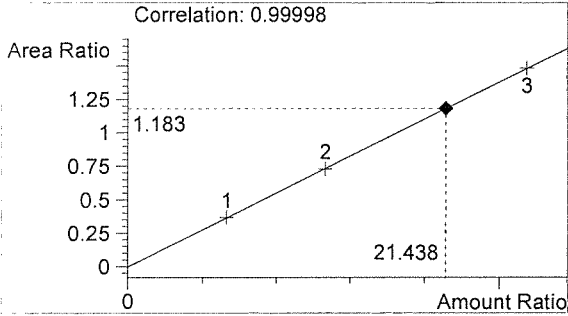

Ethanol 0.257 g/100mL

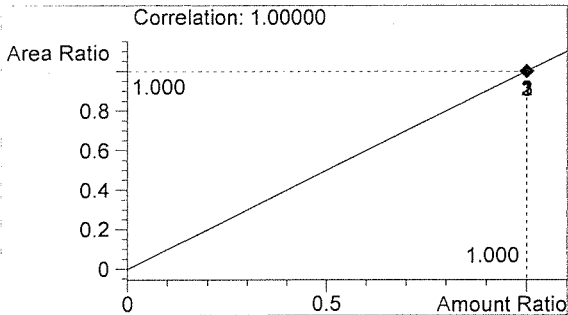

n-Propanol 0.012 g/100mL

EW

EW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/13/2015 1:19:32 PM

Sample Name: POS CTRL (0.10)

Instrument: HSGC#3

Operator: Elizabeth Wehner


Column: DB-ALC2

Location: Vial 43


Method: C:\HPCHEM\2\METHODS\SIMALC3.M

Sample Info: POS CTRL: 0.10 g/100mL
 15008


->

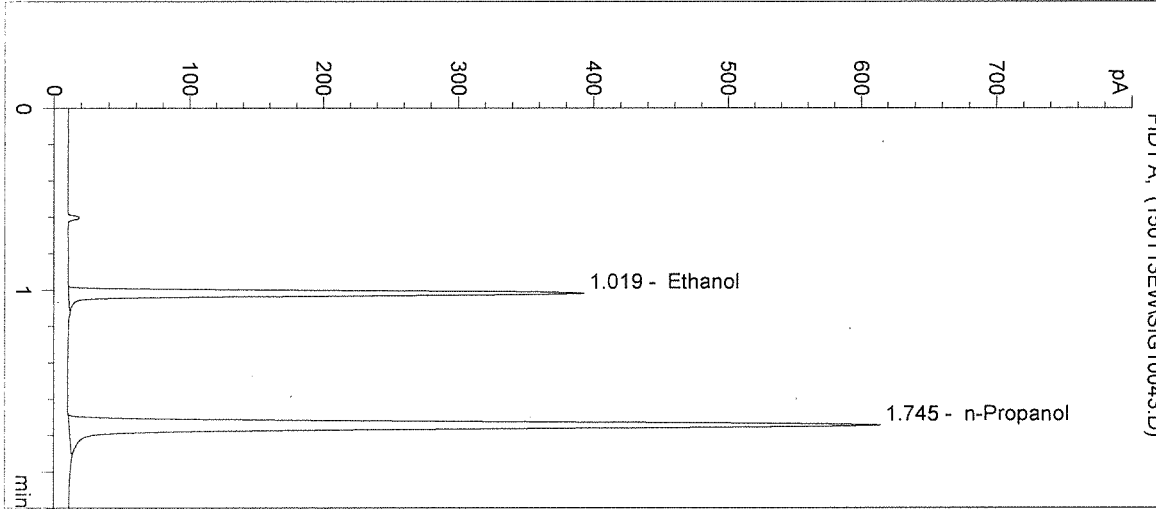

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 769 | 1.019 |
| 2 | n-Propanol | 1620 | 1.745 |

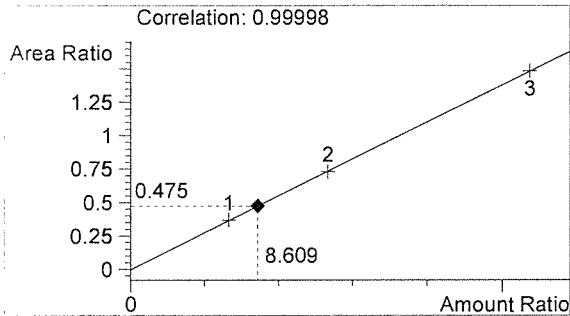

Ethanol 0.103 g/100mL

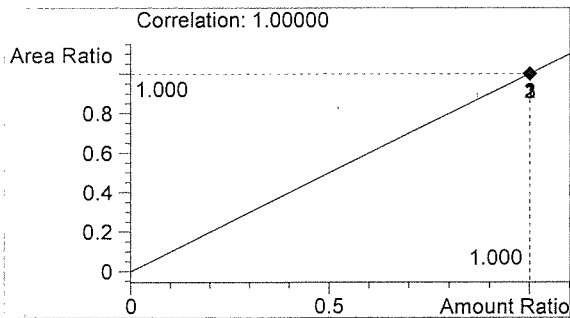

n-Propanol 0.012 g/100mL

EW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/13/2015 1:22:46 PM

Sample Name: NEG CTRL

Instrument: HSGC#3


Operator: Elizabeth Wehner

Column: DB-ALC2


Location: Vial 44

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info: 15008

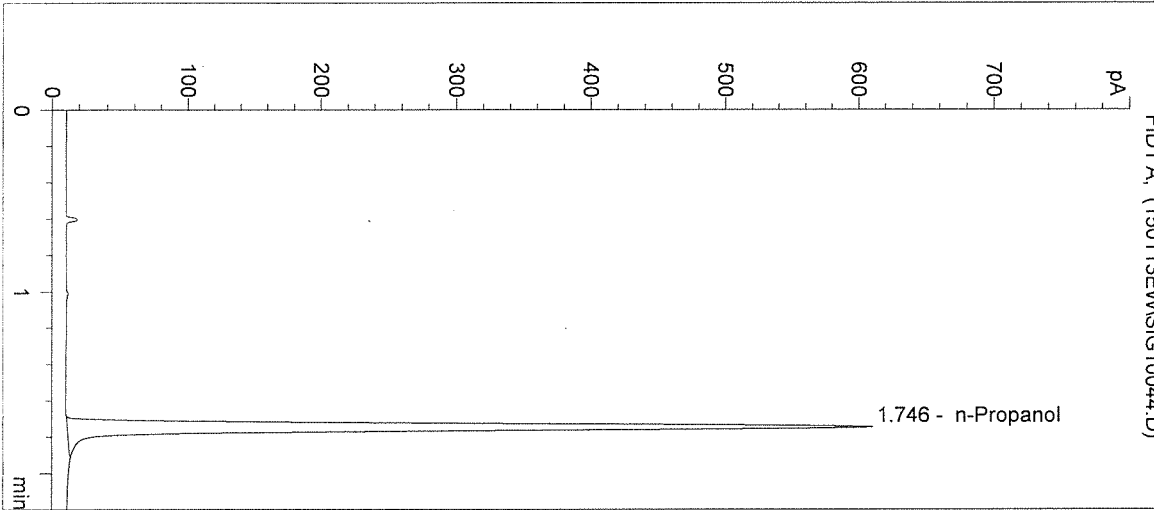

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 0 | 0.000 |
| 2 | n-Propanol | 1608 | 1.746 |

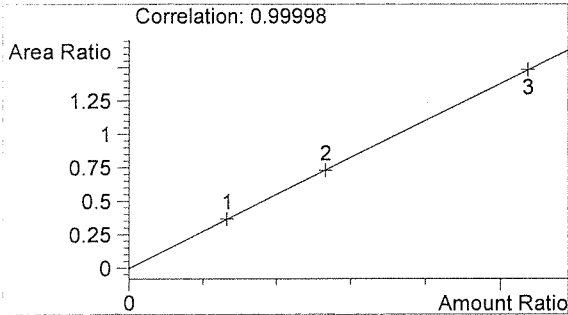

Ethanol 0.000 g/100mL

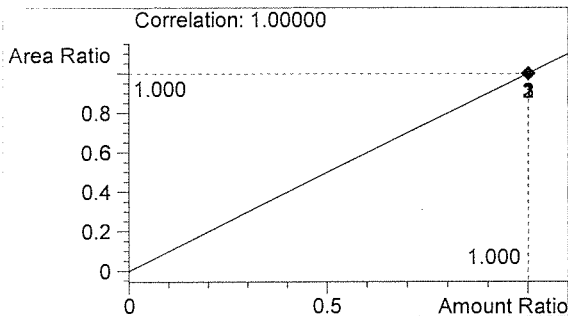

n-Propanol 0.012 g/100mL

fr

EW

Sequence Parameters:

Operator: David Nguyen
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\2\DATA\
 Data Subdirectory: 150114D1
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

CAL 1: 0.079 g/100mL - Lot#: E0814-01 Exp. 02/19/2015
 CAL 2: 0.158 g/100mL - Lot#: E0814-02 Exp. 02/19/2015
 CAL 3: 0.316 g/100mL - Lot#: E0814-03 Exp. 02/19/2015

CTRL 1: 0.04 g/100mL - Lot#: FN05011301 Exp. 05/2018
 CTRL 2: 0.10 g/100mL - Lot#: FN08051301 Exp. 10/2018
 CTRL 3: 0.20 g/100mL - Lot#: FN03211401 Exp. 06/2019

n-Propanol ISTD - Lot#: P1114 Exp. 02/20/2015

Calibration vials 1-9 filed with 15008.

Sequence Table (Front Injector):

Method and Injection Info Part:

| Line | Location | SampleName | Method | Inj | SampleType | InjVolume | DataFile |
|------|----------|-----------------|---------|-----|------------|-----------|----------|
| 1 | Vial 1 | BLANK | SIMALC3 | 1 | Sample | | |
| 2 | Vial 2 | CAL 1 (0.079) | SIMALC3 | 1 | Calib | | |
| 3 | Vial 3 | CAL 2 (0.158) | SIMALC3 | 1 | Calib | | |
| 4 | Vial 4 | CAL 3 (0.316) | SIMALC3 | 1 | Calib | | |
| 5 | Vial 5 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 6 | Vial 6 | CTRL 1 (0.04) | SIMALC3 | 1 | Ctrl Samp | | |
| 7 | Vial 7 | CTRL 2 (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 8 | Vial 8 | CTRL 3 (0.20) | SIMALC3 | 1 | Ctrl Samp | | |
| 9 | Vial 9 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 10 | Vial 10 | 15008 #1 | SIMALC3 | 1 | Sample | | |
| 11 | Vial 11 | 15008 #2 | SIMALC3 | 1 | Sample | | |
| 12 | Vial 12 | 15008 #3 | SIMALC3 | 1 | Sample | | |
| 13 | Vial 13 | 15008 #4 | SIMALC3 | 1 | Sample | | |
| 14 | Vial 14 | 15008 #5 | SIMALC3 | 1 | Sample | | |
| 15 | Vial 15 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 16 | Vial 16 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |

15008
Initials

Calibration Part:

| Line | Location | SampleName | Method | CalLev | Update | RF | Update | RT | Interval |
|------|----------|---------------|---------|--------|---------|----|---------|----|----------|
| 2 | Vial 2 | CAL 1 (0.079) | SIMALC3 | 1 | Replace | | Replace | | |

DN

| Line | Location | SampleName | Method | CalLev | Update RF | Update RT | Interval |
|------|----------|---------------|---------|--------|-----------|-----------|----------|
| 3 | Vial 3 | CAL 2 (0.158) | SIMALC3 | 2 | Replace | Replace | |
| 4 | Vial 4 | CAL 3 (0.316) | SIMALC3 | 3 | Replace | Replace | |

Sequence Table (Back Injector):

No entries - empty table!

15008
m/2/15

fu

DN

=====
Calibration Table
=====

Calib. Data Modified : Wednesday, January 14, 2015 2:39:09 PM
Calculate : Internal Standard
Based on : Peak Area
Rel. Reference Window : 5.000 %
Abs. Reference Window : 0.050 min
Rel. Non-ref. Window : 5.000 %
Abs. Non-ref. Window : 0.050 min
Multiplier : 1.0000
Dilution : 1.0000
Sample Amount : 0.00000
Use Multiplier & Dilution Factor with ISTDs
Uncalibrated Peaks : not reported
Partial Calibration : No recalibration if peaks missing
Curve Type : Linear
Origin : Included
Weight : Equal
Recalibration Settings:
Average Response : No Update
Average Retention Time: No Update

Calibration Report Options :
Printout of recalibrations within a sequence:
Normal Report after Recalibration

Sample ISTD Information:

| ISTD # | ISTD Amount [g/100mL] | Name |
|--------|-----------------------|------------|
| 1 | 1.20000e-2 | n-Propanol |

Signal 1: FID1 A,

| RetTime [min] | Lvl Sig | Amount [g/100mL] | Area | Amt/Area | Ref Grp Name |
|---------------|---------|------------------|------------|------------|---------------|
| 1.019 | 1 1 | 7.95500e-2 | 664.52954 | 1.19709e-4 | 1 Ethanol |
| | | 2 1.59740e-1 | 1190.13892 | 1.34220e-4 | |
| | | 3 3.21980e-1 | 2512.08325 | 1.28173e-4 | |
| 1.745 | 1 1 | 1.20000e-2 | 1775.50073 | 6.75866e-6 | I1 n-Propanol |
| | | 2 1.20000e-2 | 1603.26538 | 7.48472e-6 | |
| | | 3 1.20000e-2 | 1666.61804 | 7.20021e-6 | |

=====
Peak Sum Table
=====

No Entries in table
=====


15008

frutzelis


fr

DN

=====
Calibration Curves
=====

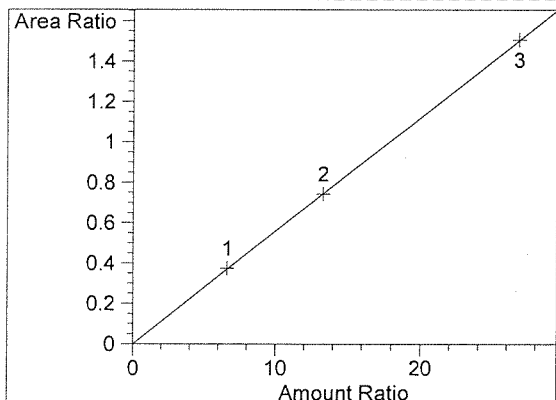

Ethanol at exp. RT: 1.019
FID1 A,
Correlation: 0.99999
Residual Std. Dev.: 0.00383
Formula: $y = mx + b$
m: 5.61293e-2
b: -3.54087e-4
x: Amount Ratio
y: Area Ratio

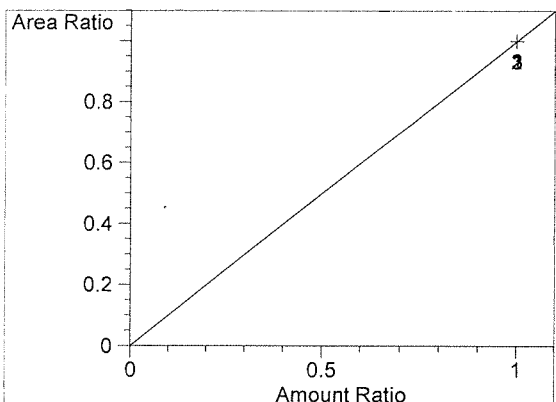

n-Propanol at exp. RT: 1.745
FID1 A,
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio


15008
Jan/27/15

Handwritten signature


DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:27:04 PM Sample Name: BLANK
Instrument: HSGC#3 Operator: David Nguyen
Column: DB-ALC2 Location: Vial 1
Method: C:\HPCHEM\2\METHODS\SIMALC3.M
Sample Info: 15008

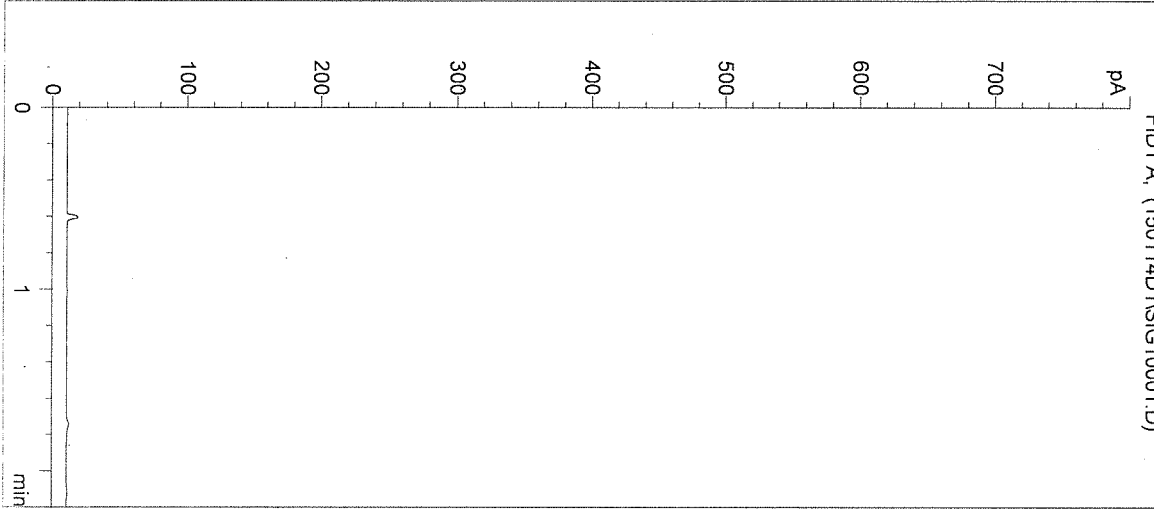

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 0 | 0.000 |
| 2 | n-Propanol | 0 | 0.000 |

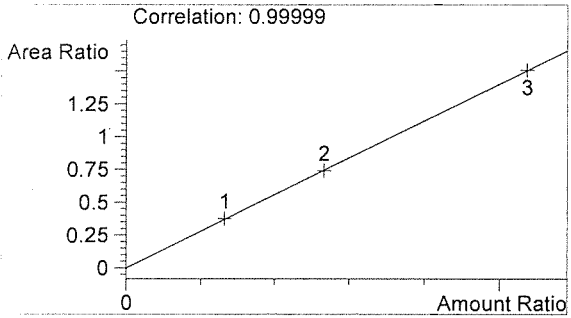

Ethanol 0.000 g/100mL




n-Propanol 0.000 g/100mL

fu


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:30:23 PM Sample Name: CAL 1 (0.079)
 Instrument: HSGC#3 Operator: David Nguyen
 Column: DB-ALC2 Location: Vial 2
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: CAL 1: 0.079 g/100mL
 15008

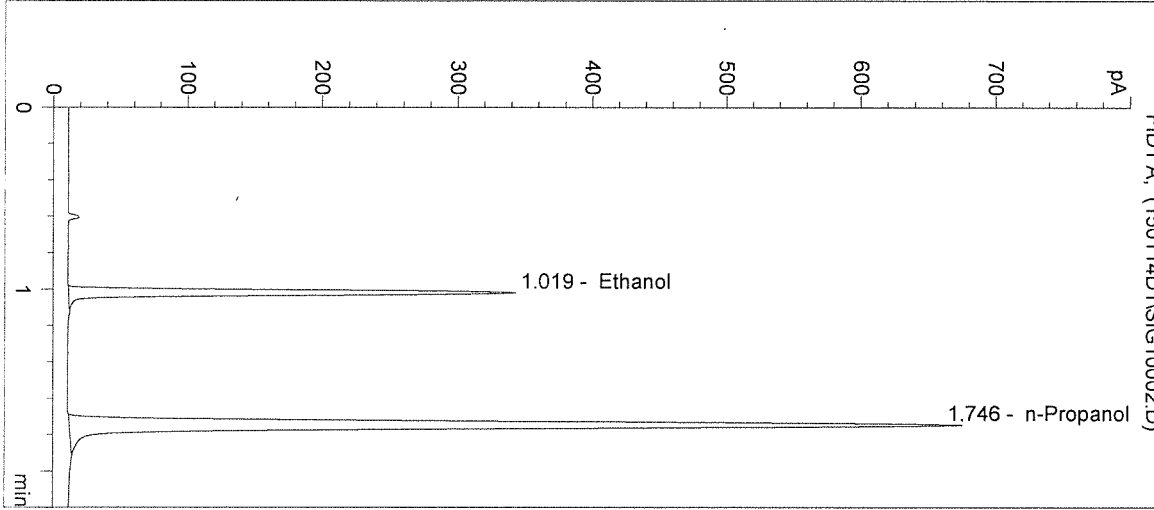

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 665 | 1.019 |
| 2 | n-Propanol | 1776 | 1.746 |



Ethanol 0.080 g/100mL




n-Propanol 0.012 g/100mL


Handwritten initials/signature
 DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:33:40 PM Sample Name: CAL 2 (0.158)
 Instrument: HSGC#3 Operator: David Nguyen
 Column: DB-ALC2 Location: Vial 3
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: CAL 2: 0.158 g/100mL
 15008

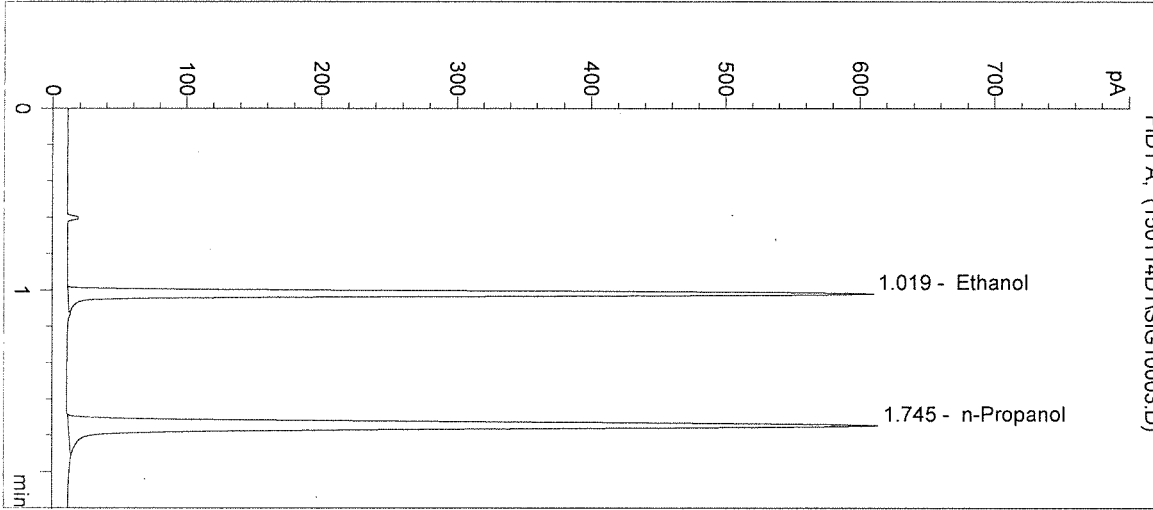

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1190 | 1.019 |
| 2 | n-Propanol | 1603 | 1.745 |

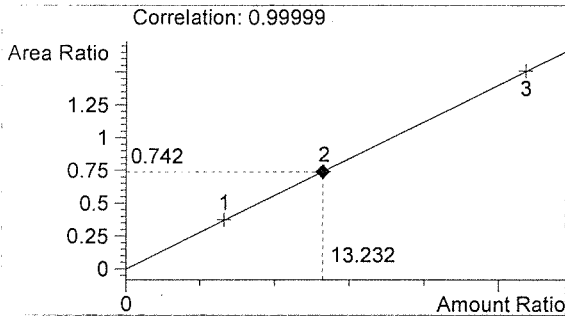

Ethanol 0.159 g/100mL

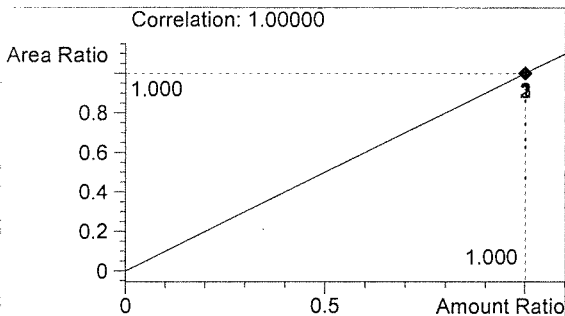


n-Propanol 0.012 g/100mL

fn


DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:36:57 PM Sample Name: CAL 3 (0.316)
Instrument: HSGC#3 Operator: David Nguyen
Column: DB-ALC2 Location: Vial 4
Method: C:\HPCHEM\2\METHODS\SIMALC3.M
Sample Info: CAL 3: 0.316 g/100mL
15008

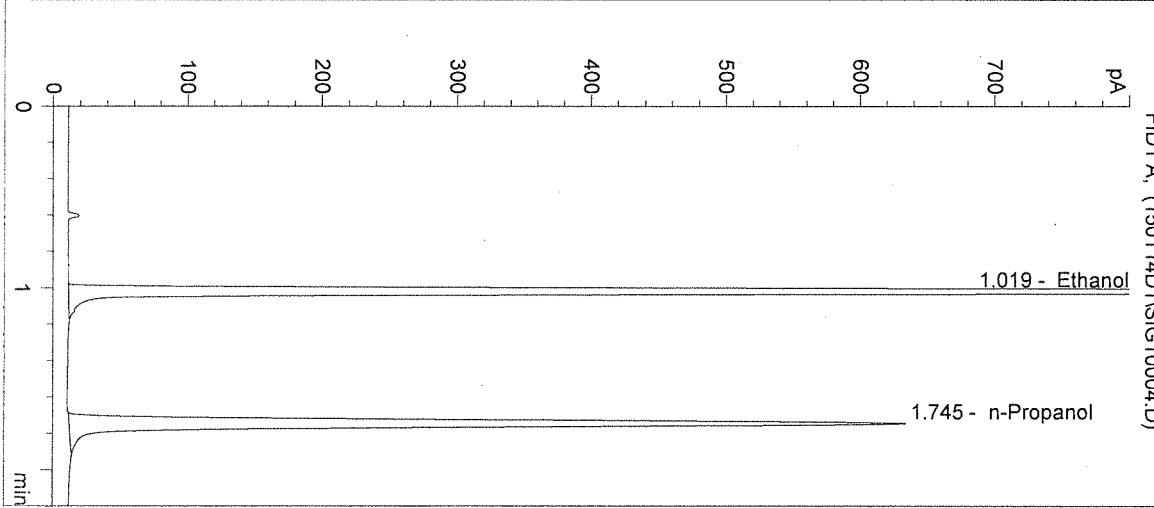

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 2512 | 1.019 |
| 2 | n-Propanol | 1667 | 1.745 |



Ethanol 0.322 g/100mL




n-Propanol 0.012 g/100mL


h
DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:40:11 PM Sample Name: NEG CTRL
Instrument: HSGC#3 Operator: David Nguyen
Column: DB-ALC2 Location: Vial 5
Method: C:\HPCHEM\2\METHODS\SIMALC3.M
Sample Info: 15008

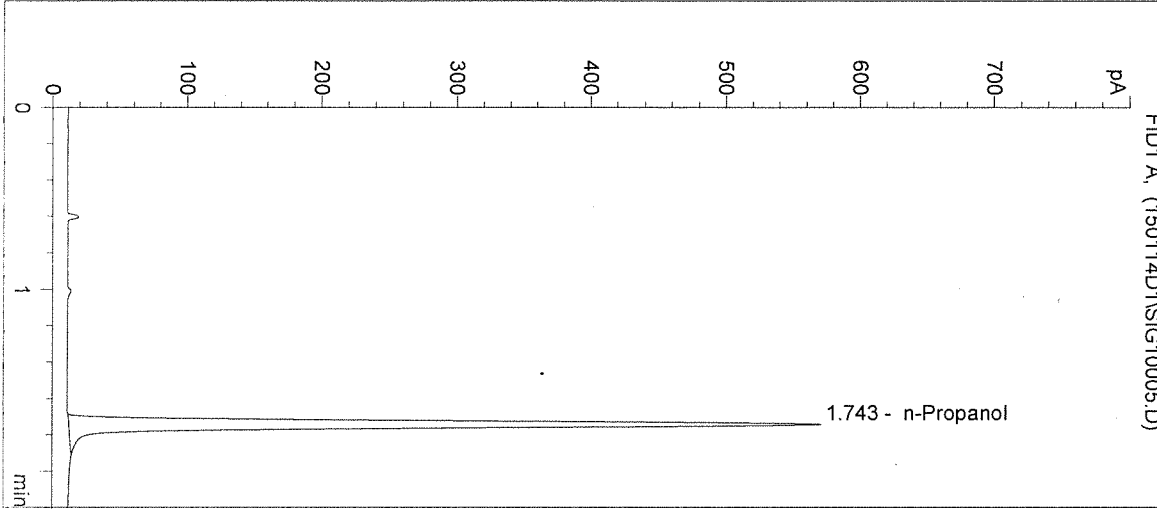

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 0 | 0.000 |
| 2 | n-Propanol | 1494 | 1.743 |



Ethanol 0.000 g/100mL



n-Propanol 0.012 g/100mL

fr


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:43:24 PM
 Instrument: HSGC#3
 Column: DB-ALC2
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: CTRL 1: 0.04 g/100mL
 15008

Sample Name: CTRL 1 (0.04)
 Operator: David Nguyen
 Location: Vial 6


->

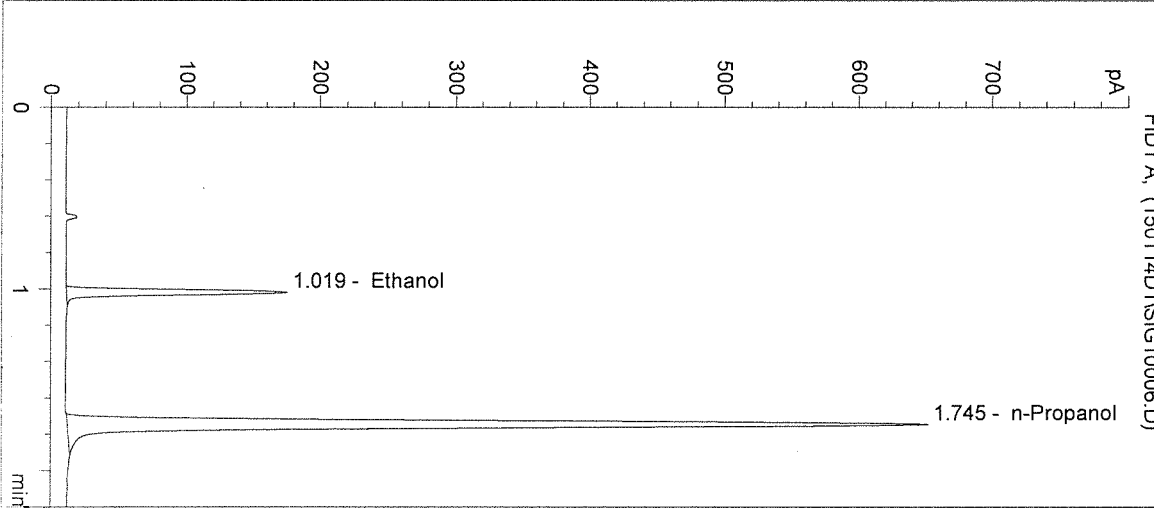

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 325 | 1.019 |
| 2 | n-Propanol | 1709 | 1.745 |

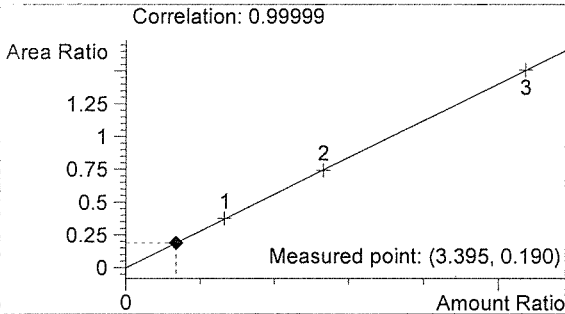


Ethanol 0.041 g/100mL

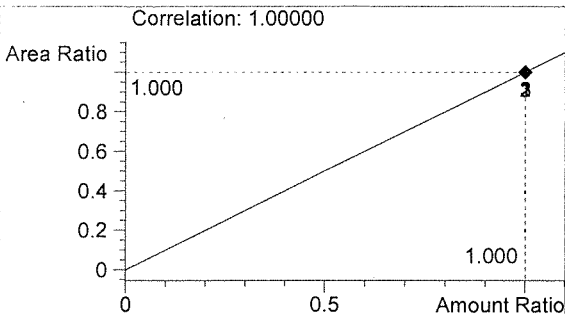


n-Propanol 0.012 g/100mL

DN


Inj. Date: 1/14/2015 2:46:37 PM Sample Name: CTRL 2 (0.10)
 Instrument: HSGC#3 Operator: David Nguyen
 Column: DB-ALC2 Location: Vial 7
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: CTRL 2: 0.10 g/100mL
 15008

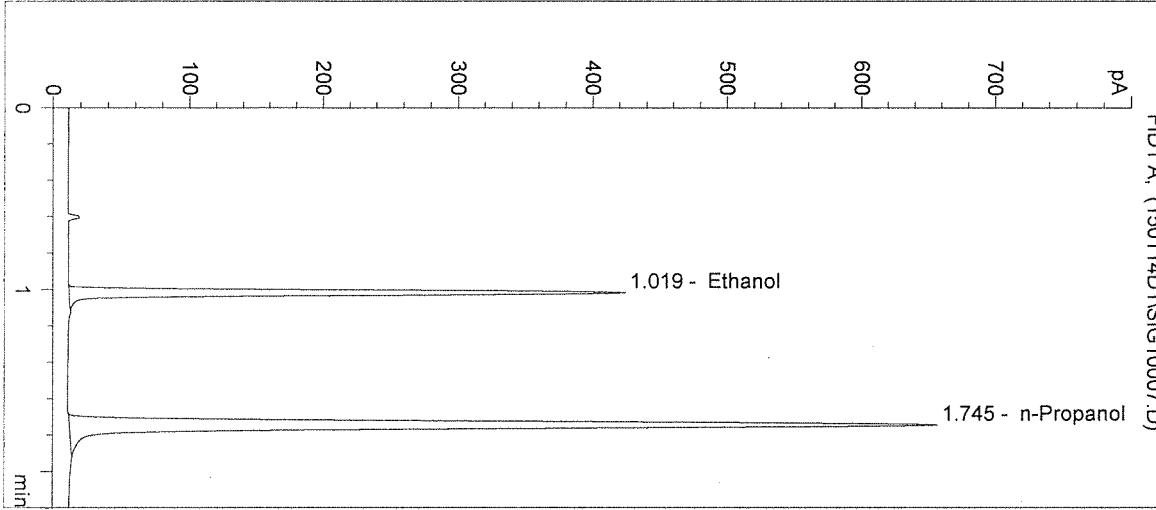

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 820 | 1.019 |
| 2 | n-Propanol | 1721 | 1.745 |

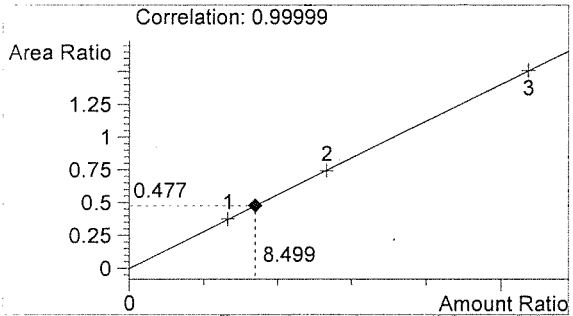

Ethanol 0.102 g/100mL

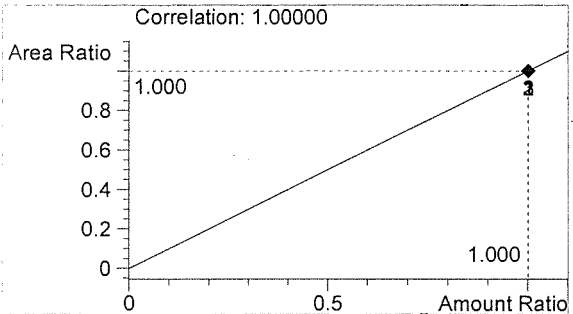


n-Propanol 0.012 g/100mL

DN


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 2:49:50 PM Sample Name: CTRL 3 (0.20)
 Instrument: HSGC#3 Operator: David Nguyen
 Column: DB-ALC2 Location: Vial 8
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: CTRL 3: 0.20 g/100mL
 15008


->

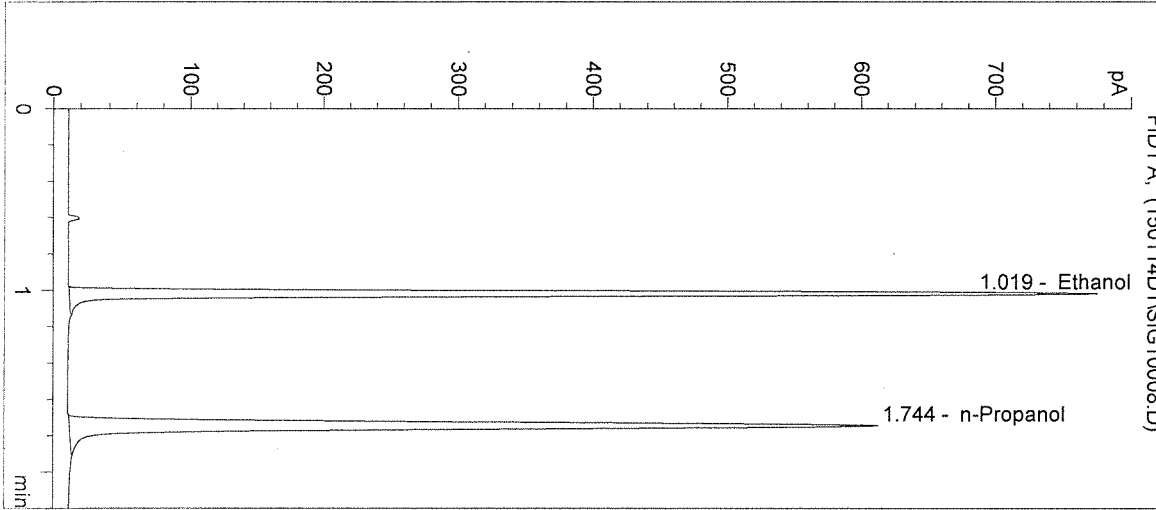

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1519 | 1.019 |
| 2 | n-Propanol | 1599 | 1.744 |

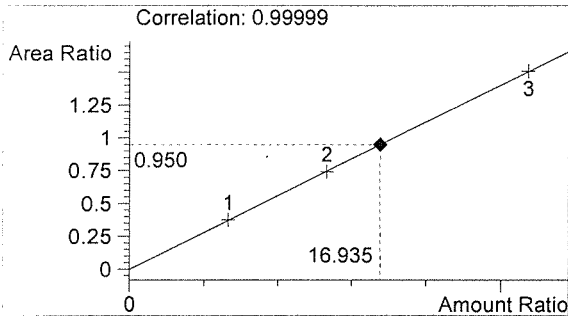

Ethanol 0.203 g/100mL

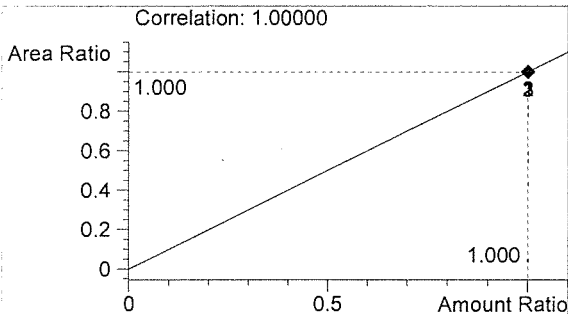


n-Propanol 0.012 g/100mL


Ju
 DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:53:04 PM Sample Name: NEG CTRL
Instrument: HSGC#3 Operator: David Nguyen
Column: DB-ALC2 Location: Vial 9
Method: C:\HPCHEM\2\METHODS\SIMALC3.M
Sample Info: 15008

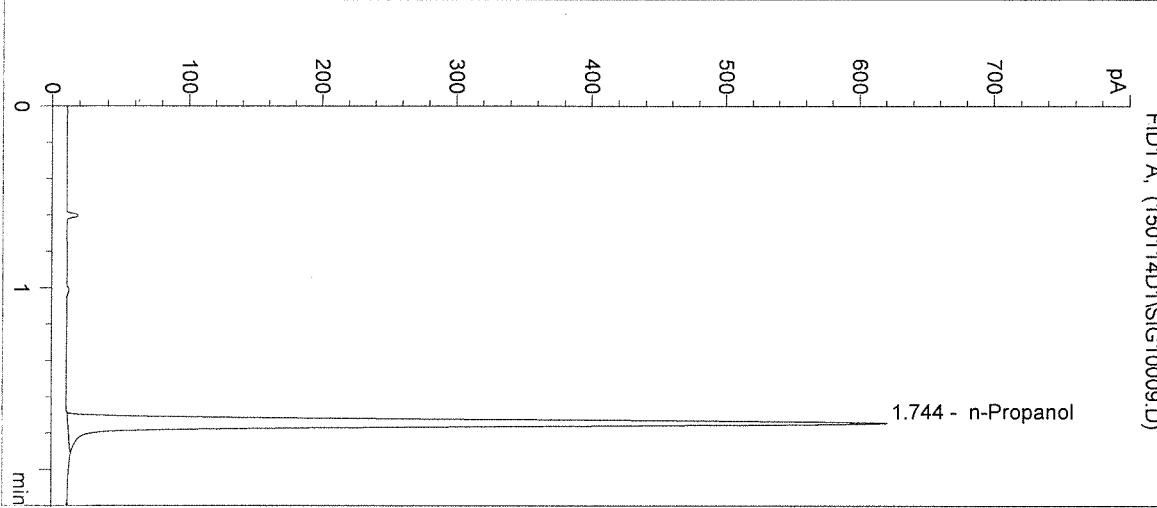

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 0 | 0.000 |
| 2 | n-Propanol | 1624 | 1.744 |

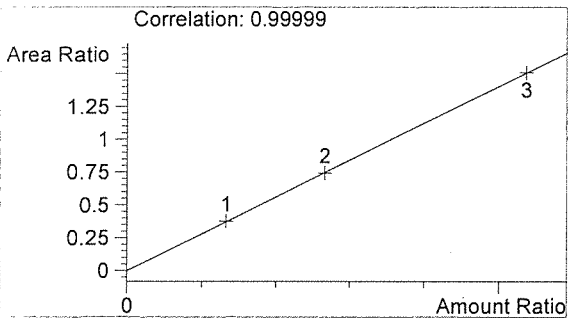

Ethanol 0.000 g/100mL

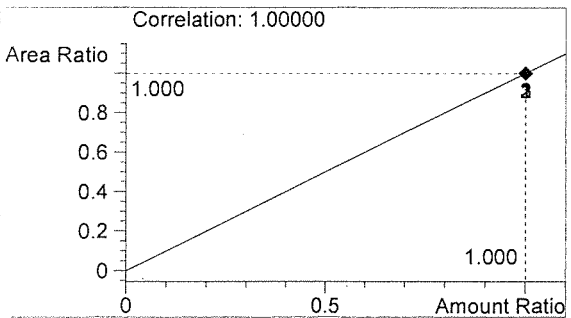


n-Propanol 0.012 g/100mL


for
DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 2:56:18 PM Sample Name: 15008 #1
Instrument: HSGC#3 Operator: David Nguyen
Column: DB-ALC2 Location: Vial 10
Method: C:\HPCHEM\2\METHODS\SIMALC3.M
Sample Info:

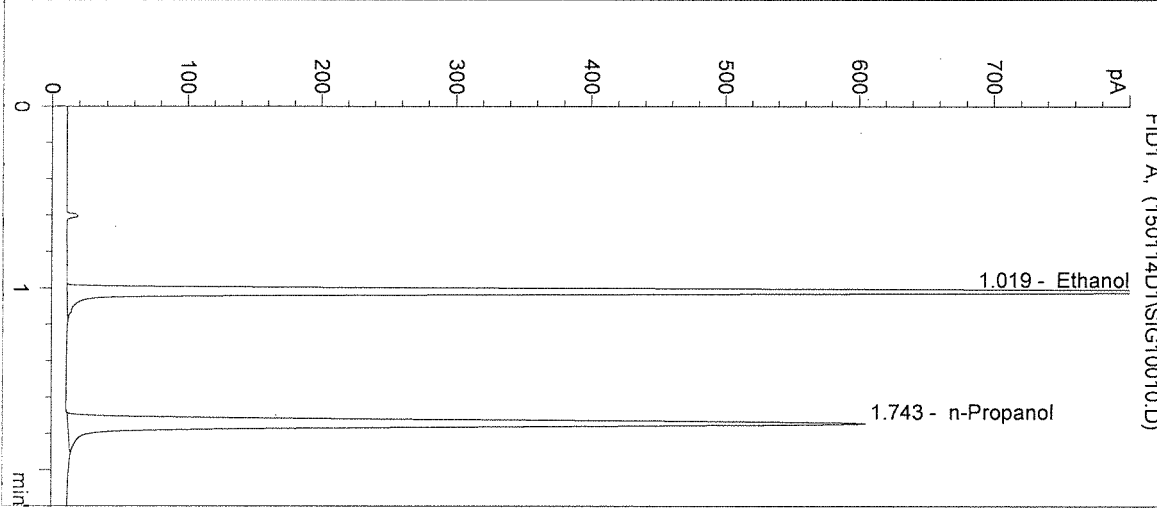

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1841 | 1.019 |
| 2 | n-Propanol | 1580 | 1.743 |

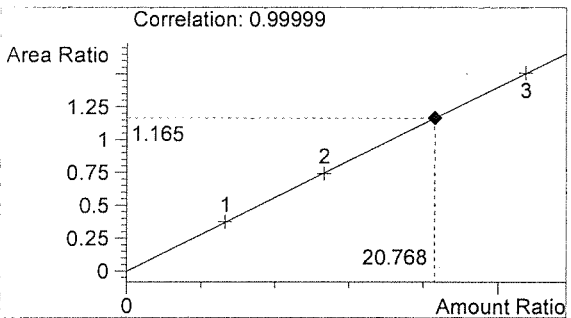

Ethanol 0.249 g/100mL

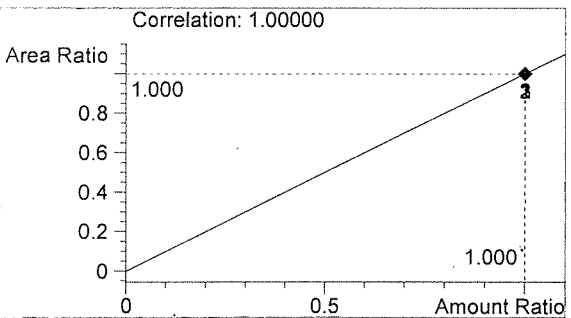

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 2:59:29 PM

Sample Name: 15008 #2

Instrument: HSGC#3


Operator: David Nguyen

Column: DB-ALC2


Location: Vial 11

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

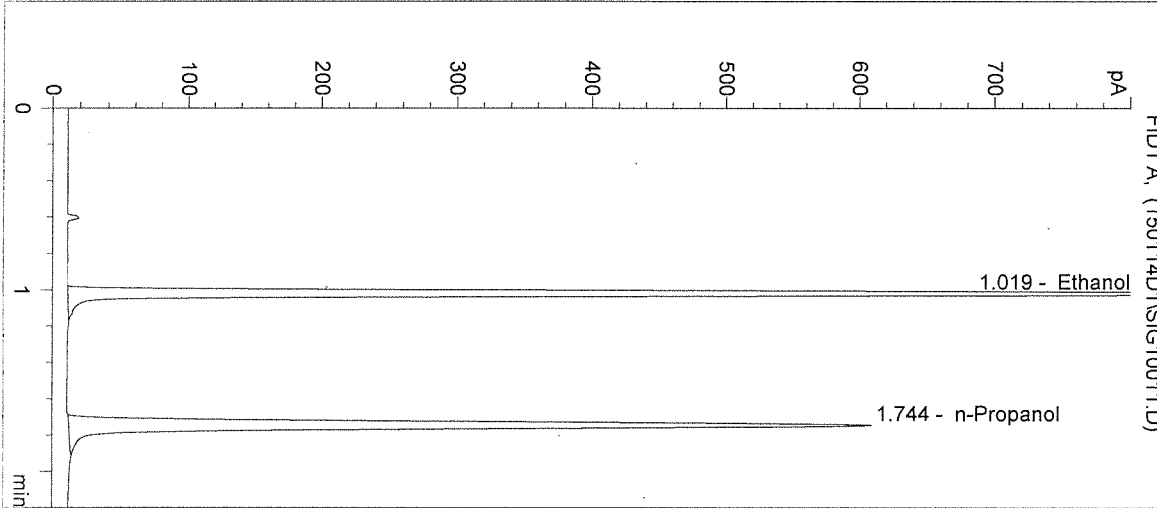

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1867 | 1.019 |
| 2 | n-Propanol | 1592 | 1.744 |

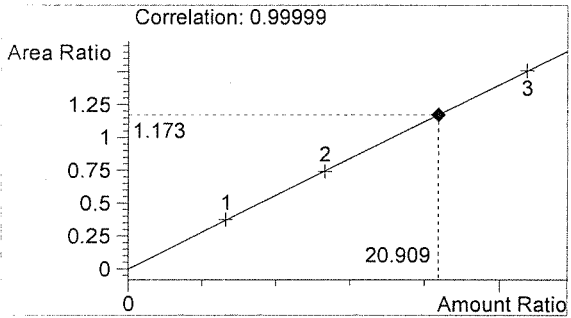

Ethanol 0.251 g/100mL



n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 3:02:42 PM

Sample Name: 15008 #3

Instrument: HSGC#3


Operator: David Nguyen

Column: DB-ALC2


Location: Vial 12

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

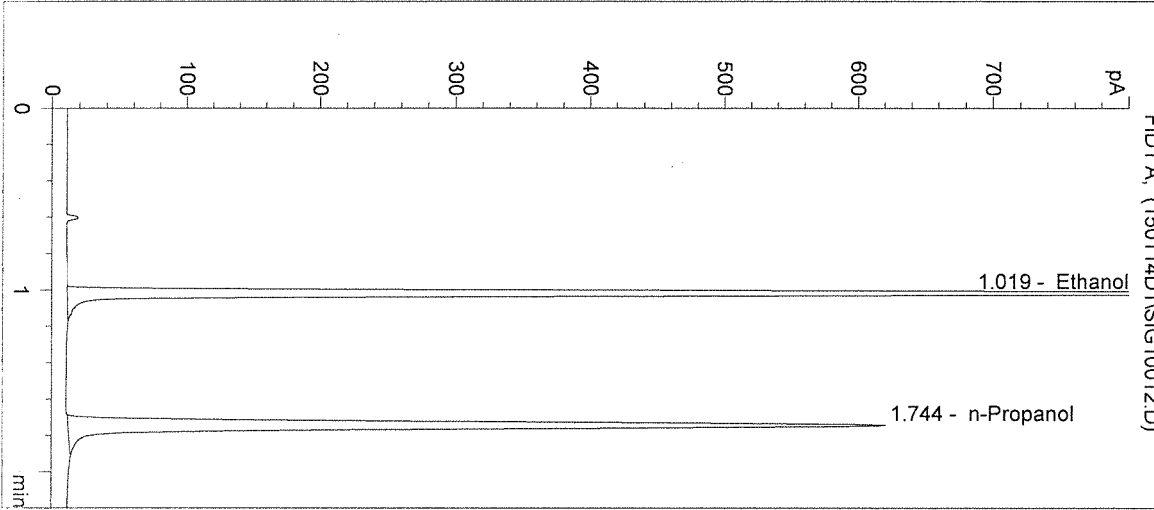

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1910 | 1.019 |
| 2 | n-Propanol | 1624 | 1.744 |

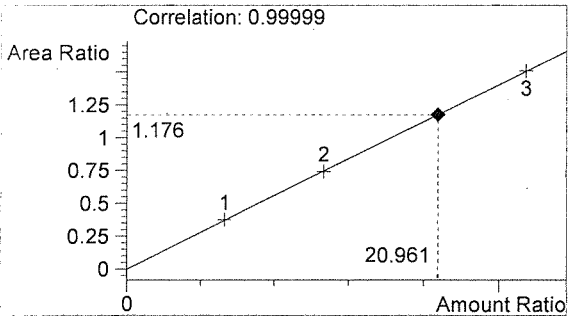

Ethanol 0.252 g/100mL

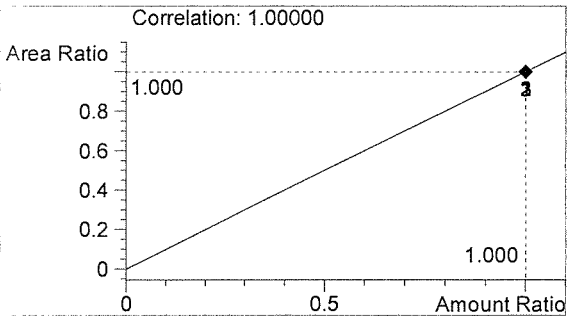

n-Propanol 0.012 g/100mL

Ju
DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 3:05:55 PM

Sample Name: 15008 #4

Instrument: HSGC#3


Operator: David Nguyen

Column: DB-ALC2


Location: Vial 13

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

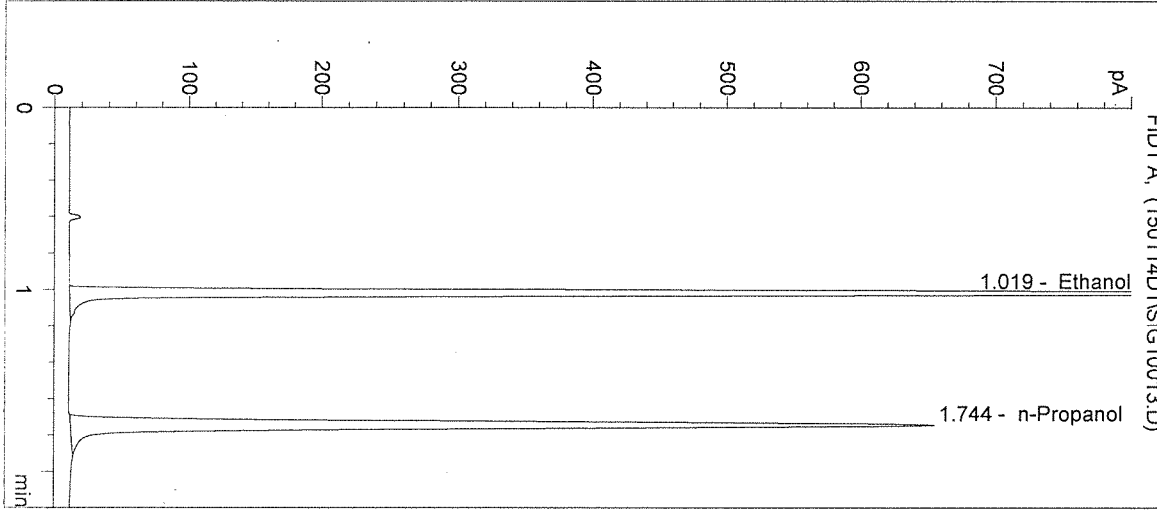

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 2045 | 1.019 |
| 2 | n-Propanol | 1713 | 1.744 |



Ethanol 0.255 g/100mL




n-Propanol 0.012 g/100mL


JN
DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 3:09:09 PM Sample Name: 15008 #5
Instrument: HSGC#3 Operator: David Nguyen
Column: DB-ALC2 Location: Vial 14
Method: C:\HPCHEM\2\METHODS\SIMALC3.M
Sample Info:

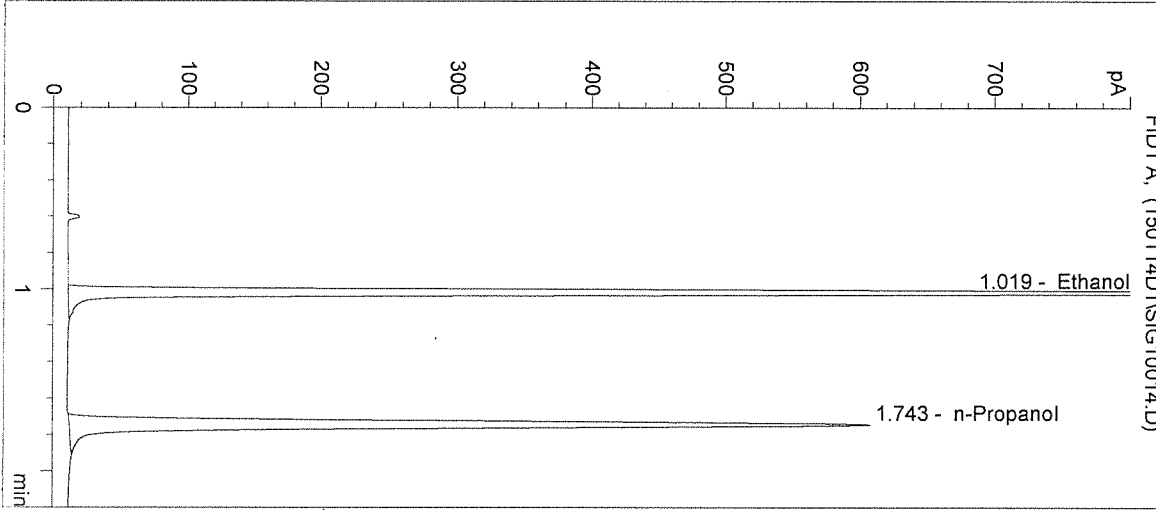

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1888 | 1.019 |
| 2 | n-Propanol | 1591 | 1.743 |

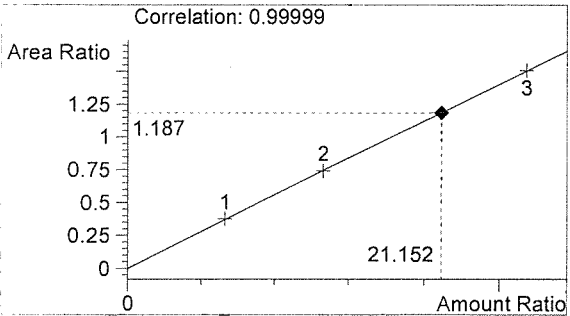

Ethanol 0.254 g/100mL

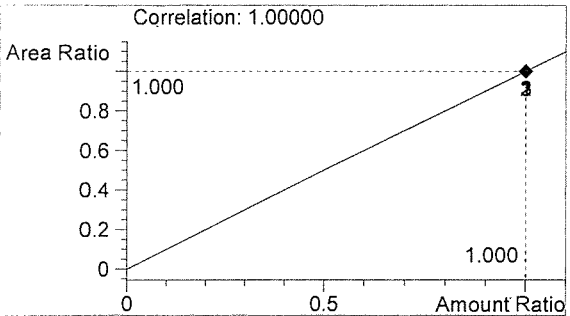


n-Propanol 0.012 g/100mL


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 3:12:22 PM Sample Name: POS CTRL (0.10)
 Instrument: HSGC#3 Operator: David Nguyen
 Column: DB-ALC2 Location: Vial 15
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: POS CTRL: 0.10 g/100mL
 15008

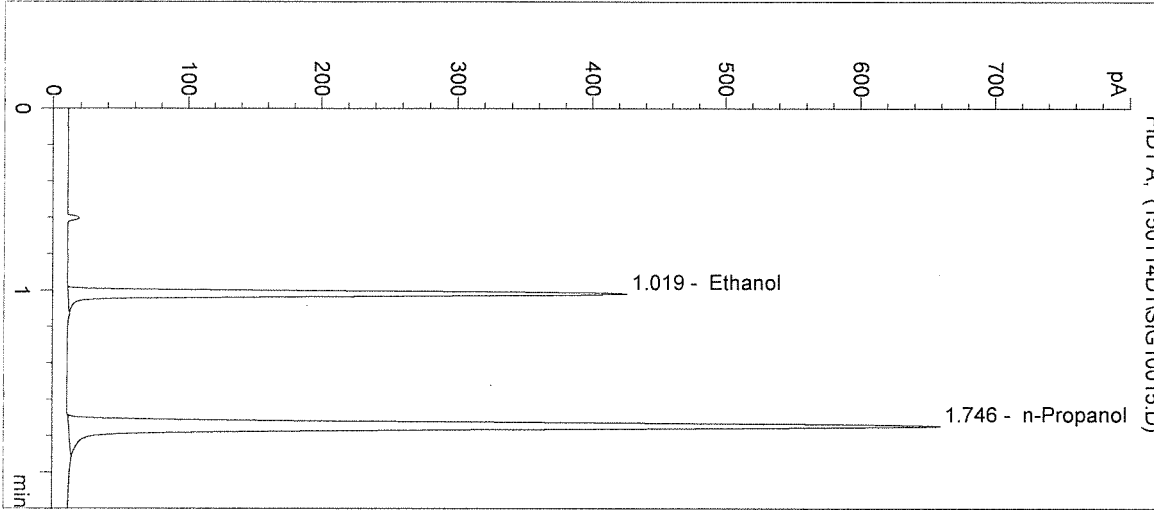

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 825 | 1.019 |
| 2 | n-Propanol | 1727 | 1.746 |

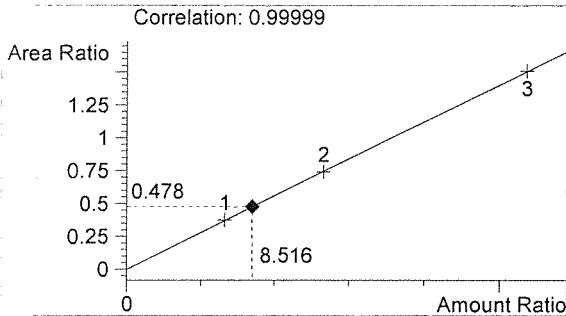

Ethanol 0.102 g/100mL

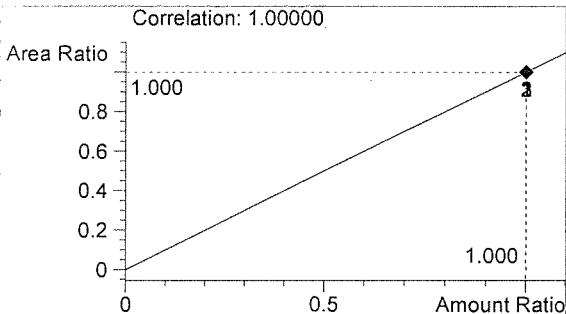

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 3:15:35 PM

Sample Name: NEG CTRL

Instrument: HSGC#3


Operator: David Nguyen

Column: DB-ALC2


Location: Vial 16

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info: 15008

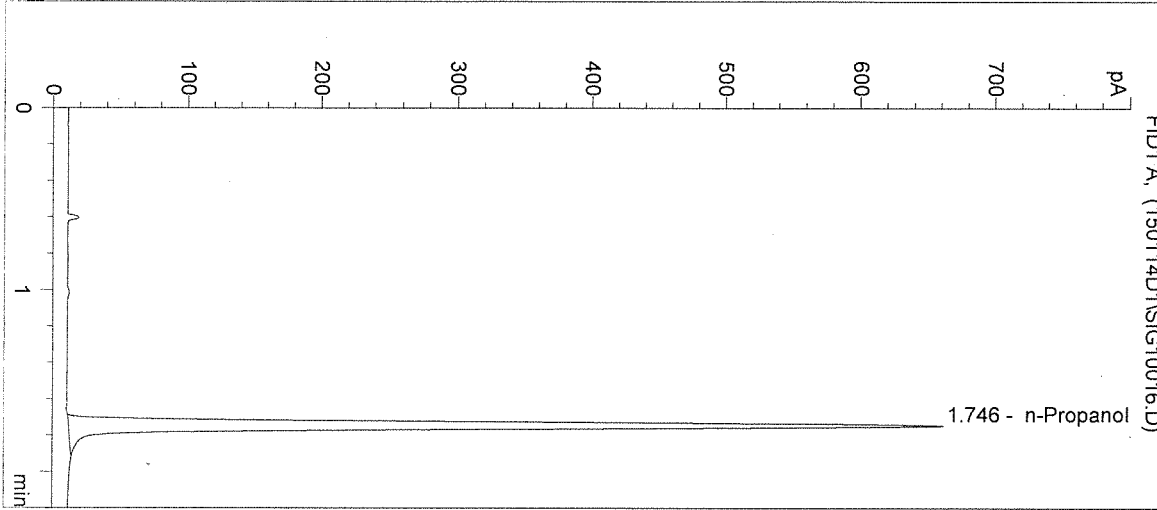

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 0 | 0.000 |
| 2 | n-Propanol | 1737 | 1.746 |

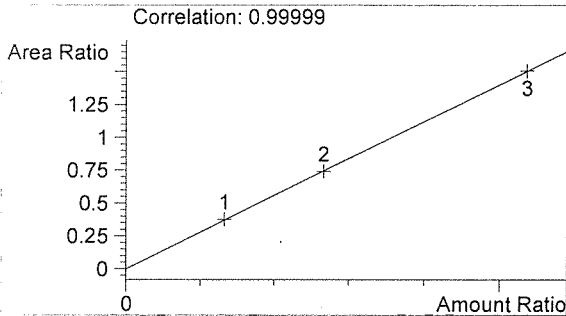

Ethanol 0.000 g/100mL

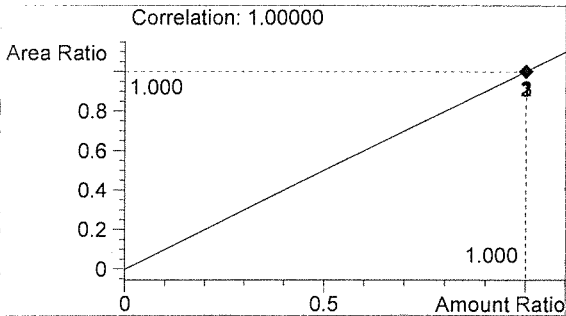

n-Propanol 0.012 g/100mL

DN

DN

Sequence Parameters:

Operator: Naziha Nuwayhid, PhD
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\2\DATA\
 Data Subdirectory: 150114NN
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

CAL 1: 0.079 g/100mL - Lot#: E0814-01 Exp. 02/19/2015
 CAL 2: 0.158 g/100mL - Lot#: E0814-02 Exp. 02/19/2015
 CAL 3: 0.316 g/100mL - Lot#: E0814-03 Exp. 02/19/2015

 CTRL 1: 0.04 g/100mL - Lot#: FN05011301 Exp. 05/2018
 CTRL 2: 0.10 g/100mL - Lot#: FN08051301 Exp. 10/2018
 CTRL 3: 0.20 g/100mL - Lot#: FN03211401 Exp. 06/2019

 n-Propanol ISTD - Lot#: P1114 Exp. 02/20/2015

 Calibration vials 1-9 filed with 15004.

Sequence Table (Front Injector):

Method and Injection Info Part:

| Line | Location | SampleName | Method | Inj | SampleType | InjVolume | DataFile |
|------|----------|-----------------|---------|-----|------------|-----------|----------|
| 1 | Vial 1 | BLANK | SIMALC3 | 1 | Sample | | |
| 2 | Vial 2 | CAL 1 (0.079) | SIMALC3 | 1 | Calib | | |
| 3 | Vial 3 | CAL 2 (0.158) | SIMALC3 | 1 | Calib | | |
| 4 | Vial 4 | CAL 3 (0.316) | SIMALC3 | 1 | Calib | | |
| 5 | Vial 5 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 6 | Vial 6 | CTRL 1 (0.04) | SIMALC3 | 1 | Ctrl Samp | | |
| 7 | Vial 7 | CTRL 2 (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 8 | Vial 8 | CTRL 3 (0.20) | SIMALC3 | 1 | Ctrl Samp | | |
| 9 | Vial 9 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 10 | Vial 10 | 15004 #1 | SIMALC3 | 1 | Sample | | |
| 11 | Vial 11 | 15004 #2 | SIMALC3 | 1 | Sample | | |
| 12 | Vial 12 | 15004 #3 | SIMALC3 | 1 | Sample | | |
| 13 | Vial 13 | 15004 #4 | SIMALC3 | 1 | Sample | | |
| 14 | Vial 14 | 15004 #5 | SIMALC3 | 1 | Sample | | |
| 15 | Vial 15 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 16 | Vial 16 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 17 | Vial 17 | 15005 #1 | SIMALC3 | 1 | Sample | | |
| 18 | Vial 18 | 15005 #2 | SIMALC3 | 1 | Sample | | |
| 19 | Vial 19 | 15005 #3 | SIMALC3 | 1 | Sample | | |
| 20 | Vial 20 | 15005 #4 | SIMALC3 | 1 | Sample | | |
| 21 | Vial 21 | 15005 #5 | SIMALC3 | 1 | Sample | | |
| 22 | Vial 22 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 23 | Vial 23 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 24 | Vial 24 | 15006 #1 | SIMALC3 | 1 | Sample | | |

~~15004~~
 Ru/27/15
 15008
 Ru/27/15
 Jf

| Line | Location | SampleName | Method | Inj | SampleType | InjVolume | DataFile |
|------|----------|-----------------|---------|-----|------------|-----------|----------|
| 25 | Vial 25 | 15006 #2 | SIMALC3 | 1 | Sample | | |
| 26 | Vial 26 | 15006 #3 | SIMALC3 | 1 | Sample | | |
| 27 | Vial 27 | 15006 #4 | SIMALC3 | 1 | Sample | | |
| 28 | Vial 28 | 15006 #5 | SIMALC3 | 1 | Sample | | |
| 29 | Vial 29 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 30 | Vial 30 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 31 | Vial 31 | 15007 #1 | SIMALC3 | 1 | Sample | | |
| 32 | Vial 32 | 15007 #2 | SIMALC3 | 1 | Sample | | |
| 33 | Vial 33 | 15007 #3 | SIMALC3 | 1 | Sample | | |
| 34 | Vial 34 | 15007 #4 | SIMALC3 | 1 | Sample | | |
| 35 | Vial 35 | 15007 #5 | SIMALC3 | 1 | Sample | | |
| 36 | Vial 36 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 37 | Vial 37 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |
| 38 | Vial 38 | 15008 #1 | SIMALC3 | 1 | Sample | | |
| 39 | Vial 39 | 15008 #2 | SIMALC3 | 1 | Sample | | |
| 40 | Vial 40 | 15008 #3 | SIMALC3 | 1 | Sample | | |
| 41 | Vial 41 | 15008 #4 | SIMALC3 | 1 | Sample | | |
| 42 | Vial 42 | 15008 #5 | SIMALC3 | 1 | Sample | | |
| 43 | Vial 43 | POS CTRL (0.10) | SIMALC3 | 1 | Ctrl Samp | | |
| 44 | Vial 44 | NEG CTRL | SIMALC3 | 1 | Ctrl Samp | | |

Calibration Part:

| Line | Location | SampleName | Method | CalLev | Update | RF | Update | RT | Interval |
|------|----------|---------------|---------|--------|---------|----|---------|----|----------|
| 2 | Vial 2 | CAL 1 (0.079) | SIMALC3 | 1 | Replace | | Replace | | |
| 3 | Vial 3 | CAL 2 (0.158) | SIMALC3 | 2 | Replace | | Replace | | |
| 4 | Vial 4 | CAL 3 (0.316) | SIMALC3 | 3 | Replace | | Replace | | |

Sequence Table (Back Injector):

No entries - empty table!

15008

Ju/27/15

for

Inj. Date: 1/14/2015 6:46:20 PM

Sample Name: 15008 #1

Instrument: HSGC#3


Operator: Naziha Nuwayhid, PhD

Column: DB-ALC2


Location: Vial 38

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

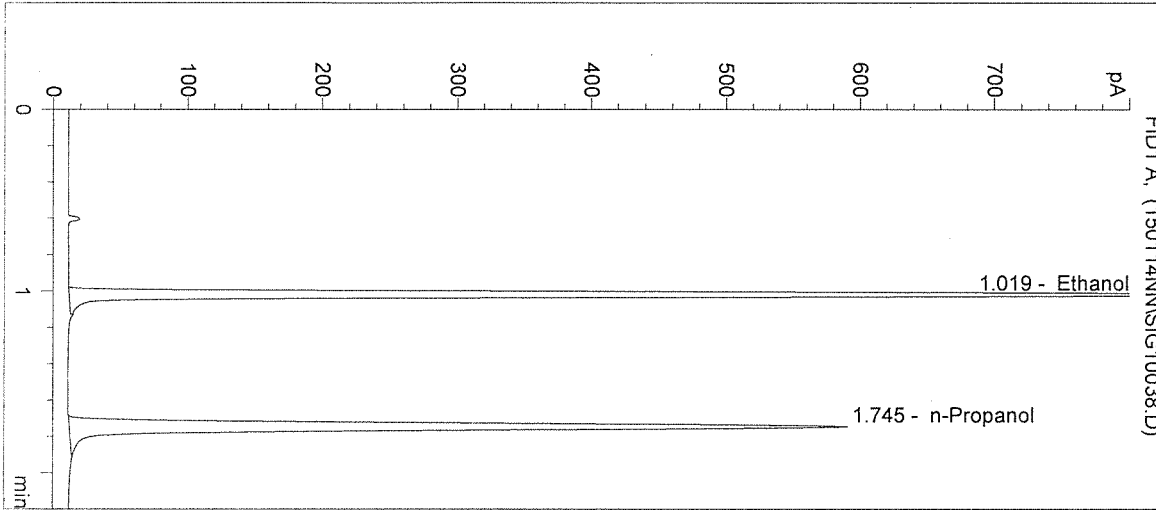

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1795 | 1.019 |
| 2 | n-Propanol | 1551 | 1.745 |

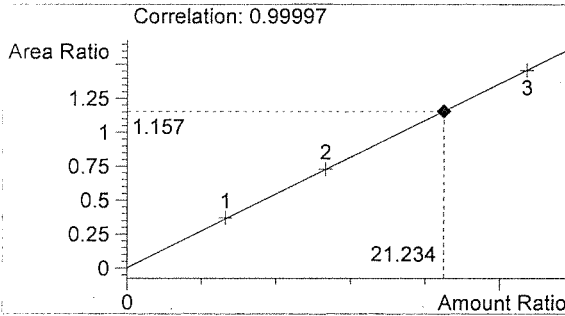

Ethanol 0.255 g/100mL

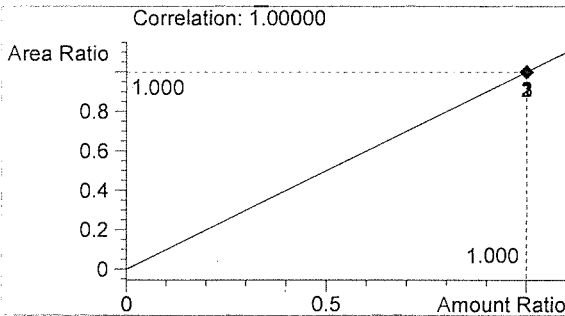

n-Propanol 0.012 g/100mL

fr

nn

Inj. Date: 1/14/2015 6:49:34 PM

Sample Name: 15008 #2

Instrument: HSGC#3


Operator: Naziha Nuwayhid, PhD

Column: DB-ALC2


Location: Vial 39

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

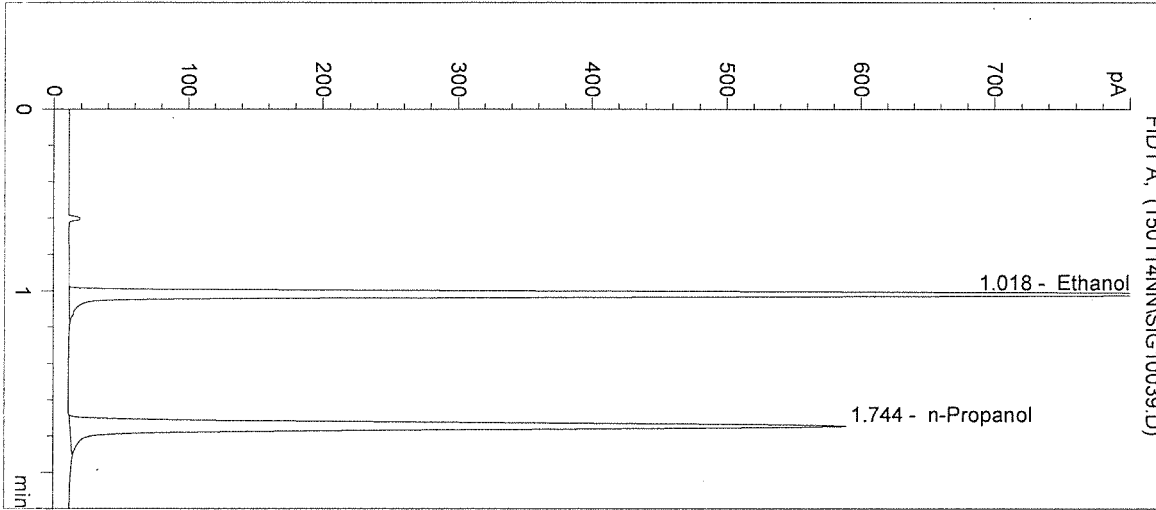

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1791 | 1.018 |
| 2 | n-Propanol | 1544 | 1.744 |

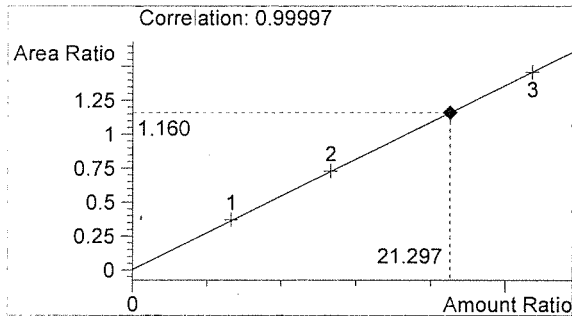

Ethanol 0.256 g/100mL

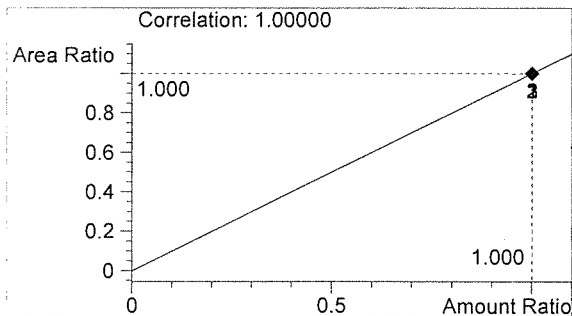

n-Propanol 0.012 g/100mL

fn

M

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 6:52:47 PM

Sample Name: 15008 #3

Instrument: HSGC#3


Operator: Naziha Nuwayhid, PhD

Column: DB-ALC2


Location: Vial 40

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

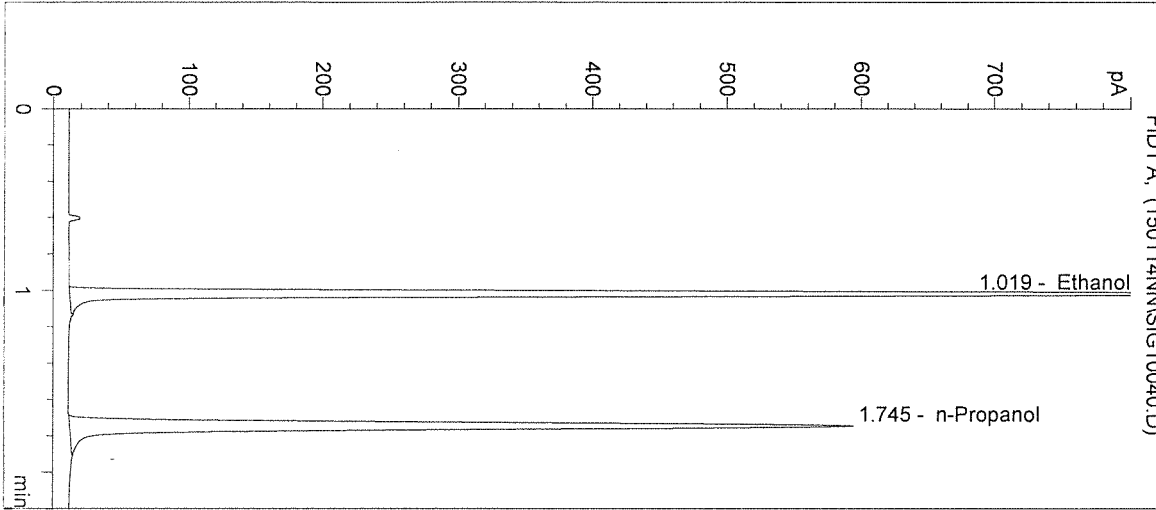

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1803 | 1.019 |
| 2 | n-Propanol | 1561 | 1.745 |

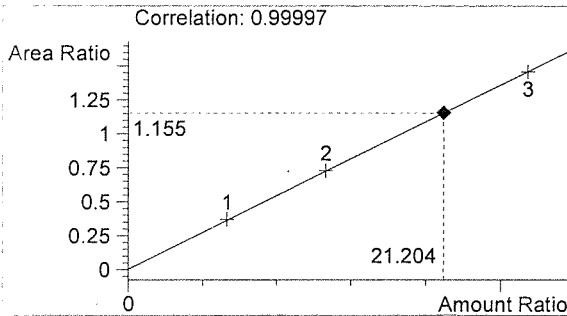

Ethanol 0.254 g/100mL

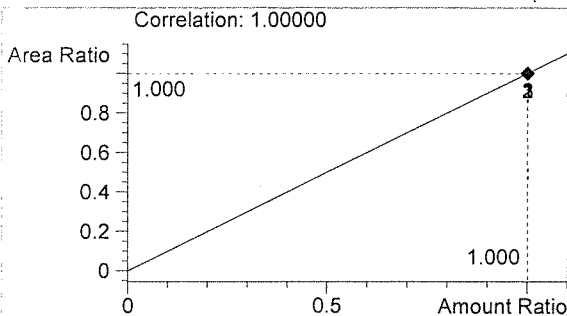

n-Propanol 0.012 g/100mL

fu

mw

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 6:56:00 PM

Sample Name: 15008 #4

Instrument: HSGC#3


Operator: Naziha Nuwayhid, PhD

Column: DB-ALC2


Location: Vial 41

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

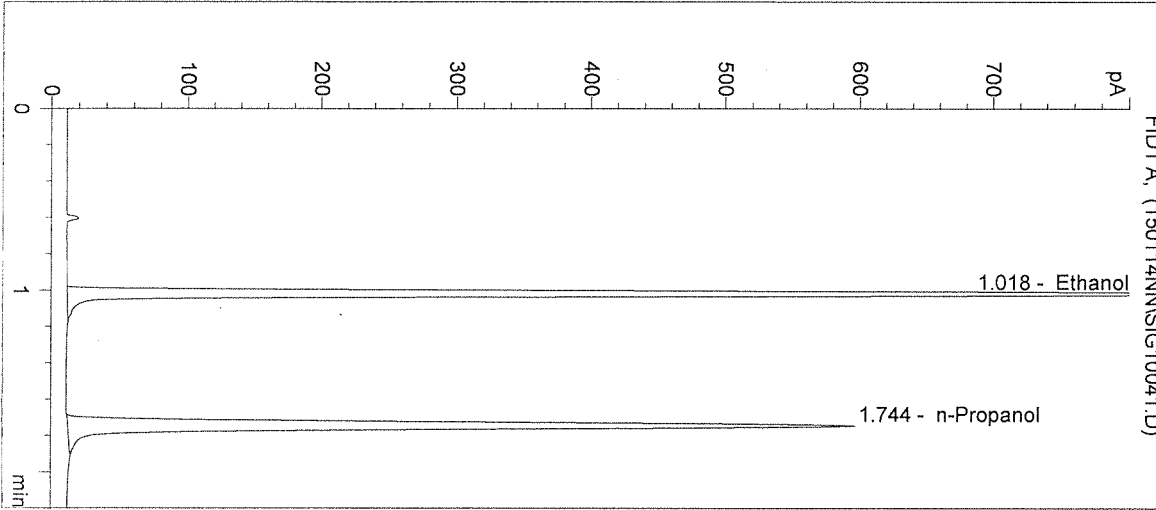

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1823 | 1.018 |
| 2 | n-Propanol | 1568 | 1.744 |

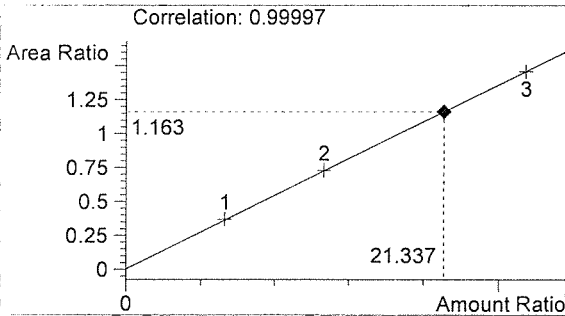

Ethanol 0.256 g/100mL

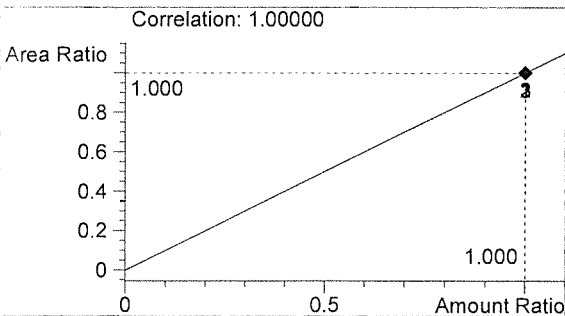

n-Propanol 0.012 g/100mL

h

MW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 6:59:14 PM

Sample Name: 15008 #5

Instrument: HSGC#3


Operator: Naziha Nuwayhid, PhD

Column: DB-ALC2


Location: Vial 42

Method: C:\HPCHEM\2\METHODS\SIMALC3.M


Sample Info:

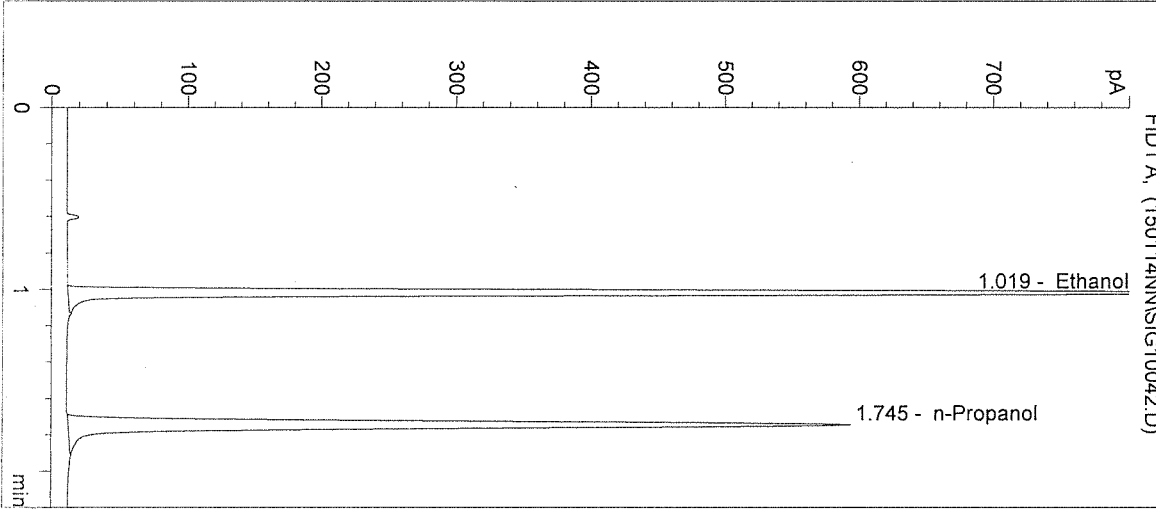

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 1791 | 1.019 |
| 2 | n-Propanol | 1556 | 1.745 |

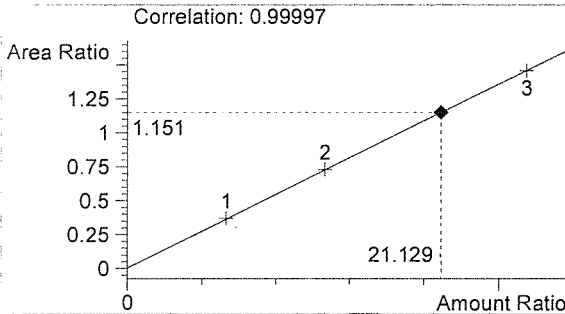

Ethanol 0.254 g/100mL

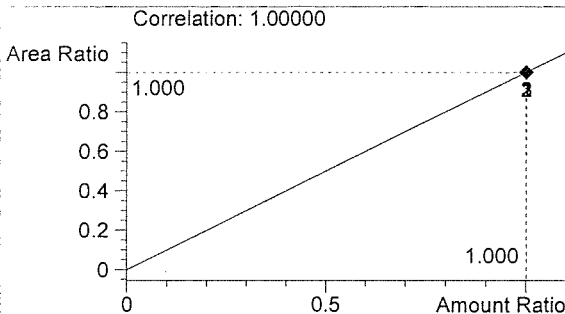


n-Propanol 0.012 g/100mL

Handwritten signature


Handwritten initials

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/14/2015 7:02:27 PM Sample Name: POS CTRL (0.10)
 Instrument: HSGC#3 Operator: Naziha Nuwayhid, PhD
 Column: DB-ALC2 Location: Vial 43
 Method: C:\HPCHEM\2\METHODS\SIMALC3.M
 Sample Info: POS CTRL: 0.10 g/100mL
~~15004, 15005, 15006, 15007, 15008~~
 1.15.15 NN

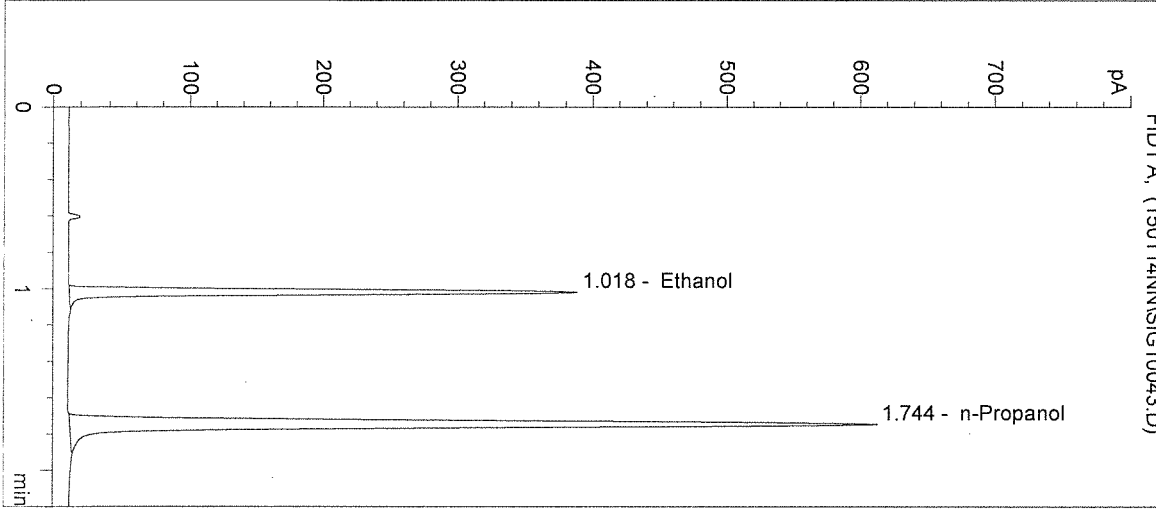

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 752 | 1.018 |
| 2 | n-Propanol | 1604 | 1.744 |

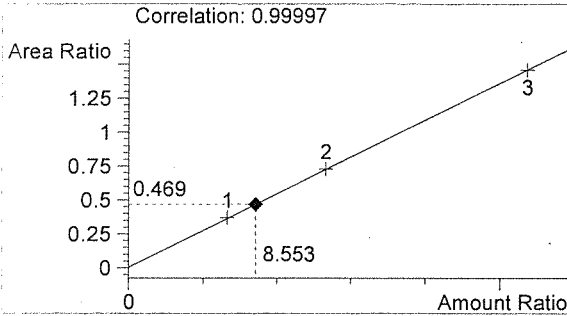

Ethanol 0.103 g/100mL

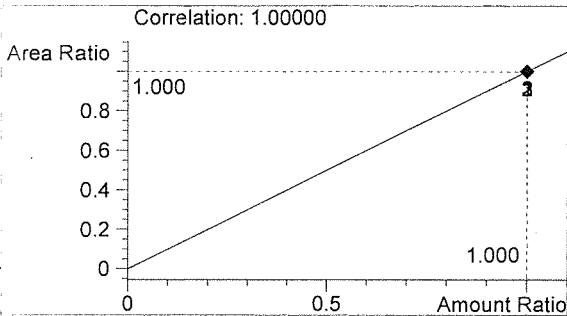

n-Propanol 0.012 g/100mL

Handwritten signature
W

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/14/2015 7:05:40 PM

Sample Name: NEG CTRL

Instrument: HSGC#3

Operator: Naziha Nuwayhid, PhD


Column: DB-ALC2

Location: Vial 44


Method: C:\HPCHEM\2\METHODS\SIMALC3.M

Sample Info: 15004, 15005, 15006, 15007, 15008


1.15.15 MW

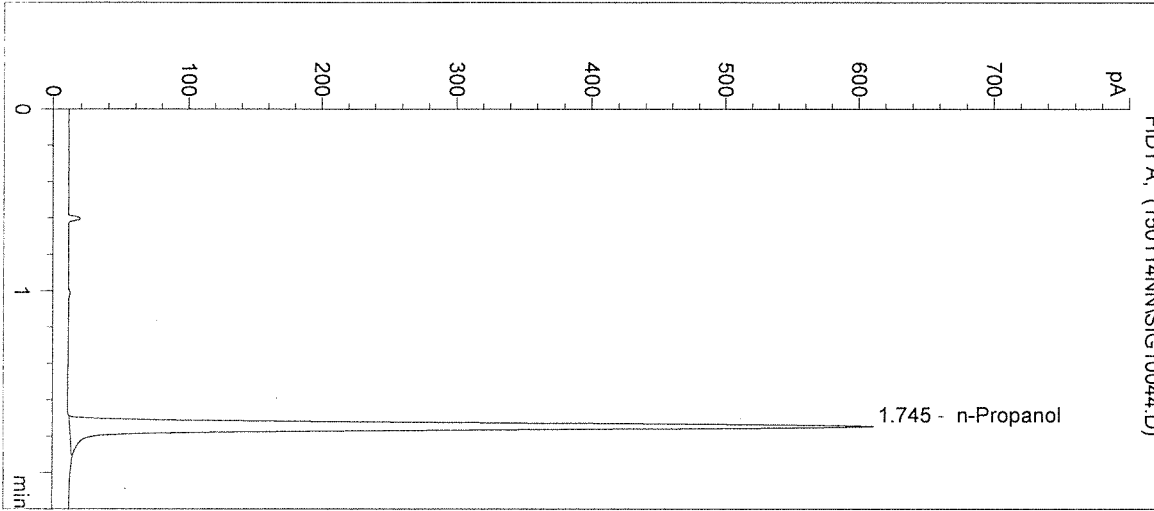

| # | Compound | Peak Area | RT (min) |
|---|------------|-----------|----------|
| 1 | Ethanol | 0 | 0.000 |
| 2 | n-Propanol | 1603 | 1.745 |

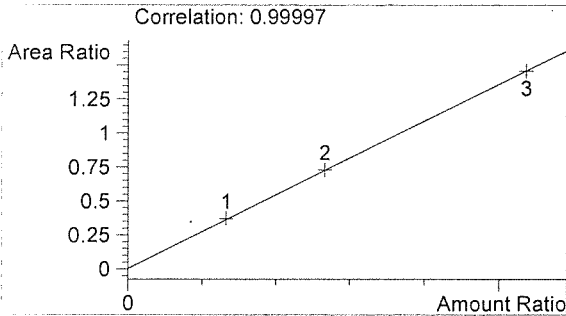

Ethanol 0.000 g/100mL

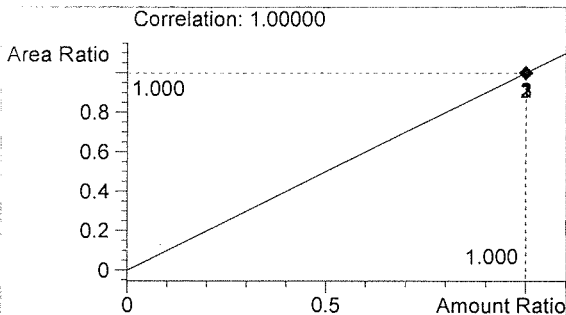

n-Propanol 0.012 g/100mL

h

NW