



QUALITY ASSURANCE PROCEDURE SOLUTION TEST REPORT

BATCH REPORT: 16018

CUSTOMER INFORMATION

Washington State Patrol – Breath Test Program
811 East Roanoke SEATTLE, WA 98102

TESTING PROCEDURE USED: TLD Technical Manual, Chapter 4.0 Certification of Simulator Solutions; Headspace-Gas Chromatography.

TESTING ITEM INFORMATION

TARGET VAPOR CONCENTRATION: 0.08 g/210L
DATE PREPARED: 05/20/2016
BATCH UNITS: g/100mL

IDENTITY: QAP Solution
PREPARED BY: Christopher S. Johnston

	CSJ	AC	KH
1	0.099	0.099	0.099
2	0.099	0.099	0.097
3	0.099	0.098	0.099
4	0.099	0.099	0.099
5	0.100	0.099	0.099
C	0.101	0.100	0.099

ETHANOL CONTROL INFORMATION

LOT NUMBER: FN08051301 EXPIRATION: 10/2018 CONCENTRATION: 0.10 g/100mL

RESULTS OF TESTING

AVERAGE SOLUTION CONCENTRATION: 0.0989 g/100mL PRECISION CV (%): 0.65
STANDARD DEVIATION: 0.00064 NUMBER OF TESTS: 15

EQUIVALENT VAPOR CONCENTRATION: **0.0804 g/210L**
EXPANDED UNCERTAINTY: ± 0.0020 (k=2, 95.45% confidence interval)

WASHINGTON STATE PATROL – TOXICOLOGY LABORATORY DIVISION

Lisa Noble

Lisa Noble Forensic Scientist Supervisor

6/29/16

DATE REPORT ISSUED

THIS TESTING WAS PERFORMED BY:			
ANALYST	NAME	SIGNATURE	DATE TESTED
CSJ	Christopher S. Johnston	<i>Chris S. Johnston</i>	05/20/2016
AC	Amanda Chandler	<i>Amanda Chandler</i>	05/24/2016
KH	Katie Harris	<i>Katie Harris</i>	05/27/2016

This report applies only to the item being tested and shall not be reproduced except in full, without the written approval of the WSP Toxicology Laboratory Division. Page 1 of 1

Washington State Patrol - Toxicology Laboratory Division
QAP Test Report Calculation Record

QAP Solution Batch #: 16018

Date Prepared: 5/20/2016

Analyst: CSJ AC KH
Date Tested: 5/20/2016 5/24/2016 5/27/2016
Instrument: HSGC #1 HSGC #1 HSGC #1

1	0.099	0.099	0.099
2	0.099	0.099	0.097
3	0.099	0.098	0.099
4	0.099	0.099	0.099
5	0.100	0.099	0.099
C	0.101	0.100	0.099

	CV^2_{COA}	$CV^2_{QAP\ Solution}$	$CV^2_{Control}$	$CV^2_{Part\ Coef}$
1018	0.0000084100	0.0000027931	0.0000333333	0.0001016326

Ethanol Control Lot #: FN08051301
Control Uncertainty (%): 0.29

Average Solution Concentration: 0.0989 g/100mL
Standard Deviation: 0.00064 g/100mL
Precision CV (%): 0.65 %
Equivalent Vapor Concentration: 0.0804 g/210L
Combined Standard Uncertainty (\pm): 0.0010 g/210L
Expanded Uncertainty (\pm): 0.0020 coverage factor (k) =2 (95.45% level of confidence)

Calculations performed by: Lisa Noble [Signature] 6/13/16
Name Signature Date

Calculations verified by: Amanda M. Black [Signature] 6-27-16
Name Signature Date

Method: Hand calculation

Tech. review performed by: Lisa Noble [Signature] 6/13/16
Name Signature Date

SIMULATOR SOLUTION DATA ENTRY REVIEW

Reviewer/s: Amanda M. Black

Date: 6-27-16

Location: WSL-FLSB Seattle, WA

Solution Batch Number: 16018

	YES	NO	N/A
Analysis dates do not precede preparation date:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Declarations signed and properly dated:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Data entry corresponds to all chromatograms:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
All signatures present on Test Report:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Average solution concentration correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Standard deviation correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
CV (%) correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Equivalent vapor concentration correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
All chromatograms and sequences included in file:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ethanol control information present: (lot # present & used within expiration)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Complies with accuracy and precision requirements established by the State Toxicologist:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Comments:

Reviewer Signature: 

Date: 6-27-16



SOLUTION CERTIFICATE REVIEW

Please check that the data on your chromatograms is the data entered into the Test Report, that the date to the right of your name is the date that you tested the solution, and then sign the Test Report.

Please initial and date below to affirm that you have:

- 1) Checked your data
- 2) Checked the date to the right of your name on the Test Report
- 3) Signed the Test Report

	Initials	Date
Amanda Chandler	AZ	6/13/16
Andrew Gingras		
Asa Louis		
Brittany Thomas		
Christie Mitchell-Mata		
Christopher Johnston	W	6/13/16
David Nguyen		
Dawn Sklerov		
Elizabeth Wehner		
Justin Knoy		
Katie Harris	KH	6/13/16
Lyndsey Lowe		
Naziha Nuwayhid		
Rebecca Flaherty		

Batch # 16018 6/13/16

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.08 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 16018**


I, Christopher S. Johnston, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Biochemistry.

The quality assurance procedure (QAP) solution, Lot Number 16018, was prepared in the Washington State Toxicology Laboratory on 5/20/2016. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 5/20/2017.

Seattle, WA



Christopher S. Johnston 5/13/2016
Forensic Scientist Date



JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.08 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 16018**


I, Amanda Chandler, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: MS degree in Forensic Toxicology.

The quality assurance procedure (QAP) solution, Lot Number 16018, was prepared in the Washington State Toxicology Laboratory on 5/20/2016. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 5/20/2017.

Seattle, WA

 4/13/14

Amanda Chandler

Date

Forensic Scientist



JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.08 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 16018**

I, Katie Harris, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS in Biochemistry and MS degree in Forensic Science.

The quality assurance procedure (QAP) solution, Lot Number 16018, was prepared in the Washington State Toxicology Laboratory on 5/20/2016. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 5/20/2017.

Seattle, WA

Katie Harris 6/13/16

Katie Harris

Date

Forensic Scientist

WSP-TLD COMBINED SIMULATOR SOLUTION PREPARATION WORKSHEET

FILE A COPY IN THE BATCH FILE FOR EACH SOLUTION LISTED ON THE WORKSHEET

Preparation Date: 5/20/16 Expiration Date: 5/20/17 Initials of Preparer: CJ

Lot # of 200-proof Ethanol used in preparation: 2EA0437

Date the 200-proof Ethanol bottle was opened: 4/7/16

After opening, each bottle of 200-proof Ethanol is approved for use for 6 months unless an extension is approved by the State Toxicologist. This timeframe applies to the 200-proof Ethanol only, not to simulator solutions which have a 1 year expiration.

Environmental conditions verified as acceptable:

Simulator Solution	Volume of Ethanol (mL)	Volume of Deionized Water (L)		Batch Number
QAP 0.04	11.2	18	<input checked="" type="checkbox"/>	<u>16017</u>
QAP 0.08	22.4	18	<input checked="" type="checkbox"/>	<u>16018</u>
QAP 0.08 QAP 0.10	22.4 28.1 <i>CJ 5/22/16</i>	18	<input checked="" type="checkbox"/>	<u>16019</u>
QAP 0.15	42.1	18	<input checked="" type="checkbox"/>	<u>16020</u>
QAP 0.20	56.1	18	<input type="checkbox"/>	_____
ESS	66.5	52	<input type="checkbox"/>	_____

Stir bar is rotating

Stirred for minimum 30 minutes; 2 hours for ESS

Spigot purged

Aliquot taken

Batch labeled, packaged and sealed Date 5/20/16

If different ethanol lot numbers are used in the preparation of solutions, record them and the corresponding solution batch numbers in the comments section.

Comments:
For operational needs I asked Chris to make two batches of 0.08 QAP.
In 5/22/16

[Signature]
Analyst Signature

5/20/16
Date

Sequence Parameters:

Operator: Chris Johnston
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 160520CJ
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

Ethanol Calibrator 1, E0416-01 - Exp. 10/01/2016
 Ethanol Calibrator 2, E0416-02 - Exp. 10/01/2016
 Ethanol Calibrator 3, E0416-03 - Exp. 10/01/2016
 CTRL1 (0.04g/100mL), Lot # FN05011301 - Exp. 05/2018
 CTRL2 (0.10g/100mL), Lot # FN08051301 - Exp. 10/2018
 CTRL3 (0.20g/100mL), Lot # FN03211401 - Exp. 06/2019
 Internal Standard Lot#P0316 - Exp. 06/29/2016

Calibration vials 1-9 filed with 16017.

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	NEG CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	NEG CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	16017-1	SIMALC1	1	Sample		
11	Vial 11	16017-2	SIMALC1	1	Sample		
12	Vial 12	16017-3	SIMALC1	1	Sample		
13	Vial 13	16017-4	SIMALC1	1	Sample		
14	Vial 14	16017-5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	NEG CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	16018-1	SIMALC1	1	Sample		
18	Vial 18	16018-2	SIMALC1	1	Sample		
19	Vial 19	16018-3	SIMALC1	1	Sample		
20	Vial 20	16018-4	SIMALC1	1	Sample		
21	Vial 21	16018-5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	NEG CTRL	SIMALC1	1	Ctrl Samp		
24	Vial 24	16019-1	SIMALC1	1	Sample		
25	Vial 25	16019-2	SIMALC1	1	Sample		
26	Vial 26	16019-3	SIMALC1	1	Sample		

16018

Handwritten signature

W W

Sequence: C:\HPCHEM\1\SEQUENCE\CJQAP1.S

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
27	Vial 27	16019-4	SIMALC1	1	Sample		
28	Vial 28	16019-5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL	SIMALC1	1	Ctrl Samp		
30	Vial 30	NEG CTRL	SIMALC1	1	Ctrl Samp		
31	Vial 31	16020-1	SIMALC1	1	Sample		
32	Vial 32	16020-2	SIMALC1	1	Sample		
33	Vial 33	16020-3	SIMALC1	1	Sample		
34	Vial 34	16020-4	SIMALC1	1	Sample		
35	Vial 35	16020-5	SIMALC1	1	Sample		
36	Vial 36	0.10 CTRL	SIMALC1	1	Ctrl Samp		
37	Vial 37	NEG CTRL	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

16018

2/6/16

✓

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:15:11 PM

Sample Name: 16018-1

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 17

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

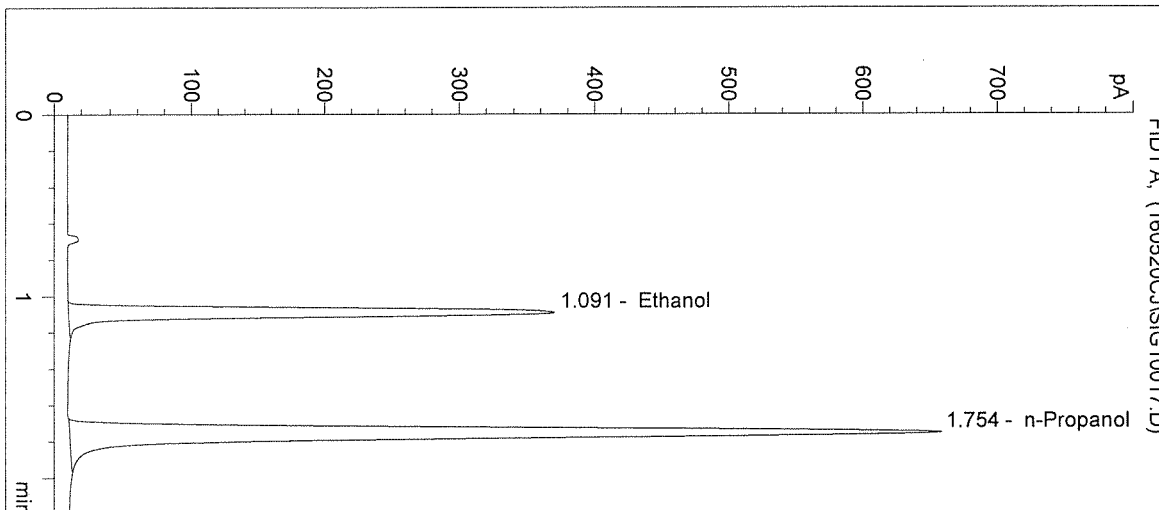

#	Compound	Peak Area	RT (min)
1	Ethanol	1224	1.091
2	n-Propanol	2550	1.754

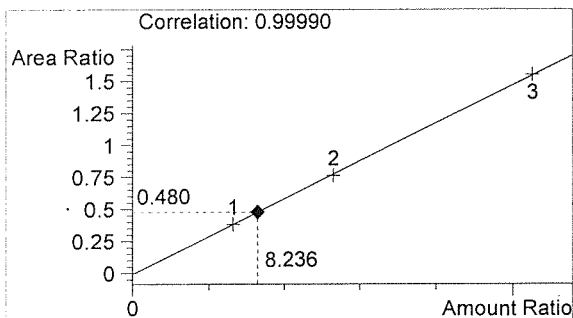

Ethanol 0.099 g/100mL

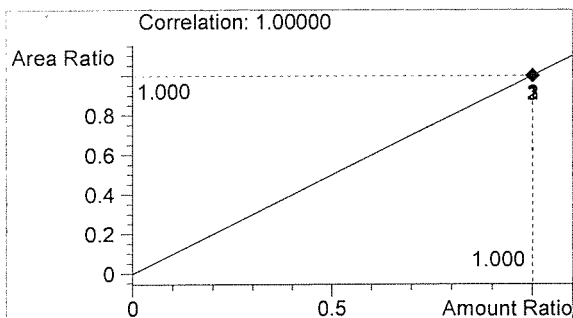

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten mark

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:18:24 PM

Sample Name: 16018-2

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 18

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

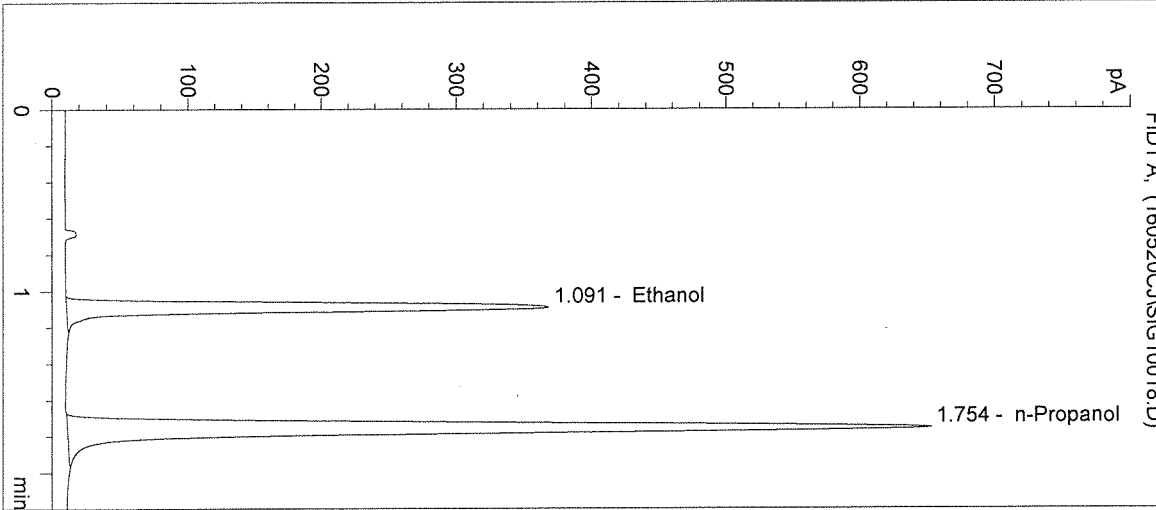

#	Compound	Peak Area	RT (min)
1	Ethanol	1220	1.091
2	n-Propanol	2540	1.754

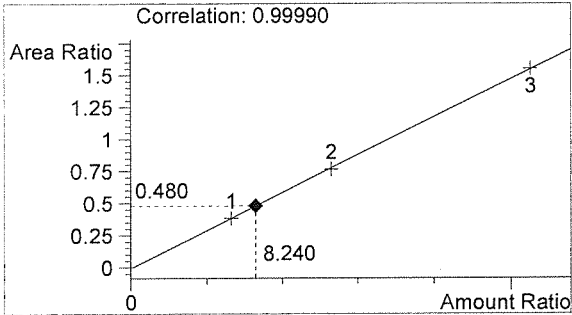

Ethanol 0.099 g/100mL

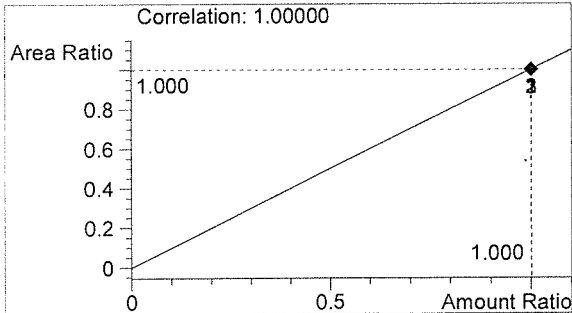

n-Propanol 0.012 g/100mL

fr

W

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:21:37 PM

Sample Name: 16018-3

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 19

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

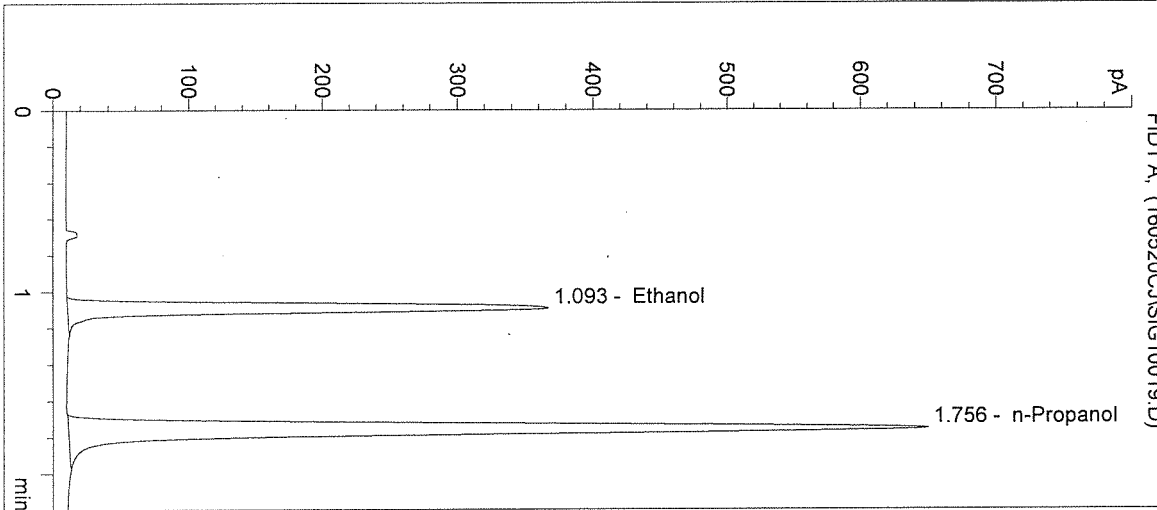

#	Compound	Peak Area	RT (min)
1	Ethanol	1223	1.093
2	n-Propanol	2536	1.756

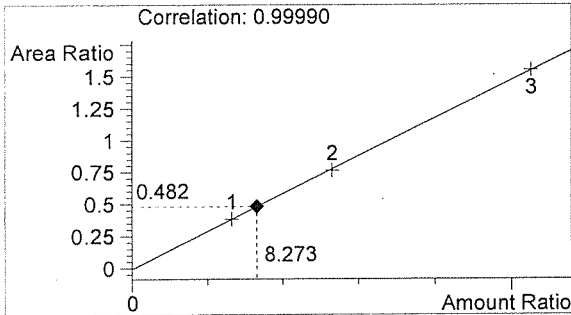

Ethanol 0.099 g/100mL

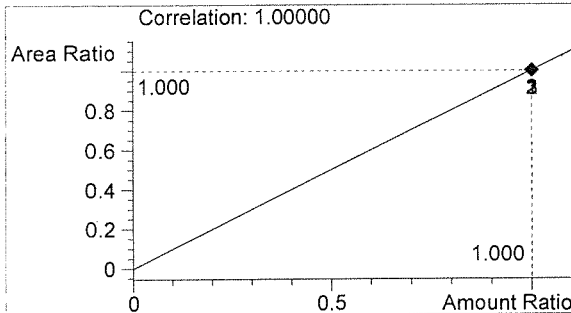

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten mark

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:24:51 PM

Sample Name: 16018-4

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 20

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

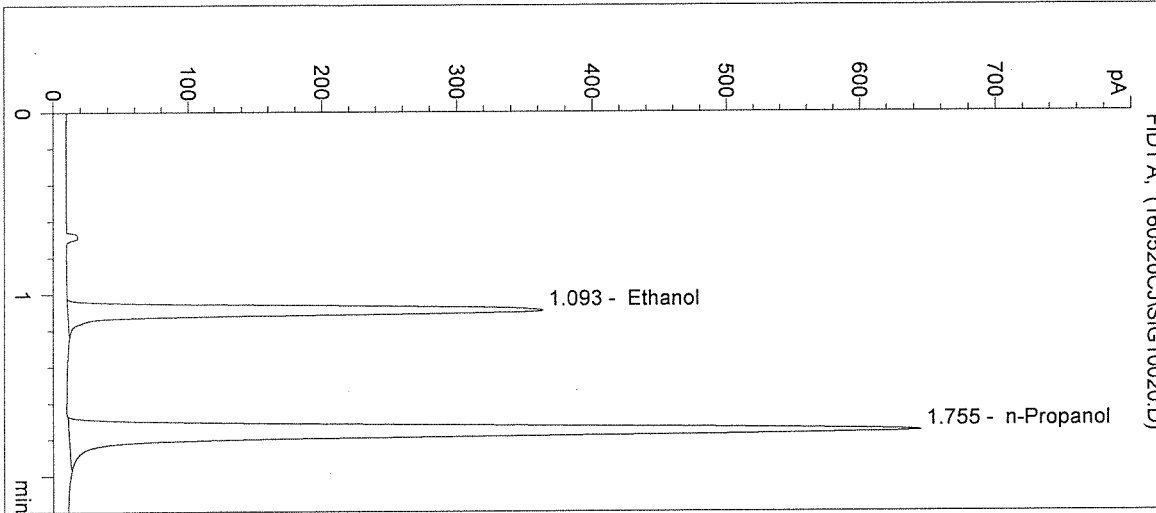

#	Compound	Peak Area	RT (min)
1	Ethanol	1216	1.093
2	n-Propanol	2518	1.755

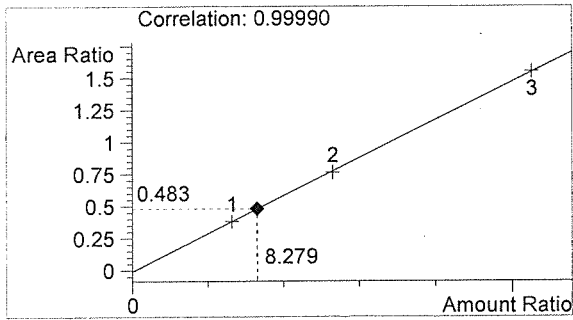

Ethanol 0.099 g/100mL

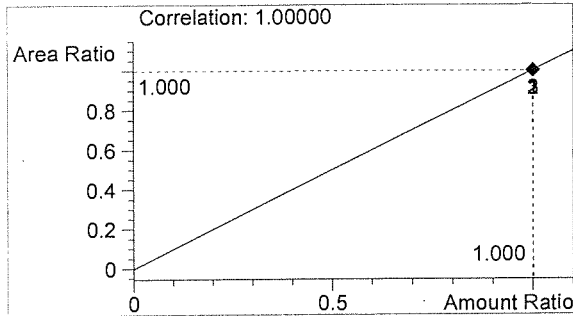

n-Propanol 0.012 g/100mL

Handwritten signature

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:28:04 PM

Sample Name: 16018-5

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 21

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

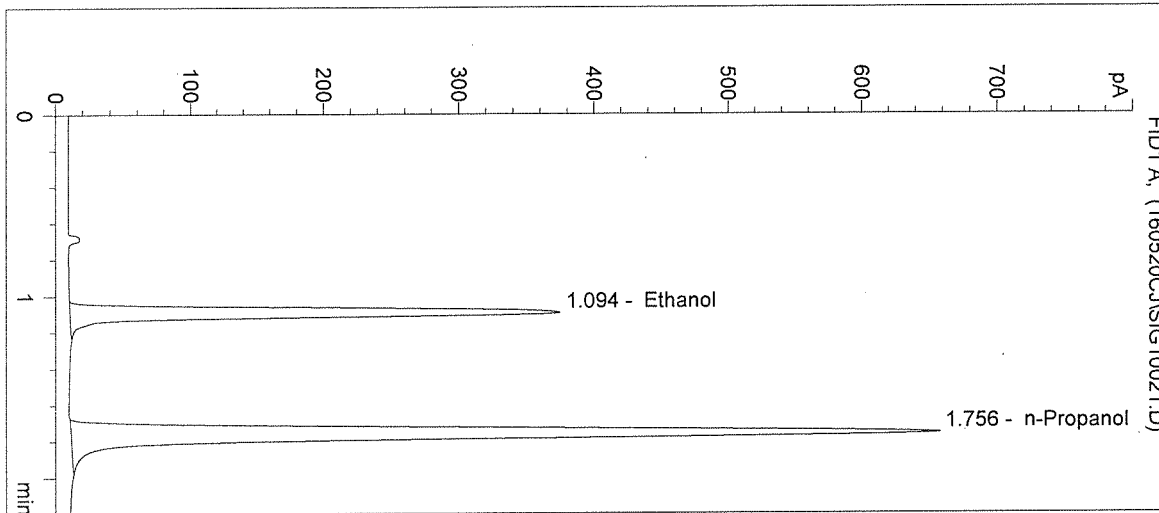

#	Compound	Peak Area	RT (min)
1	Ethanol	1249	1.094
2	n-Propanol	2572	1.756

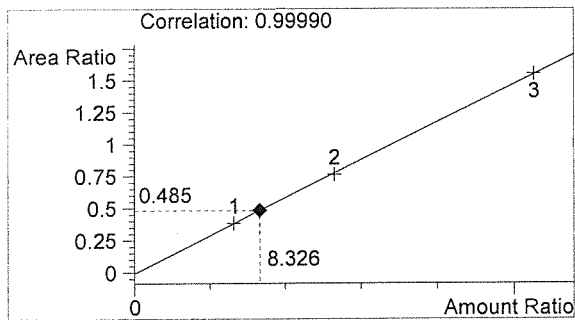

Ethanol 0.100 g/100mL

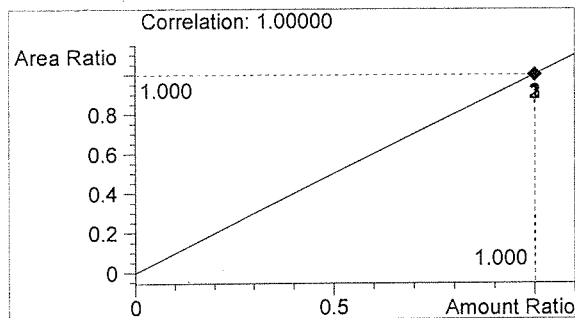

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten mark

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:31:17 PM

Sample Name: 0.10 CTRL

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 22

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: 16018

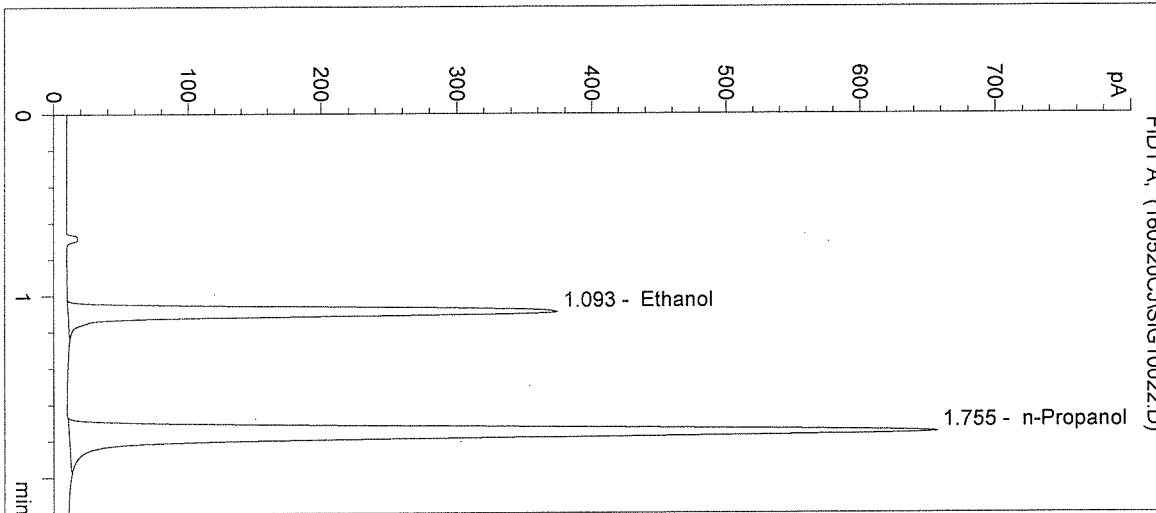

#	Compound	Peak Area	RT (min)
1	Ethanol	1263	1.093
2	n-Propanol	2583	1.755

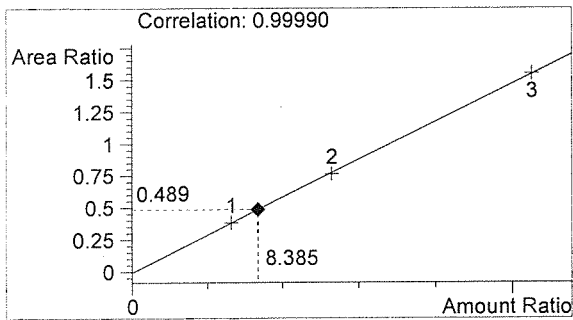

Ethanol 0.101 g/100mL

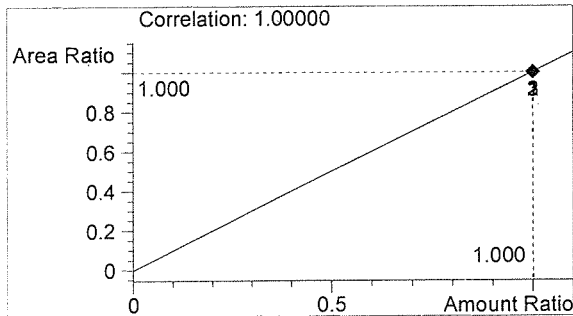

n-Propanol 0.012 g/100mL

jh

w

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/20/2016 3:34:30 PM

Sample Name: NEG CTRL

Instrument: HSGC#1


Operator: Chris Johnston

Column: DB-ALC1


Location: Vial 23

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: 16018

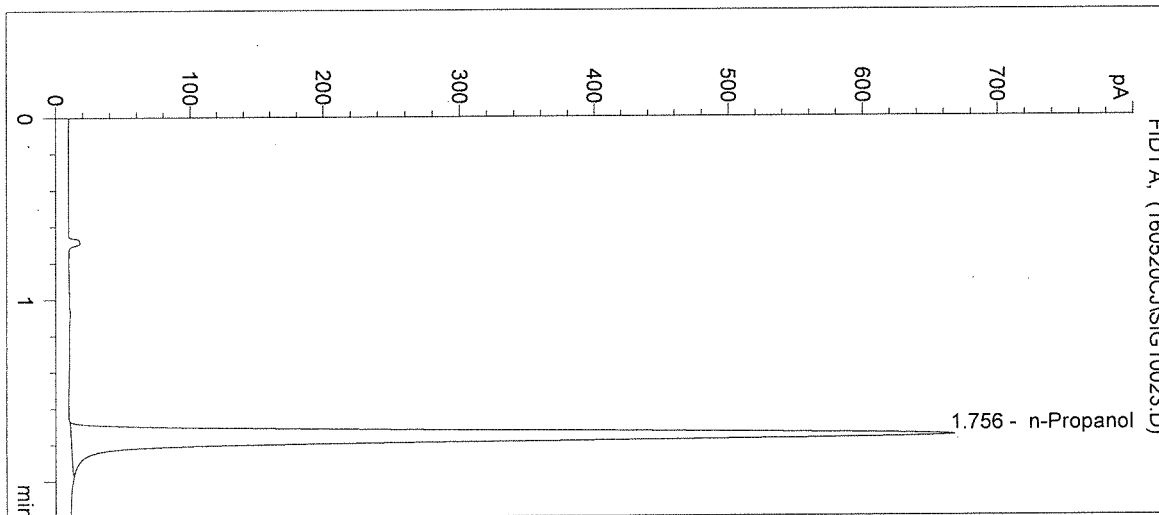

#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2624	1.756

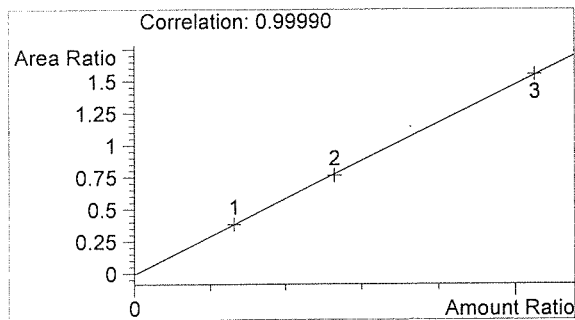

Ethanol 0.000 g/100mL

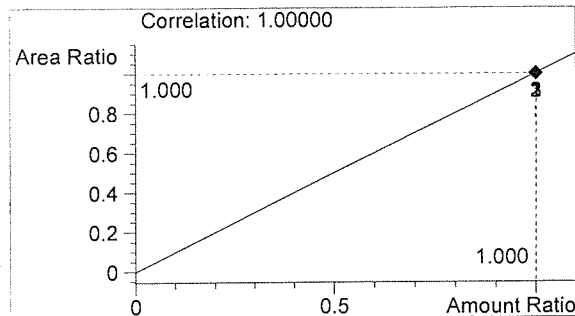

n-Propanol 0.012 g/100mL

jh

W

Sequence Parameters:

Operator: Amanda Chandler
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 160524AC
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

Ethanol Calibrator 1, E0416-01 - Exp. 10/01/2016
 Ethanol Calibrator 2, E0416-02 - Exp. 10/01/2016
 Ethanol Calibrator 3, E0416-03 - Exp. 10/01/2016
 CTRL1 (0.04g/100mL), Lot # FN05011301 - Exp. 05/2018
 CTRL2 (0.10g/100mL), Lot # FN08051301 - Exp. 10/2018
 CTRL3 (0.20g/100mL), Lot # FN03211401 - Exp. 06/2019
 Internal Standard Lot#P0316 - Exp. 06/29/2016

Calibration vials 1-9 filed with 16017.

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	NEG CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	NEG CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	16017-1	SIMALC1	1	Sample		
11	Vial 11	16017-2	SIMALC1	1	Sample		
12	Vial 12	16017-3	SIMALC1	1	Sample		
13	Vial 13	16017-4	SIMALC1	1	Sample		
14	Vial 14	16017-5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	NEG CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	16018-1	SIMALC1	1	Sample		
18	Vial 18	16018-2	SIMALC1	1	Sample		
19	Vial 19	16018-3	SIMALC1	1	Sample		
20	Vial 20	16018-4	SIMALC1	1	Sample		
21	Vial 21	16018-5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	NEG CTRL	SIMALC1	1	Ctrl Samp		
24	Vial 24	16019-1	SIMALC1	1	Sample		
25	Vial 25	16019-2	SIMALC1	1	Sample		
26	Vial 26	16019-3	SIMALC1	1	Sample		

16018

fn6/13/16

AR

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
27	Vial 27	16019-4	SIMALC1	1	Sample		
28	Vial 28	16019-5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL	SIMALC1	1	Ctrl Samp		
30	Vial 30	NEG CTRL	SIMALC1	1	Ctrl Samp		
31	Vial 31	16020-1	SIMALC1	1	Sample		
32	Vial 32	16020-2	SIMALC1	1	Sample		
33	Vial 33	16020-3	SIMALC1	1	Sample		
34	Vial 34	16020-4	SIMALC1	1	Sample		
35	Vial 35	16020-5	SIMALC1	1	Sample		
36	Vial 36	0.10 CTRL	SIMALC1	1	Ctrl Samp		
37	Vial 37	NEG CTRL	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

16018

Jn 6/13/16

AZ

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:26:04 PM

Sample Name: 16018-1

Instrument: HSGC#1


Operator: Amanda Chandler

Column: DB-ALC1


Location: Vial 17

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

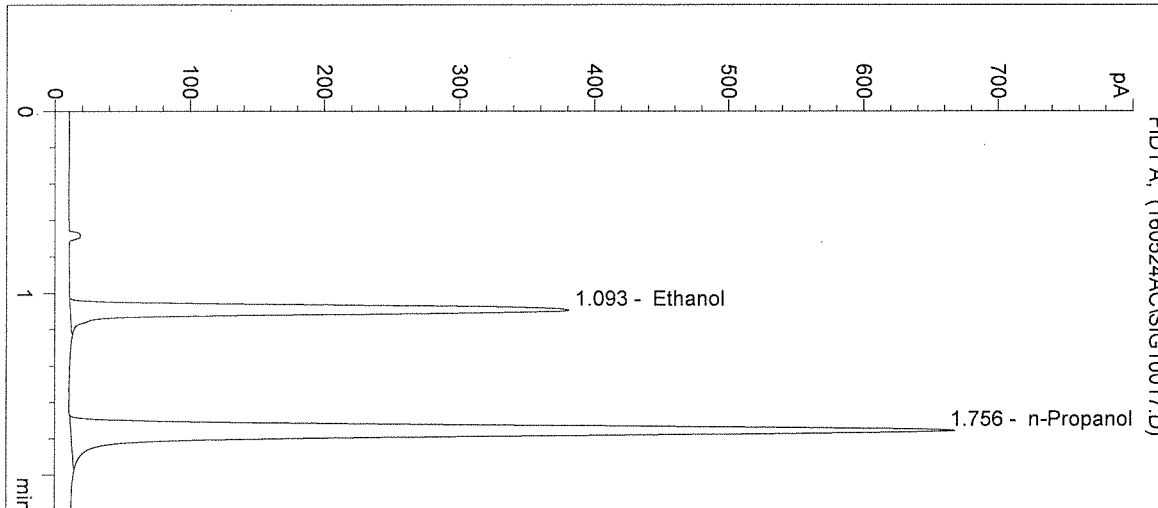

#	Compound	Peak Area	RT (min)
1	Ethanol	1254	1.093
2	n-Propanol	2587	1.756

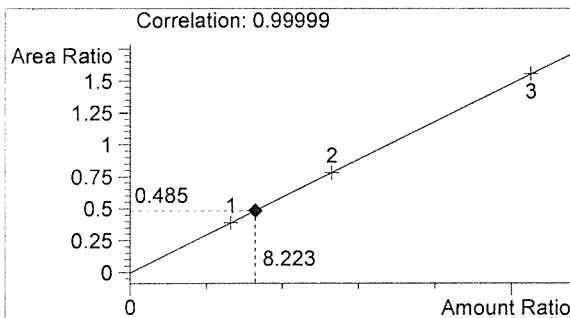

Ethanol 0.099 g/100mL

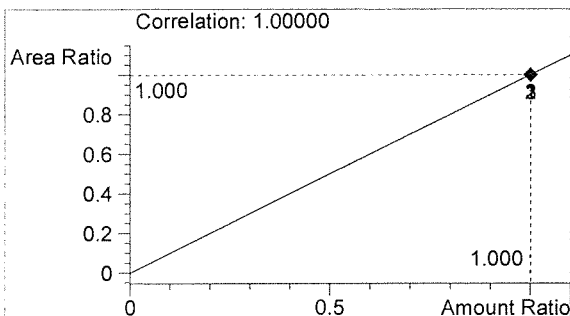

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten signature


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:29:18 PM
 Instrument: HSGC#1
 Column: DB-ALC1


Sample Name: 16018-2
 Operator: Amanda Chandler
 Location: Vial 18

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

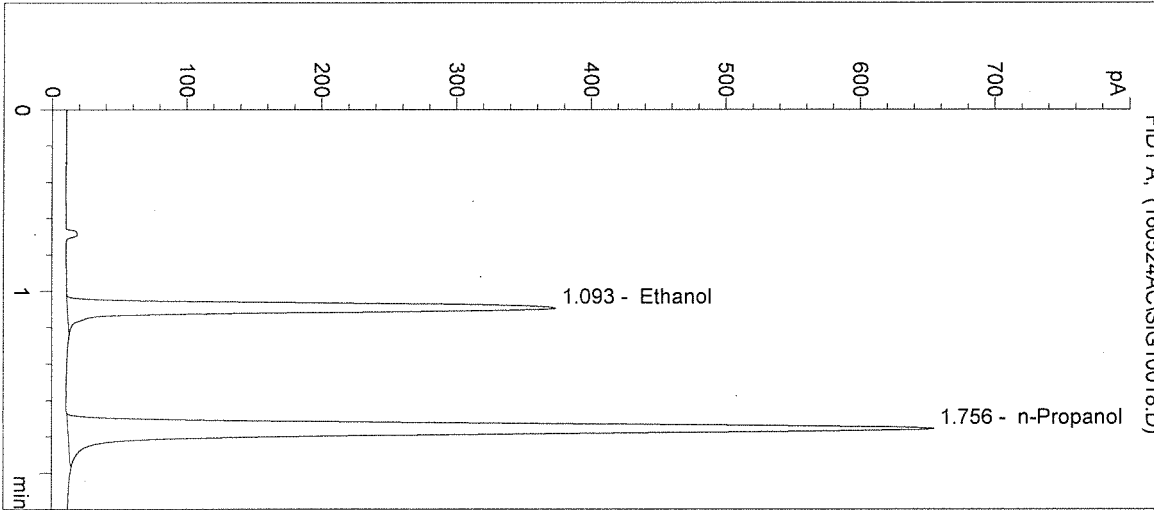

#	Compound	Peak Area	RT (min)
1	Ethanol	1231	1.093
2	n-Propanol	2543	1.756

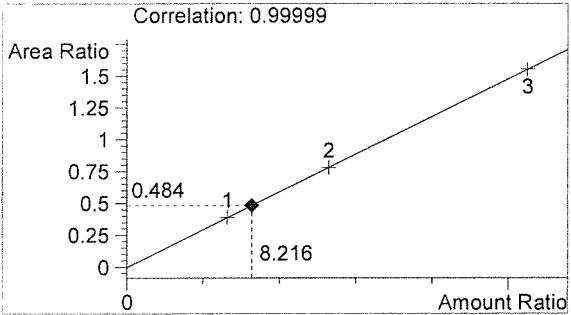

Ethanol 0.099 g/100mL

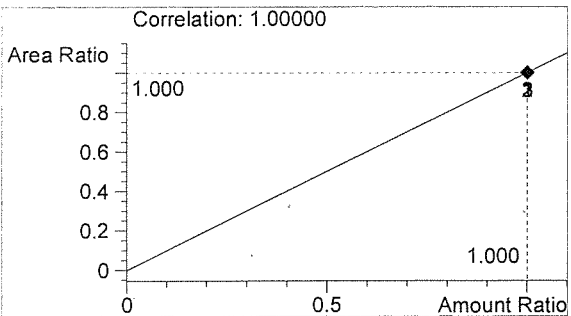

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten initials AR


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:32:31 PM
 Instrument: HSGC#1
 Column: DB-ALC1


Sample Name: 16018-3
 Operator: Amanda Chandler
 Location: Vial 19

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

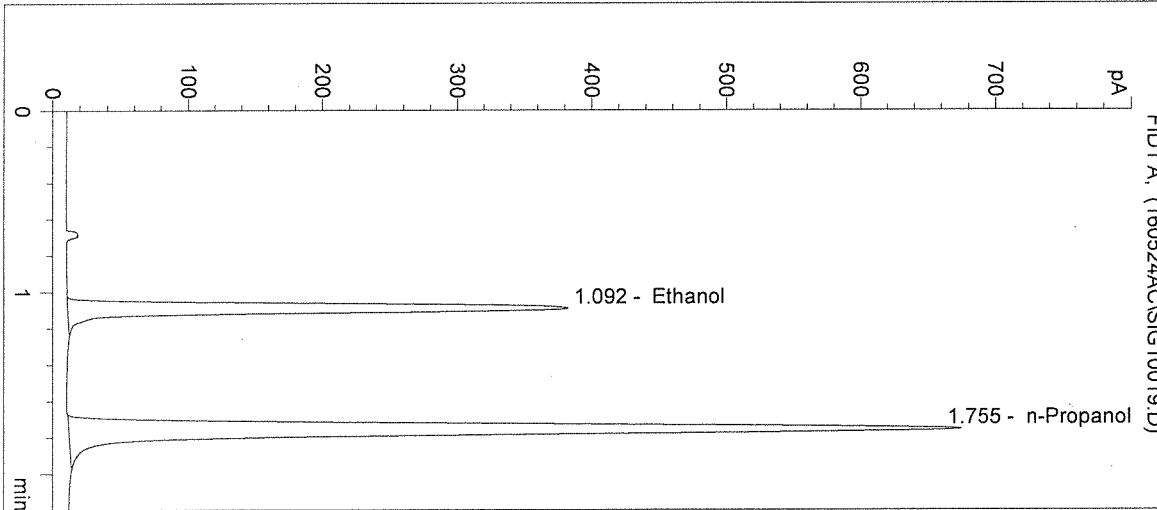

#	Compound	Peak Area	RT (min)
1	Ethanol	1265	1.092
2	n-Propanol	2616	1.755

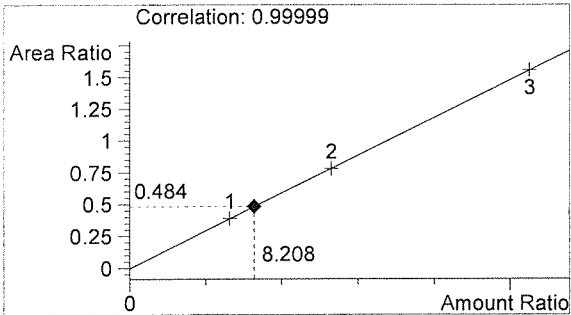

Ethanol 0.098 g/100mL

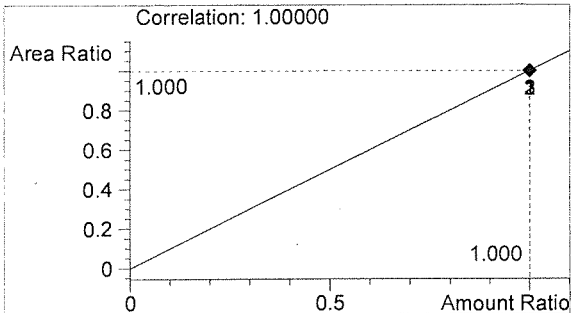

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten initials 'AR'

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:35:44 PM

Sample Name: 16018-4

Instrument: HSGC#1


Operator: Amanda Chandler

Column: DB-ALC1


Location: Vial 20

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

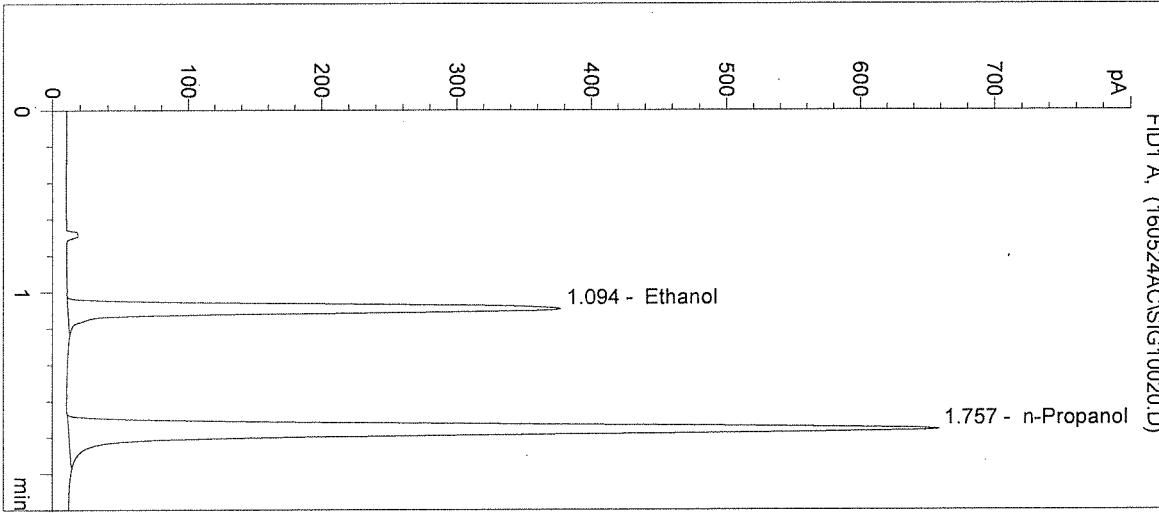

#	Compound	Peak Area	RT (min)
1	Ethanol	1241	1.094
2	n-Propanol	2556	1.757

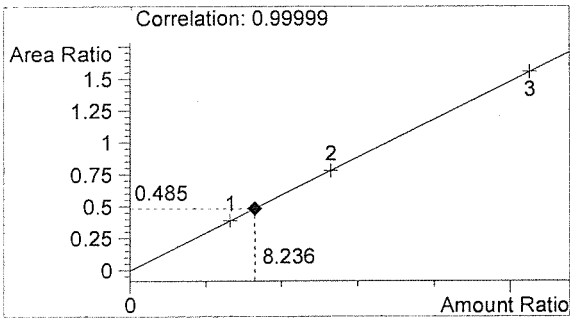

Ethanol 0.099 g/100mL

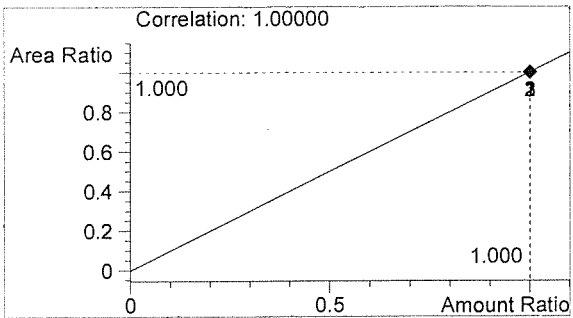

n-Propanol 0.012 g/100mL

fr

AR

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:38:58 PM

Sample Name: 16018-5

Instrument: HSGC#1


Operator: Amanda Chandler

Column: DB-ALC1


Location: Vial 21

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

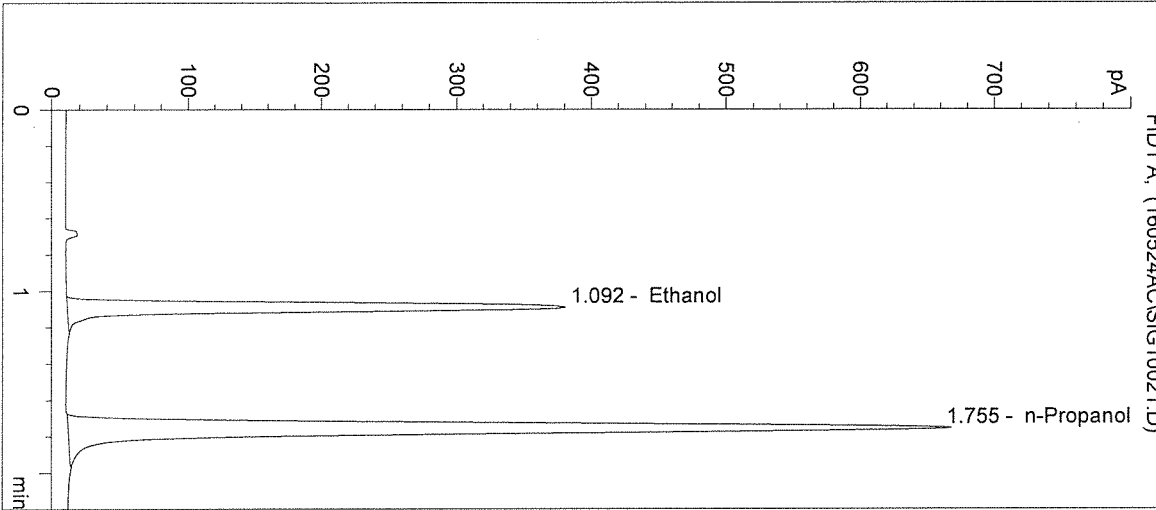

#	Compound	Peak Area	RT (min)
1	Ethanol	1252	1.092
2	n-Propanol	2583	1.755

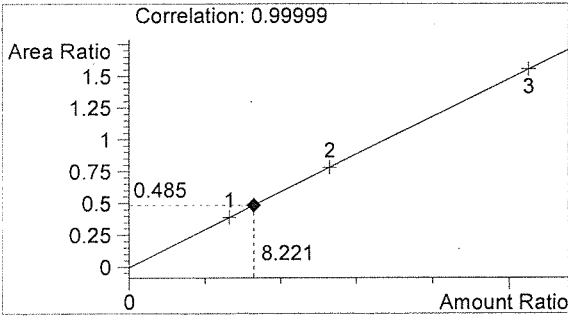

Ethanol 0.099 g/100mL

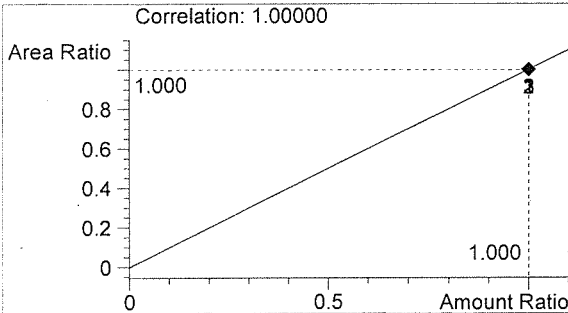

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten initials

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:42:11 PM

Sample Name: 0.10 CTRL

Instrument: HSGC#1.


Operator: Amanda Chandler

Column: DB-ALC1


Location: Vial 22

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: 16018

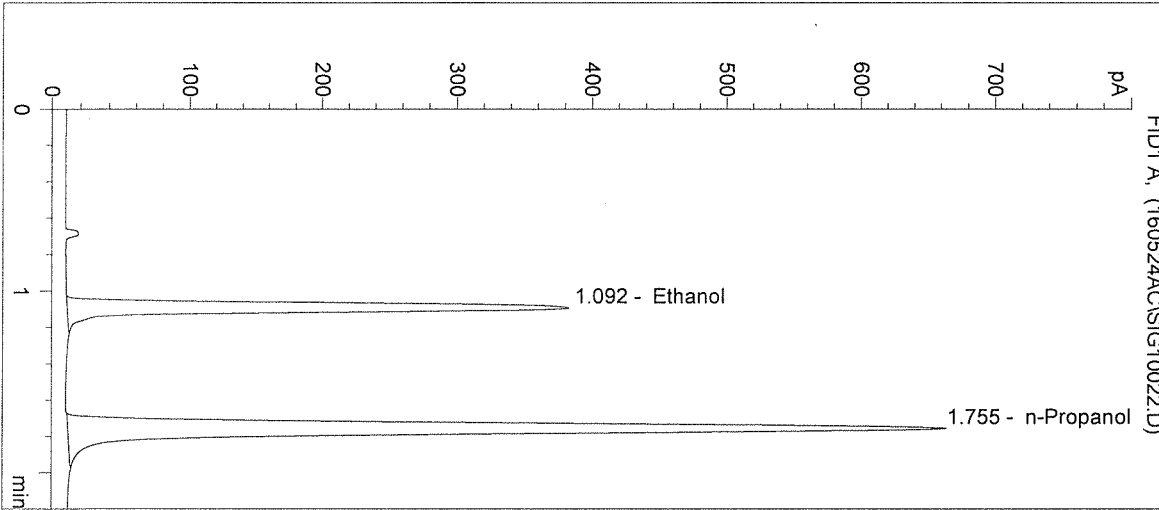

#	Compound	Peak Area	RT (min)
1	Ethanol	1263	1.092
2	n-Propanol	2575	1.755

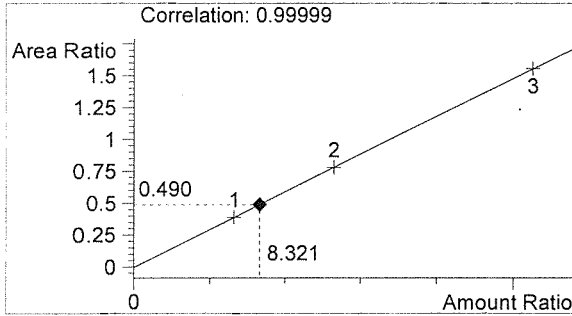

Ethanol 0.100 g/100mL

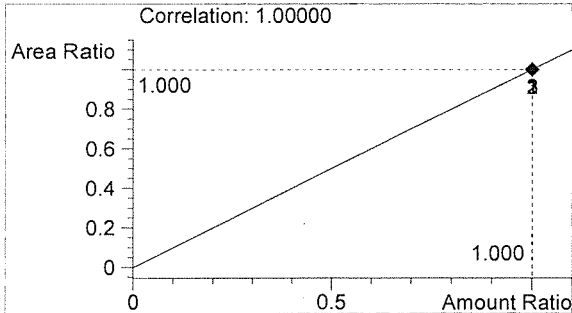

n-Propanol 0.012 g/100mL

fr

AC

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/24/2016 1:45:24 PM

Sample Name: NEG CTRL

Instrument: HSGC#1


Operator: Amanda Chandler

Column: DB-ALC1


Location: Vial 23

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: 16018

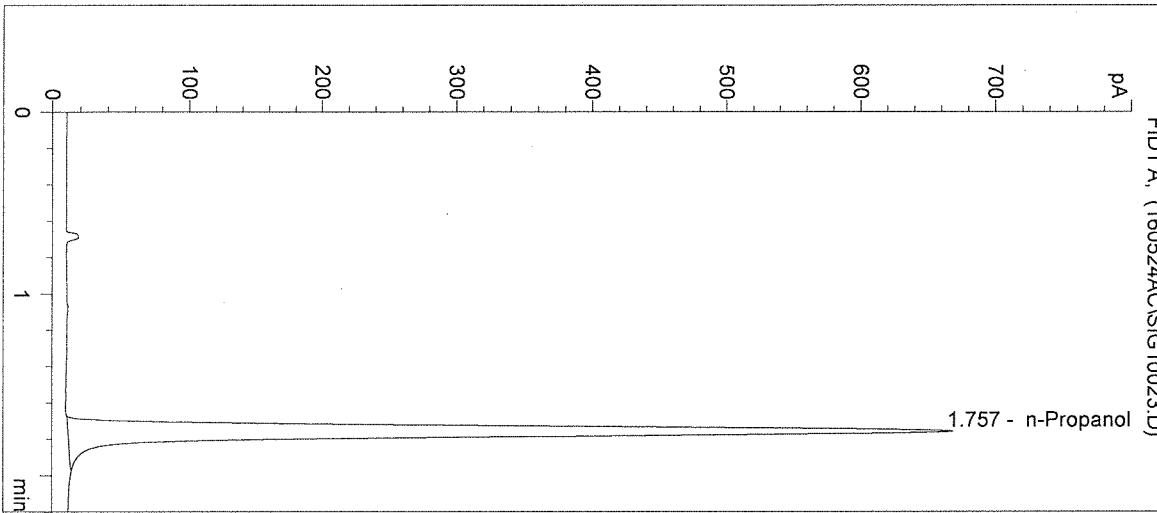

#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2605	1.757

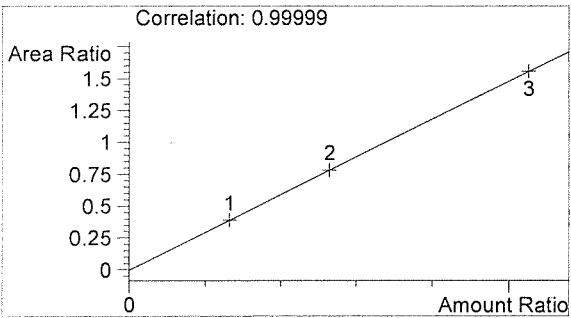

Ethanol 0.000 g/100mL

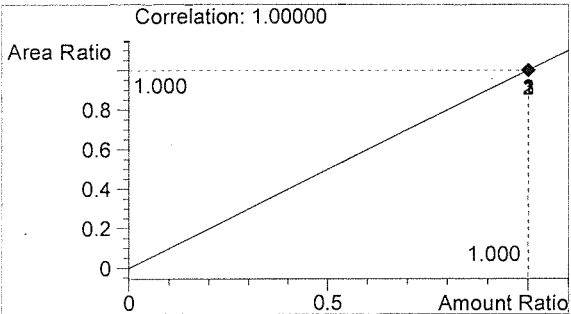

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten signature

Sequence Parameters:

Operator: Katie Harris
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 160527KH
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

Ethanol Calibrator 1, E0416-01 - Exp. 10/01/2016
 Ethanol Calibrator 2, E0416-02 - Exp. 10/01/2016
 Ethanol Calibrator 3, E0416-03 - Exp. 10/01/2016
 CTRL1 (0.04g/100mL), Lot # FN05011301 - Exp. 05/2018
 CTRL2 (0.10g/100mL), Lot # FN08051301 - Exp. 10/2018
 CTRL3 (0.20g/100mL), Lot # FN03211401 - Exp. 06/2019
 Internal Standard Lot#P0316 - Exp. 06/29/2016

Calibration vials 1-9 filed with 16017.

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	NEG CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	NEG CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	16017-1	SIMALC1	1	Sample		
11	Vial 11	16017-2	SIMALC1	1	Sample		
12	Vial 12	16017-3	SIMALC1	1	Sample		
13	Vial 13	16017-4	SIMALC1	1	Sample		
14	Vial 14	16017-5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	NEG CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	16018-1	SIMALC1	1	Sample		
18	Vial 18	16018-2	SIMALC1	1	Sample		
19	Vial 19	16018-3	SIMALC1	1	Sample		
20	Vial 20	16018-4	SIMALC1	1	Sample		
21	Vial 21	16018-5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	NEG CTRL	SIMALC1	1	Ctrl Samp		
24	Vial 24	16019-1	SIMALC1	1	Sample		
25	Vial 25	16019-2	SIMALC1	1	Sample		
26	Vial 26	16019-3	SIMALC1	1	Sample		

16018

fn0113/16

KH

Sequence: C:\HPCHEM\1\SEQUENCE\KHQAP.S

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
27	Vial 27	16019-4	SIMALC1	1	Sample		
28	Vial 28	16019-5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL	SIMALC1	1	Ctrl Samp		
30	Vial 30	NEG CTRL	SIMALC1	1	Ctrl Samp		
31	Vial 31	16020-1	SIMALC1	1	Sample		
32	Vial 32	16020-2	SIMALC1	1	Sample		
33	Vial 33	16020-3	SIMALC1	1	Sample		
34	Vial 34	16020-4	SIMALC1	1	Sample		
35	Vial 35	16020-5	SIMALC1	1	Sample		
36	Vial 36	0.10 CTRL	SIMALC1	1	Ctrl Samp		
37	Vial 37	NEG CTRL	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

16018

For 6/13/16

KN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/27/2016 12:17:36 PM

Sample Name: 16018-1

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 17

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

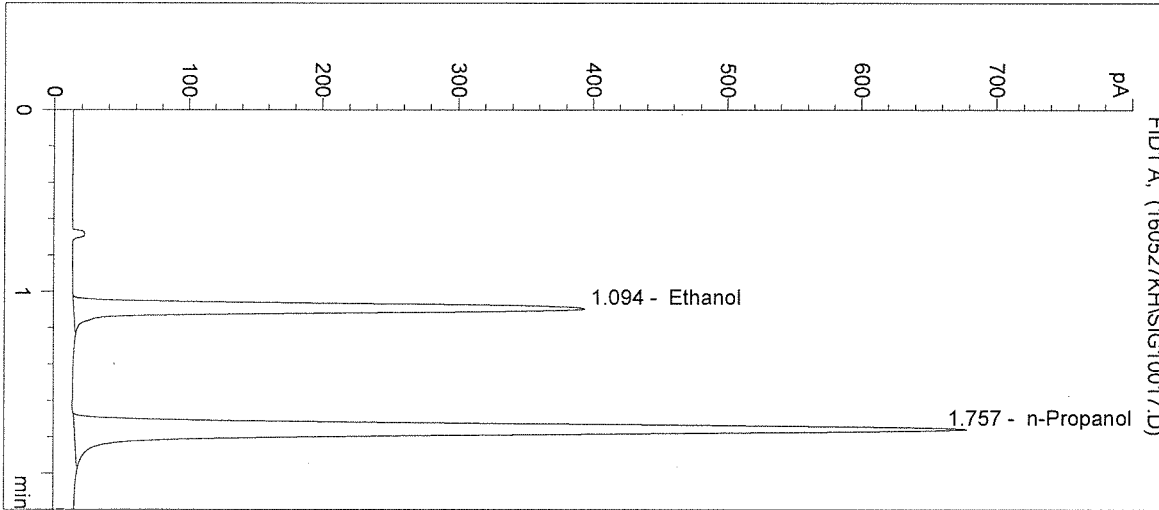

#	Compound	Peak Area	RT (min)
1	Ethanol	1305	1.094
2	n-Propanol	2632	1.757

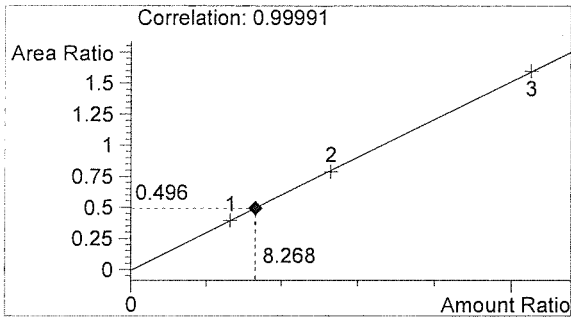

Ethanol 0.099 g/100mL

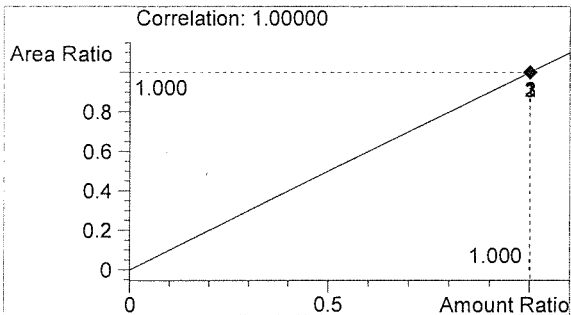

n-Propanol 0.012 g/100mL


fr

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 5/27/2016 12:20:49 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: 16018-2
 Operator: Katie Harris
 Location: Vial 18


Sample Info:

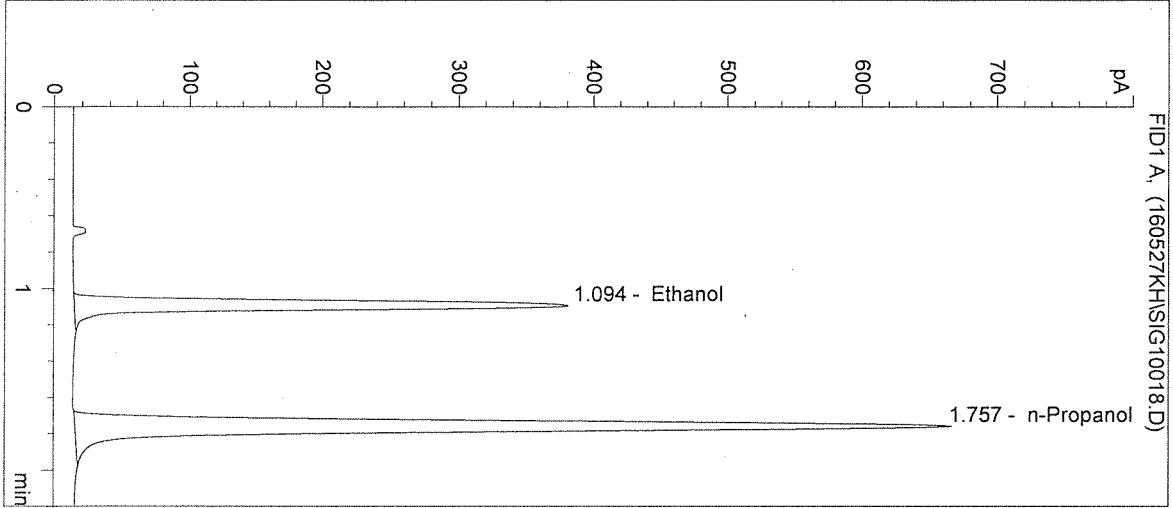

#	Compound	Peak Area	RT (min)
1	Ethanol	1263	1.094
2	n-Propanol	2595	1.757

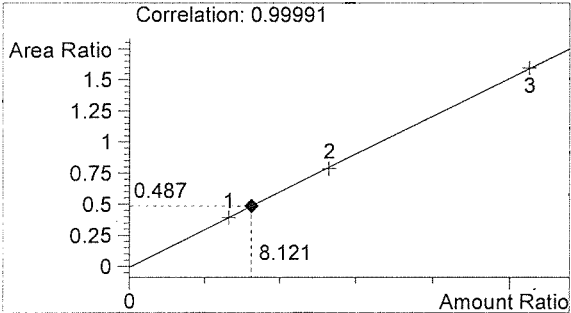

Ethanol 0.097 g/100mL

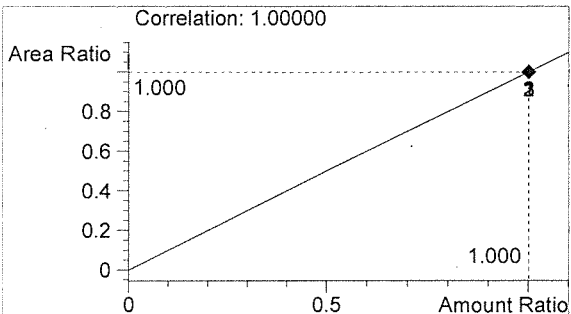

n-Propanol 0.012 g/100mL

Handwritten signature


KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 5/27/2016 12:24:02 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: 16018-3
 Operator: Katie Harris
 Location: Vial 19


Sample Info:

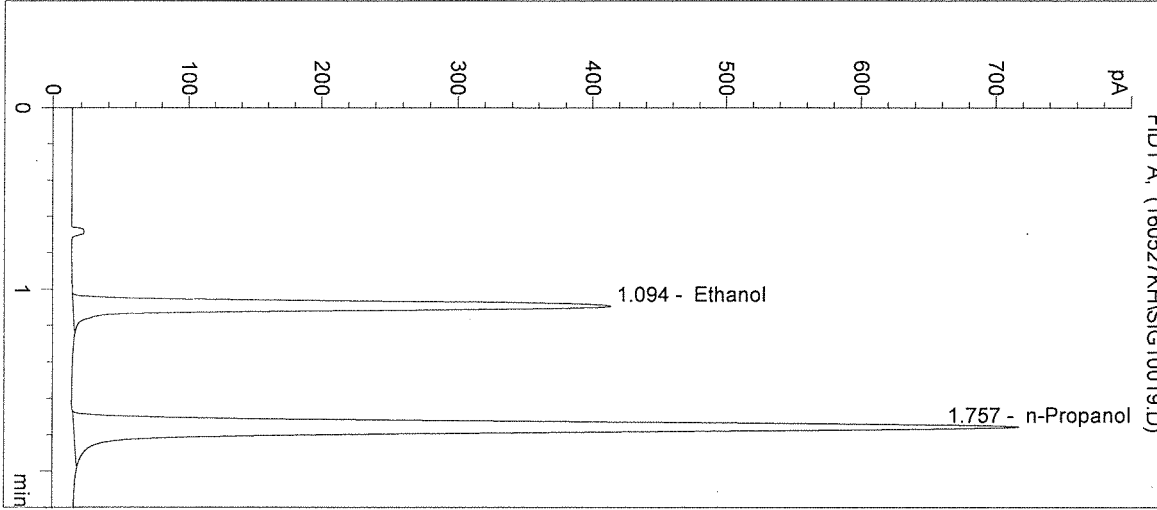

#	Compound	Peak Area	RT (min)
1	Ethanol	1377	1.094
2	n-Propanol	2794	1.757

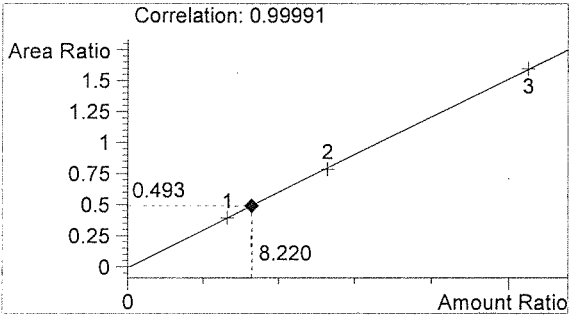

Ethanol 0.099 g/100mL

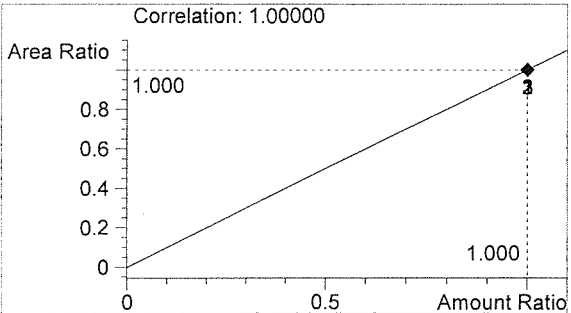


n-Propanol 0.012 g/100mL

Handwritten signature


KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 5/27/2016 12:27:15 PM Sample Name: 16018-4
 Instrument: HSGC#1 Operator: Katie Harris
 Column: DB-ALC1 Location: Vial 20
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info:

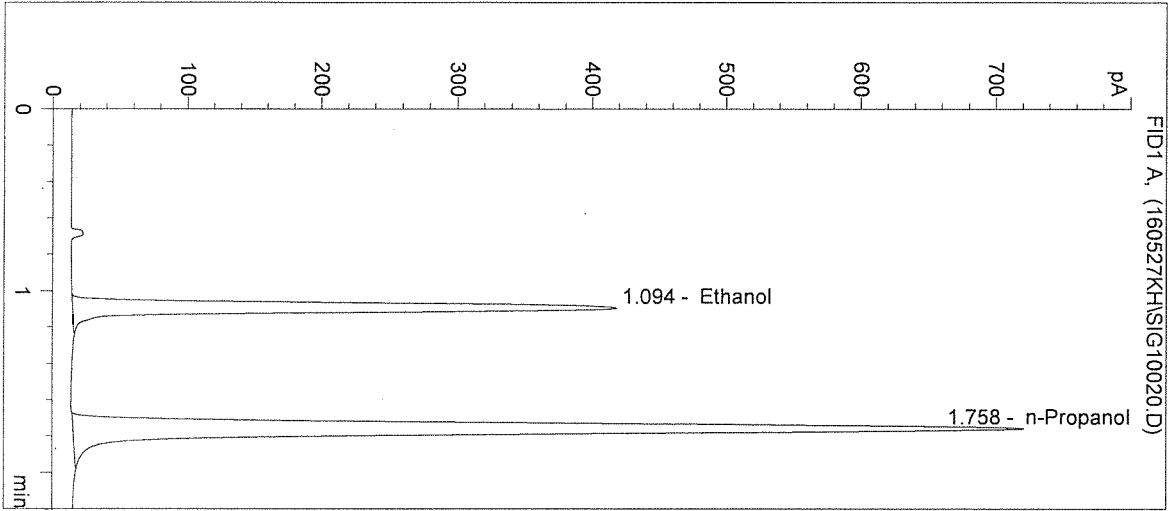

#	Compound	Peak Area	RT (min)
1	Ethanol	1395	1.094
2	n-Propanol	2807	1.758

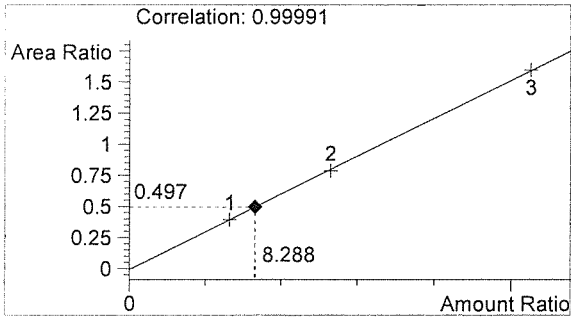

Ethanol 0.099 g/100mL

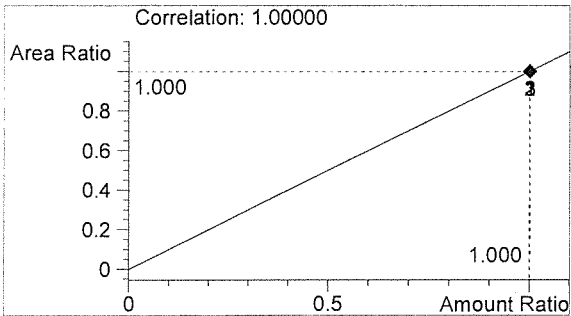

n-Propanol 0.012 g/100mL

Handwritten signature

Handwritten initials

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/27/2016 12:30:29 PM

Sample Name: 16018-5

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 21

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info:

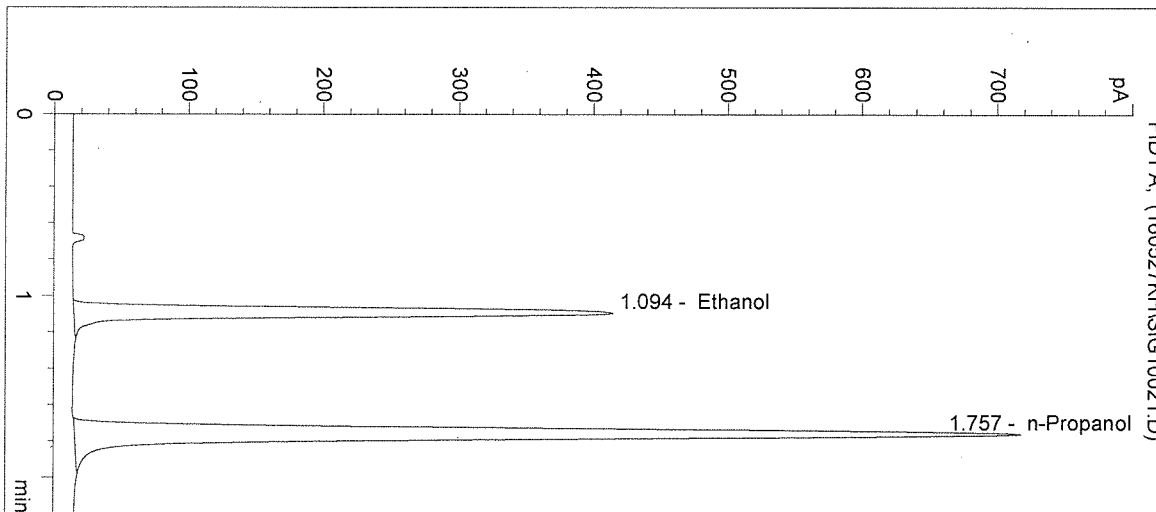

#	Compound	Peak Area	RT (min)
1	Ethanol	1381	1.094
2	n-Propanol	2797	1.757

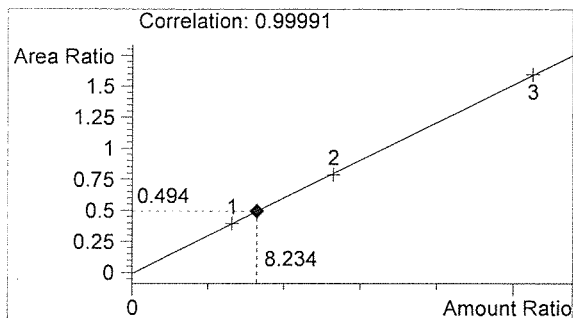

Ethanol 0.099 g/100mL

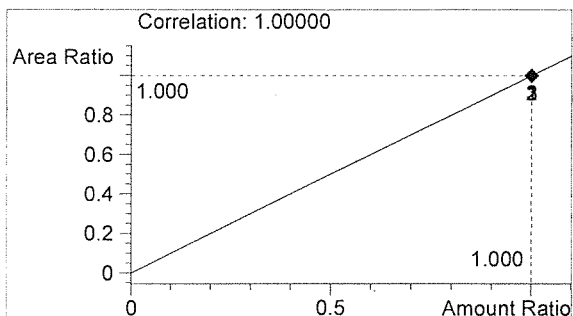

n-Propanol 0.012 g/100mL

Handwritten signature

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/27/2016 12:33:42 PM

Sample Name: 0.10 CTRL

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 22

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: 16018

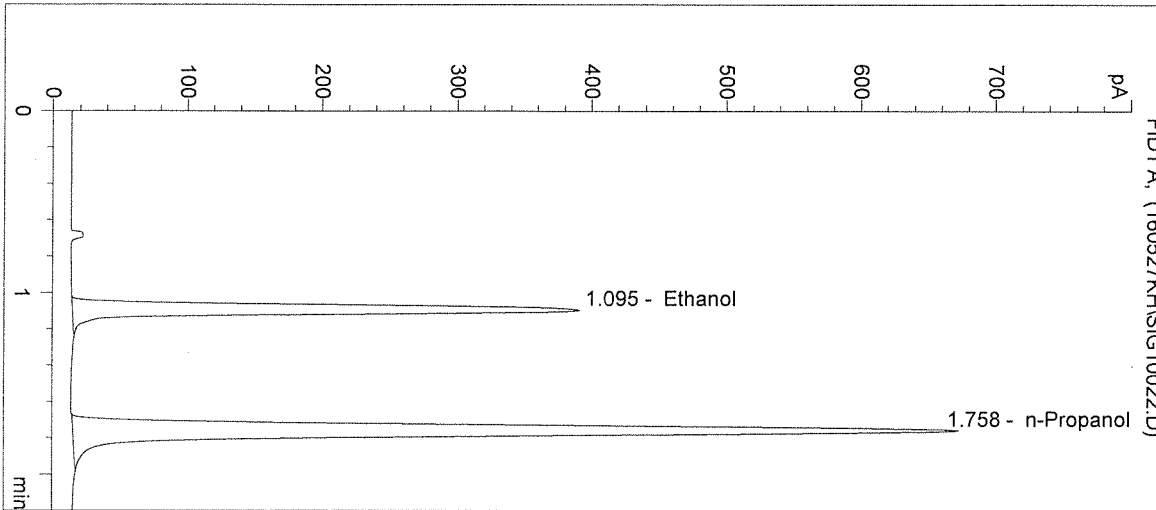

#	Compound	Peak Area	RT (min)
1	Ethanol	1301	1.095
2	n-Propanol	2625	1.758

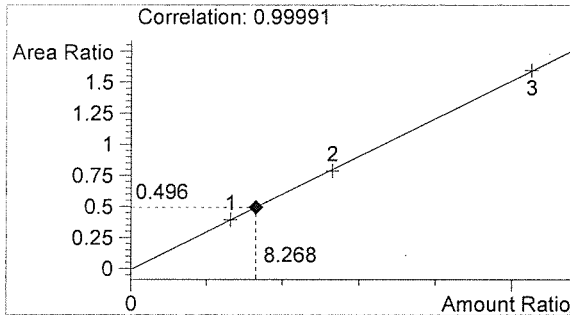

Ethanol 0.099 g/100mL

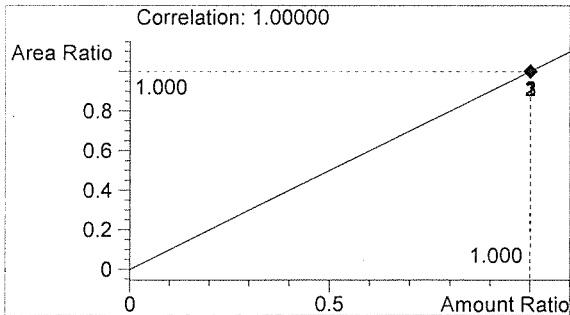

n-Propanol 0.012 g/100mL

Handwritten signature

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 5/27/2016 12:36:55 PM

Sample Name: NEG CTRL

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 23

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: 16018

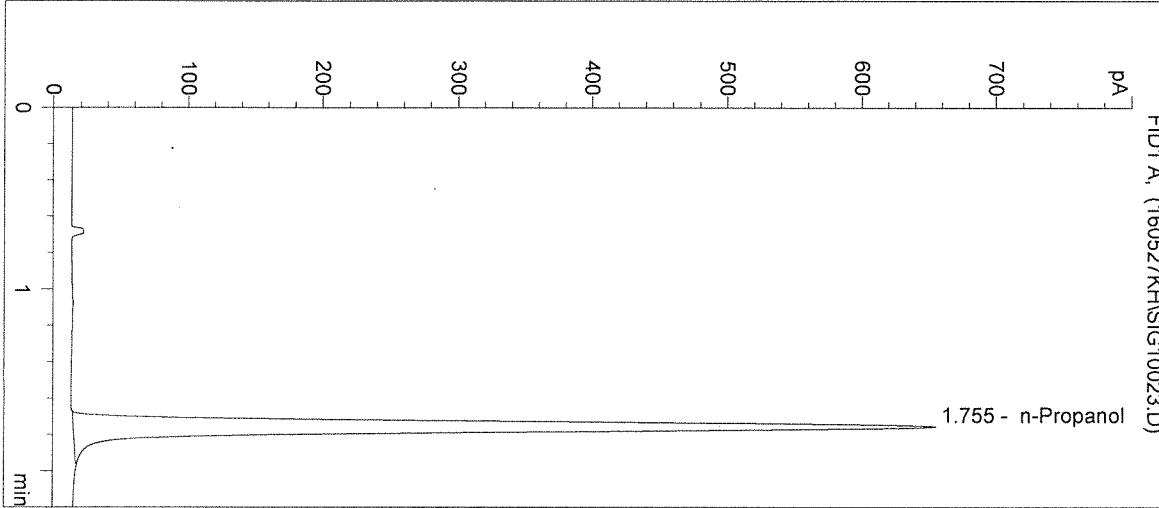

#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2539	1.755

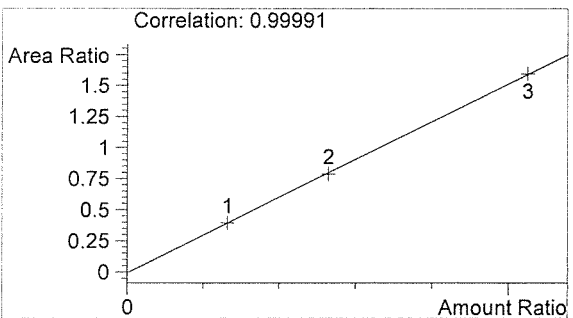

Ethanol 0.000 g/100mL

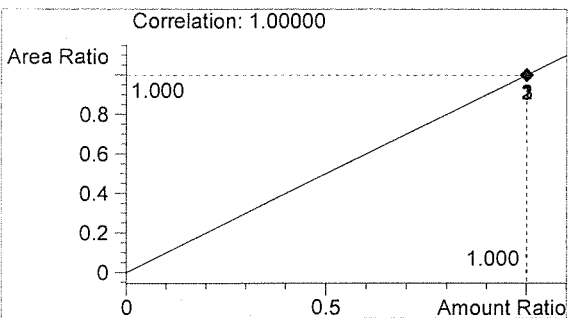

n-Propanol 0.012 g/100mL

Handwritten signature

KH