



QUALITY ASSURANCE PROCEDURE SOLUTION TEST REPORT

BATCH REPORT: 17007

CUSTOMER INFORMATION

Washington State Patrol – Breath Test Program
811 East Roanoke SEATTLE, WA 98102

TESTING PROCEDURE USED: TLD Technical Manual, Chapter 4.0 Certification of Simulator Solutions;
Headspace-Gas Chromatography.

TESTING ITEM INFORMATION

TARGET VAPOR CONCENTRATION: 0.20 g/210L
DATE PREPARED: 01/15/2017
BATCH UNITS: g/100mL

IDENTITY: QAP Solution
PREPARED BY: Brittany Thomas

	BT	KH	DN
1	0.251	0.253	0.253
2	0.250	0.250	0.257
3	0.251	0.251	0.255
4	0.250	0.253	0.252
5	0.250	0.253	0.256
C	0.101	0.100	0.103

ETHANOL CONTROL INFORMATION

LOT NUMBER: FN08051301 EXPIRATION: 10/2018 CONCENTRATION: 0.10 g/100mL

RESULTS OF TESTING

AVERAGE SOLUTION CONCENTRATION: 0.2523 g/100mL PRECISION CV (%): 0.89
STANDARD DEVIATION: 0.00226 NUMBER OF TESTS: 15

EQUIVALENT VAPOR CONCENTRATION: **0.2051 g/210L**
EXPANDED UNCERTAINTY: ± 0.0056 (k=2, 95.45% confidence interval)

WASHINGTON STATE PATROL – TOXICOLOGY LABORATORY DIVISION

Brianne E. O'Reilly

Brianne E. O'Reilly Technical Lead

2-1-2017

DATE REPORT ISSUED

ANALYST	NAME	THIS TESTING WAS PERFORMED BY:	
		SIGNATURE	DATE TESTED
BT	Brittany Thomas	<i>Brittany Thomas</i>	01/15/2017
KH	Katie Harris	<i>Katie Harris</i>	01/15/2017
DN	David Nguyen	<i>David Nguyen</i>	01/17/2017

SIMULATOR SOLUTION DATA ENTRY REVIEW

Reviewer/s: Amanda M. Black Date: 2-2-17

Location: WSP-FLSB Seattle, WA Solution Batch Number: 17007

	YES	NO	N/A
Analysis dates do not precede preparation date:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Declarations signed and properly dated:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Data entry corresponds to all chromatograms:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
All signatures present on Test Report:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Average solution concentration correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Standard deviation correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
CV (%) correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Equivalent vapor concentration correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
All chromatograms and sequences included in file:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ethanol control information present: (lot # present & used within expiration)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Complies with accuracy and precision requirements established by the State Toxicologist:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Comments:

Reviewer Signature:  Date: 2-2-17

Washington State Patrol - Toxicology Laboratory Division
QAP Test Report Calculation Record

QAP Solution Batch #: 17007

Date Prepared: 1/15/2017

Analyst:	BT	KH	DN
Date Tested:	1/15/2017	1/15/2017	1/17/2017
Instrument:	HSGC 1	HSGC 1	HSGC 1
1	0.251	0.253	0.253
2	0.250	0.250	0.257
3	0.251	0.251	0.255
4	0.250	0.253	0.252
5	0.250	0.253	0.256
C	0.101	0.100	0.103

CV^2_{COA}	$CV^2_{QAP\ Solution}$	$CV^2_{Control}$	$CV^2_{Part\ Coef}$
0.000084100	0.000053349	0.0000757445	0.0001016326

Ethanol Control Lot #: FN08051301
Control Uncertainty (%): 0.29

Average Solution Concentration: 0.2523 g/100mL
Standard Deviation: 0.00226 g/100mL
Precision CV (%): 0.89
Equivalent Vapor Concentration: 0.2051 g/210L
Combined Standard Uncertainty (\pm): 0.0028 g/210L
Expanded Uncertainty (\pm): 0.0056 coverage factor (k) = 2 (95.45% level of confidence)

Calculations performed by: Brianne E. O'Reilly Brianne E. O'Reilly 1-31-2017
Name Signature Date

Calculations verified by: Amanda M. Black [Signature] 2-2-17
Name Signature Date

Method: Hand calculation

Tech. review performed by: Brianne E. O'Reilly Brianne E. O'Reilly 1-31-2017
Name Signature Date

SOLUTION CERTIFICATE REVIEW

Please check that the data on your chromatograms is the data entered into the Test Report, that the date to the right of your name is the date that you tested the solution, and then sign the Test Report.

Please initial and date below to affirm that you have:

- 1) Checked your data
- 2) Checked the date to the right of your name on the Test Report
- 3) Signed the Test Report

	Initials	Date
Amanda Chandler		
Andrew Gingras		
Asa Louis		
Brittany Thomas	BT	2/11/17
Christie Mitchell-Mata		
Christopher Johnston		
David Nguyen	DN	2/11/17
Dawn Sklerov		
Elizabeth Wehner		
Justin Knoy		
Katie Harris	KH	2/11/17
Lyndsey Knoy		
Naziha Nuwayhid		
Rebecca Flaherty		

Batch # 17007
Buo 1-31-17

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.20 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 17007**

I, Brittany Thomas, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Biology and a Masters in Forensic Science.

The quality assurance procedure (QAP) solution, Lot Number 17007, was prepared in the Washington State Toxicology Laboratory on 1/15/2017. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 1/15/2018.

Seattle, WA

 2/1/17

Brittany Thomas

Date

Forensic Scientist

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.20 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 17007**

I, Katie Harris, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS in Biochemistry and MS degree in Forensic Science.

The quality assurance procedure (QAP) solution, Lot Number 17007, was prepared in the Washington State Toxicology Laboratory on 1/15/2017. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 1/15/2018.

Seattle, WA

Katie Harris 2/1/17

Katie Harris

Date

Forensic Scientist

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.20 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 17007**


I, David Nguyen, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Chemistry.

The quality assurance procedure (QAP) solution, Lot Number 17007, was prepared in the Washington State Toxicology Laboratory on 1/15/2017. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 1/15/2018.

Seattle, WA

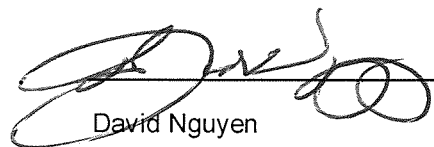 - 2/1/17
Date

David Nguyen
Forensic Scientist

FILE A COPY IN THE BATCH FILE FOR EACH SOLUTION LISTED ON THE WORKSHEET

Preparation Date: 1/15/2017 Expiration Date: 1/15/2018 Initials of Preparer: BT

Lot # of 200-proof Ethanol used in preparation: 2FE0139

Date the 200-proof Ethanol bottle was opened: 1/7/17

After opening, each bottle of 200-proof Ethanol is approved for use for 6 months unless an extension is approved by the State Toxicologist. This timeframe applies to the 200-proof Ethanol only, not to simulator solutions which have a 1 year expiration.

Environmental conditions verified as acceptable:

Simulator Solution	Volume of Ethanol (mL)	Volume of Deionized Water (L)		Batch Number
QAP 0.04	11.2	18	<input type="checkbox"/>	
QAP 0.08	22.4	18	<input checked="" type="checkbox"/>	<u>17009</u>
QAP 0.10	28.1	18	<input type="checkbox"/>	
QAP 0.15	42.1	18	<input checked="" type="checkbox"/>	<u>17008</u>
QAP 0.20	56.1	18	<input checked="" type="checkbox"/>	<u>17007</u>
ESS	66.5	52	<input type="checkbox"/>	

Stir bar is rotating

Stirred for minimum 30 minutes; 2 hours for ESS

Spigot purged

Aliquot taken

Batch labeled, packaged and sealed

1/15/17
Date

If different ethanol lot numbers are used in the preparation of solutions, record them and the corresponding solution batch numbers in the comments section.

Comments: more than two values out for batch 17008
Batch not bottled or used for calibration activities (disposed)
BT 1/18/17

William Cronas
Analyst Signature

1/15/17
Date

Sequence Parameters:

Operator: Brittany Thomas
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 170115BT
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

CAL 1 (0.079g/100mL) - LOT# E0915¹⁰-01 - EXP 3/15/2017
 CAL 2 (0.158g/100mL) - LOT# E0915¹⁰-02 - EXP 3/15/2017 BT 1/21/17
 CAL 3 (0.316g/100mL) - LOT# E0915¹⁰-03 - EXP 3/15/2017 BT 1/31/17
 CTRL 1 (0.04g/100mL) - LOT# FN12181501 - EXP 12/2020
 CTRL 2 (0.10g/100mL) - LOT# FN08051301 - EXP 10/2018
 CTRL 3 (0.20g/100mL) - LOT# FN08101505 - EXP 02/2021
 n-Propanol ISTD - LOT# P1116 - Exp 02/23/2017

Standard data located in Batch File 17007

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	NEG CTRL-BT	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL-BT	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL-BT	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL-BT	SIMALC1	1	Ctrl Samp		
9	Vial 9	NEG CTRL-BT	SIMALC1	1	Ctrl Samp		
10	Vial 10	QAP0.20 17007 #1	SIMALC1	1	Sample		
11	Vial 11	QAP0.20 17007 #2	SIMALC1	1	Sample		
12	Vial 12	QAP0.20 17007 #3	SIMALC1	1	Sample		
13	Vial 13	QAP0.20 17007 #4	SIMALC1	1	Sample		
14	Vial 14	QAP0.20 17007 #5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL-BT	SIMALC1	1	Ctrl Samp		
16	Vial 16	NEG CTRL-BT	SIMALC1	1	Ctrl Samp		
17	Vial 17	QAP0.15 17008 #1	SIMALC1	1	Sample		
18	Vial 18	QAP0.15 17008 #2	SIMALC1	1	Sample		
19	Vial 19	QAP0.15 17008 #3	SIMALC1	1	Sample		
20	Vial 20	QAP0.15 17008 #4	SIMALC1	1	Sample		
21	Vial 21	QAP0.15 17008 #5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL-BT	SIMALC1	1	Ctrl Samp		
23	Vial 23	NEG CTRL-BT	SIMALC1	1	Ctrl Samp		
24	Vial 24	QAP0.08 17009 #1	SIMALC1	1	Sample		
25	Vial 25	QAP0.08 17009 #2	SIMALC1	1	Sample		
26	Vial 26	QAP0.08 17009 #3	SIMALC1	1	Sample		

17007
 Rev 1-31-17

BT

Sequence: C:\HPCHEM\1\SEQUENCE\BTQAP1.S

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
27	Vial 27	QAP0.08 17009 #4	SIMALC1	1	Sample		
28	Vial 28	QAP0.08 17009 #5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL-BT	SIMALC1	1	Ctrl Samp		
30	Vial 30	NEG CTRL-BT	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

17007
Paw 1-31-17

POT

=====
 Calibration Table
 =====

Calib. Data Modified : Sunday, January 15, 2017 9:29:40 AM

Calculate : Internal Standard
 Based on : Peak Area

Rel. Reference Window : 5.000 %
 Abs. Reference Window : 0.050 min
 Rel. Non-ref. Window : 5.000 %
 Abs. Non-ref. Window : 0.050 min
 Multiplier : 1.0000
 Dilution : 1.0000
 Sample Amount : 0.00000

Use Multiplier & Dilution Factor with ISTDs
 Uncalibrated Peaks : not reported
 Partial Calibration : No recalibration if peaks missing

Curve Type : Linear
 Origin : Included
 Weight : Equal

Recalibration Settings:
 Average Response : No Update
 Average Retention Time: No Update

Calibration Report Options :
 Printout of recalibrations within a sequence:
 Normal Report after Recalibration

Sample ISTD Information:

ISTD #	ISTD Amount [g/100mL]	Name
1	1.20000e-2	n-Propanol

Signal 1: FID1 A,

RetTime [min]	Lvl Sig	Amount [g/100mL]	Area	Amt/Area	Ref Grp	Name
1.087	1	8.00100e-2	1097.95911	7.28716e-5	1	Ethanol
		1.61200e-1	2155.49683	7.47855e-5		
		3.21790e-1	4286.22510	7.50754e-5		
1.766	1	1.20000e-2	3063.40967	3.91720e-6	I1	n-Propanol
		1.20000e-2	2979.51172	4.02751e-6		
		1.20000e-2	3091.99170	3.88099e-6		


=====
 Peak Sum Table
 =====

No Entries in table
 =====


17007
 RW1/31/17

WOT

=====
Calibration Curves
=====

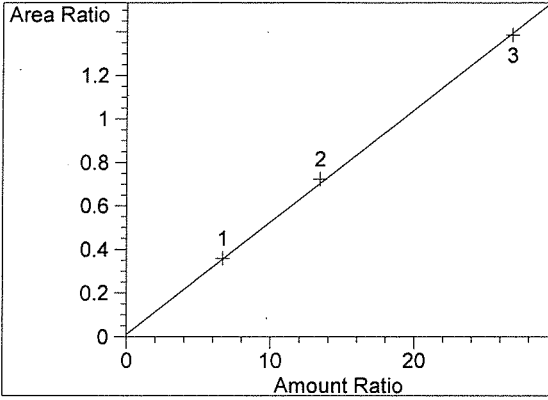

Ethanol at exp. RT: 1.087
FID1 A,
Correlation: 0.99973
Residual Std. Dev.: 0.01692
Formula: $y = mx + b$
m: 5.16436e-2
b: 1.12851e-2
x: Amount Ratio
y: Area Ratio

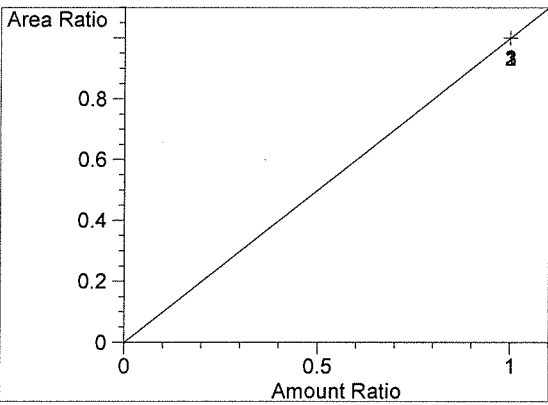

n-Propanol at exp. RT: 1.766
FID1 A,
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

= 17007
PLU 1/31/17

DOT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:17:35 AM

Sample Name: BLANK

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 1

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

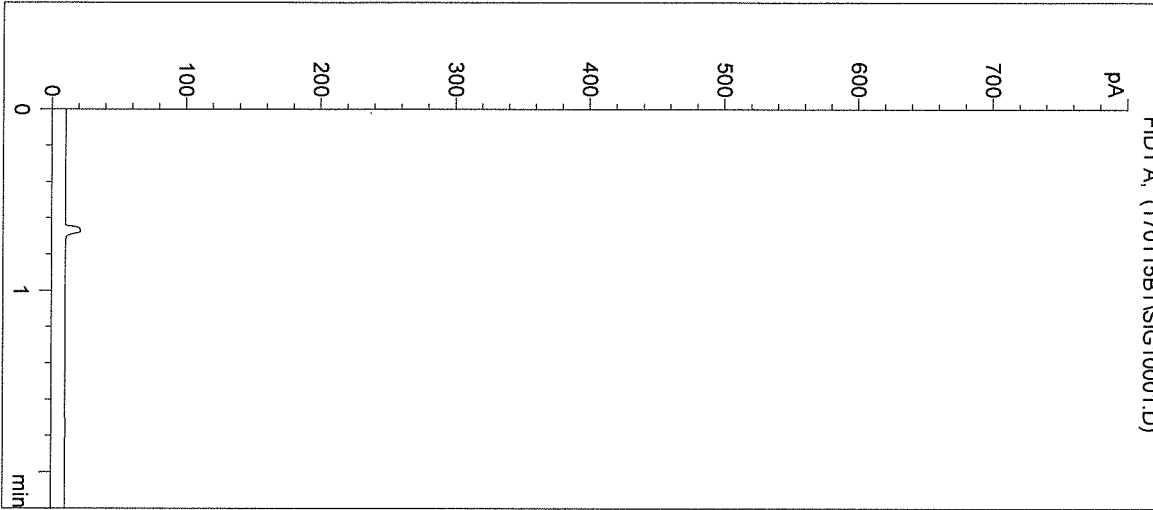


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	0	0.000



Ethanol 0.000 g/100mL

BLU



n-Propanol 0.000 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:20:55 AM

Sample Name: 0.079 CAL 1

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 2

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

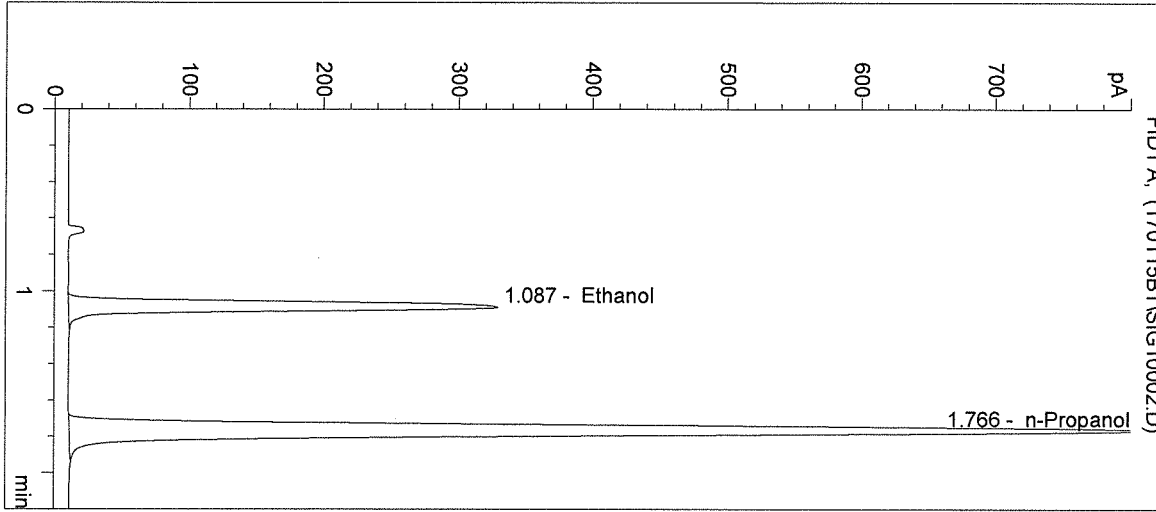


#	Compound	Peak Area	RT (min)
1	Ethanol	1098	1.087
2	n-Propanol	3063	1.766

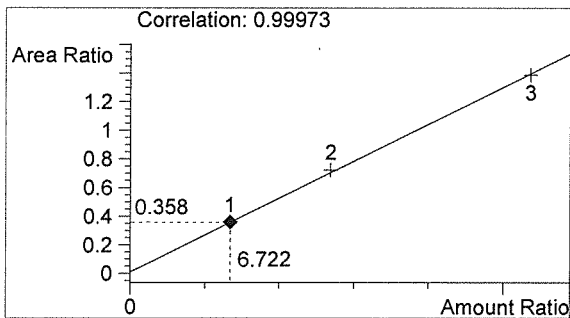

Ethanol 0.081 g/100mL

AWO

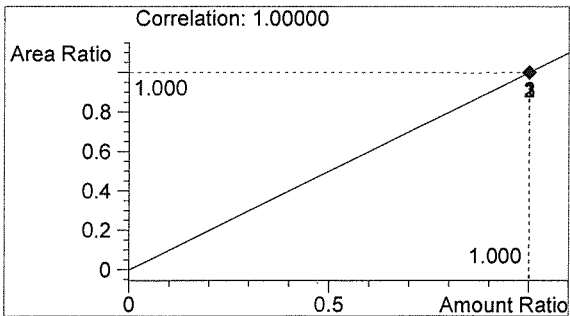

n-Propanol 0.012 g/100mL

MT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:24:10 AM

Sample Name: 0.158 CAL 2

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 3

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

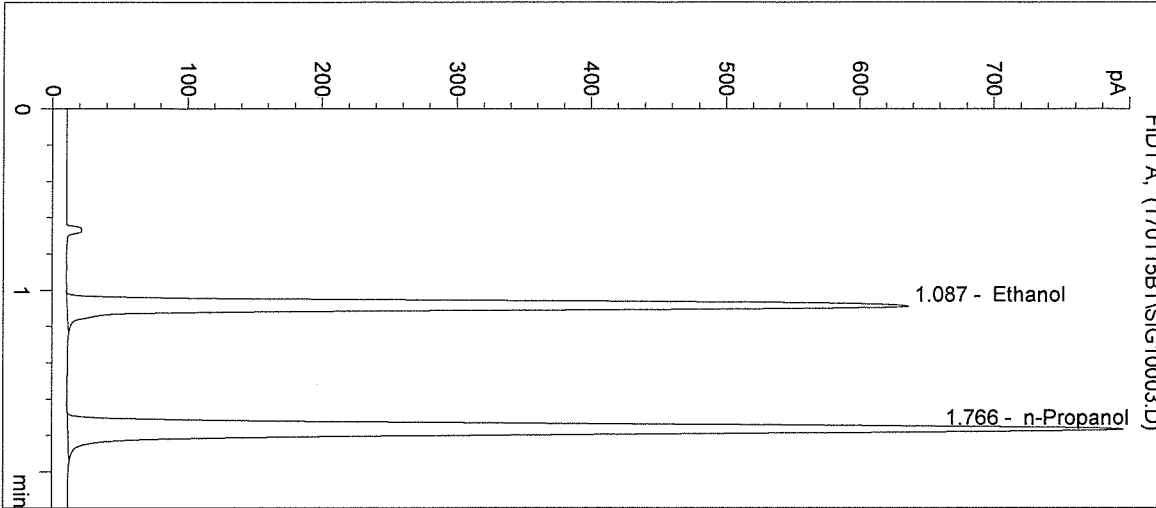


#	Compound	Peak Area	RT (min)
1	Ethanol	2155	1.087
2	n-Propanol	2980	1.766

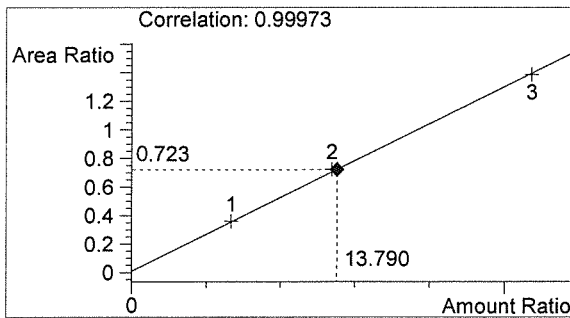

Ethanol 0.165 g/100mL

AWO

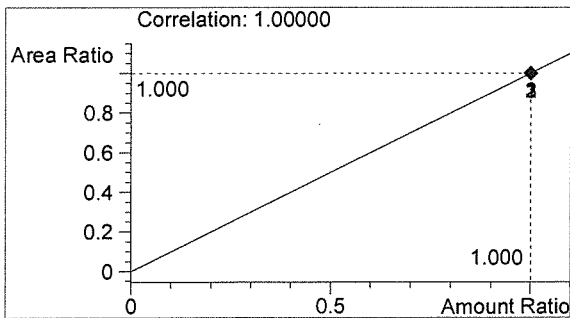

n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:27:27 AM

Sample Name: 0.316 CAL 3

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 4

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

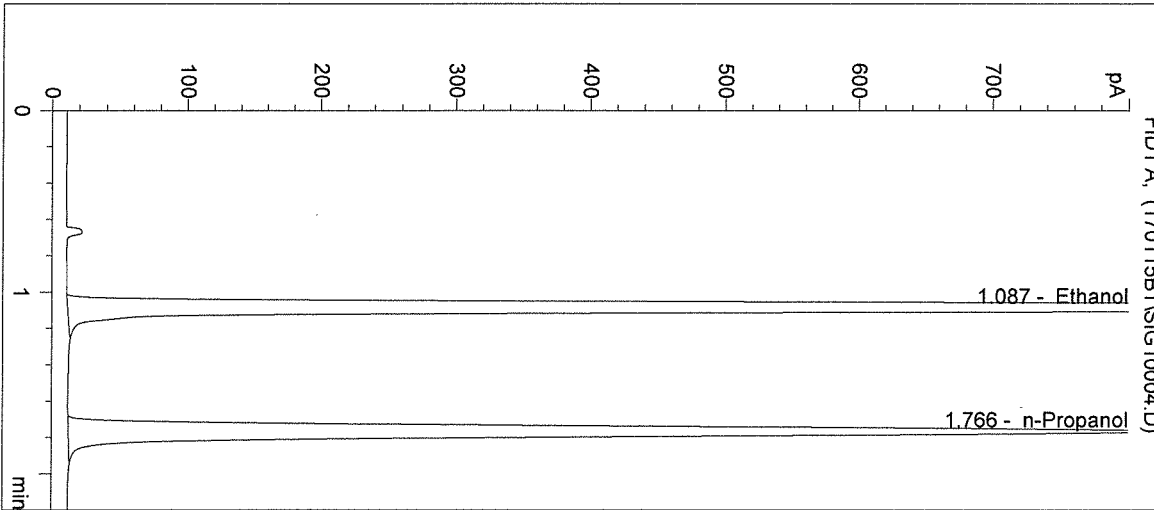


#	Compound	Peak Area	RT (min)
1	Ethanol	4286	1.087
2	n-Propanol	3092	1.766



Ethanol 0.319 g/100mL

BLU



n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:30:41 AM

Sample Name: NEG CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 5

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

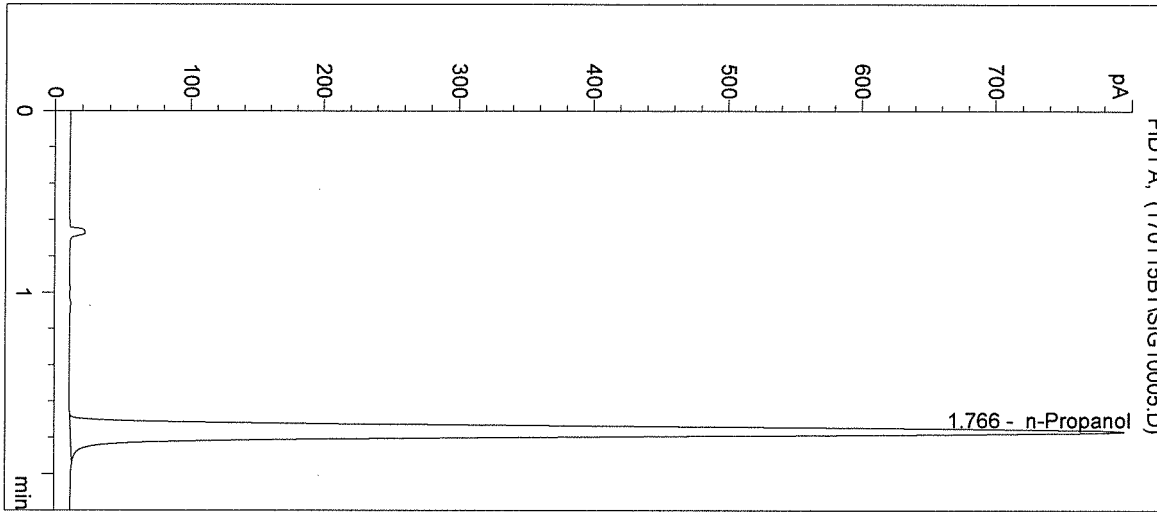


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2992	1.766

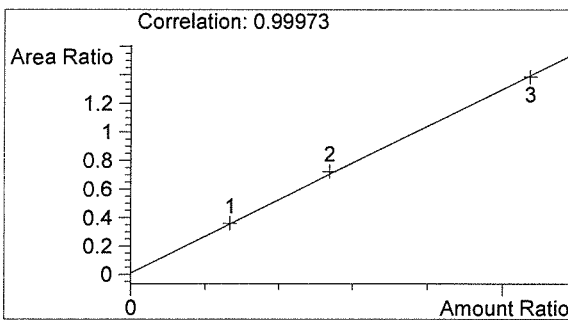

Ethanol 0.000 g/100mL

AWO



n-Propanol 0.012 g/100mL

MT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:33:54 AM

Sample Name: 0.04 CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 6

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

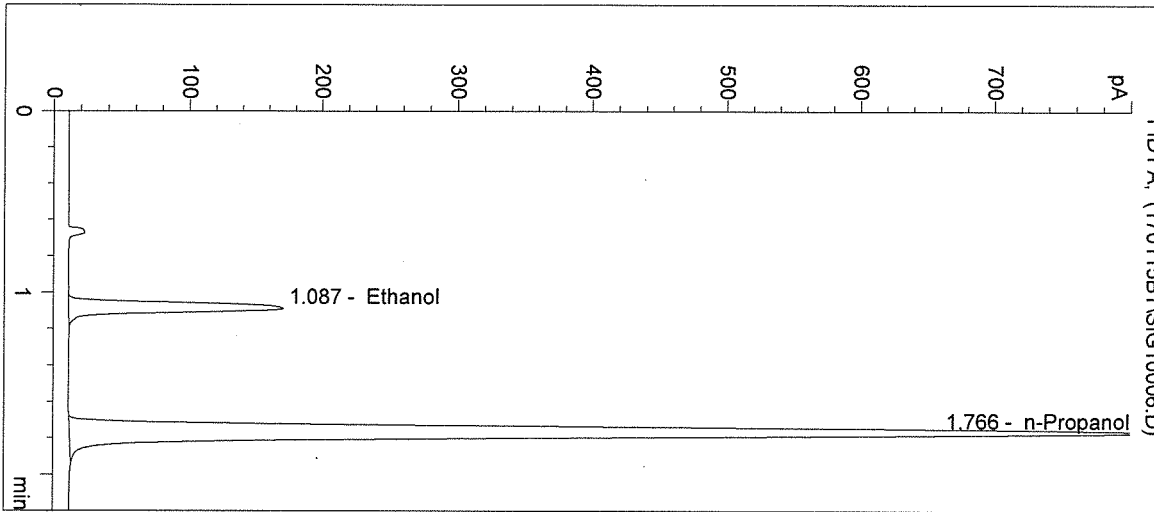


#	Compound	Peak Area	RT (min)
1	Ethanol	548	1.087
2	n-Propanol	3067	1.766

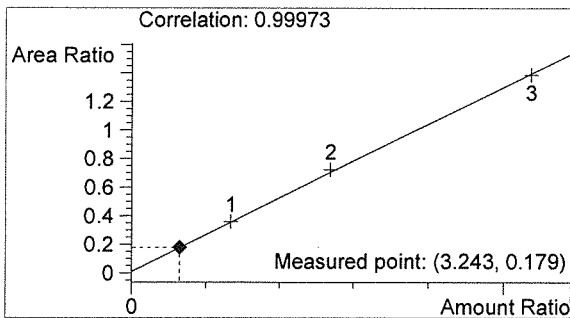

Ethanol 0.039 g/100mL

AWO

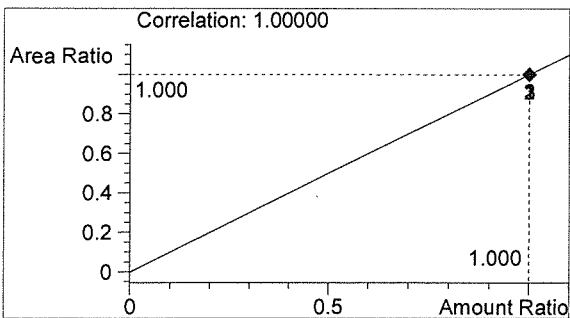

n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:37:07 AM

Sample Name: 0.10 CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 7

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

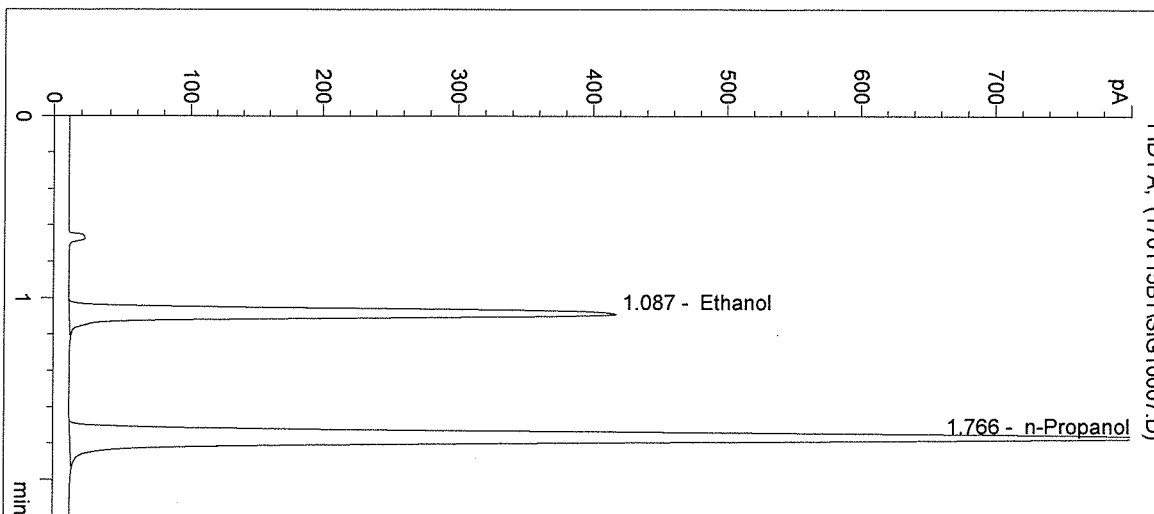


#	Compound	Peak Area	RT (min)
1	Ethanol	1402	1.087
2	n-Propanol	3139	1.766

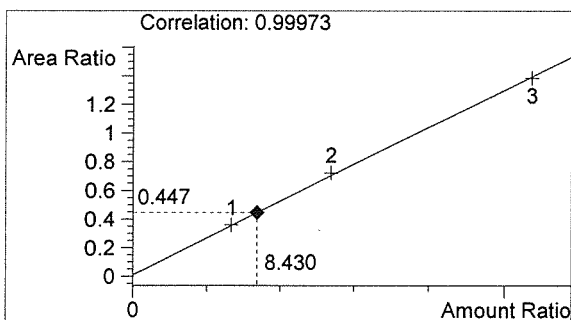

Ethanol 0.101 g/100mL

BLW

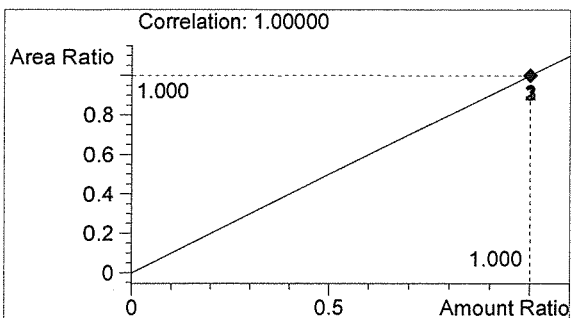

n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:40:21 AM

Sample Name: 0.20 CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 8

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

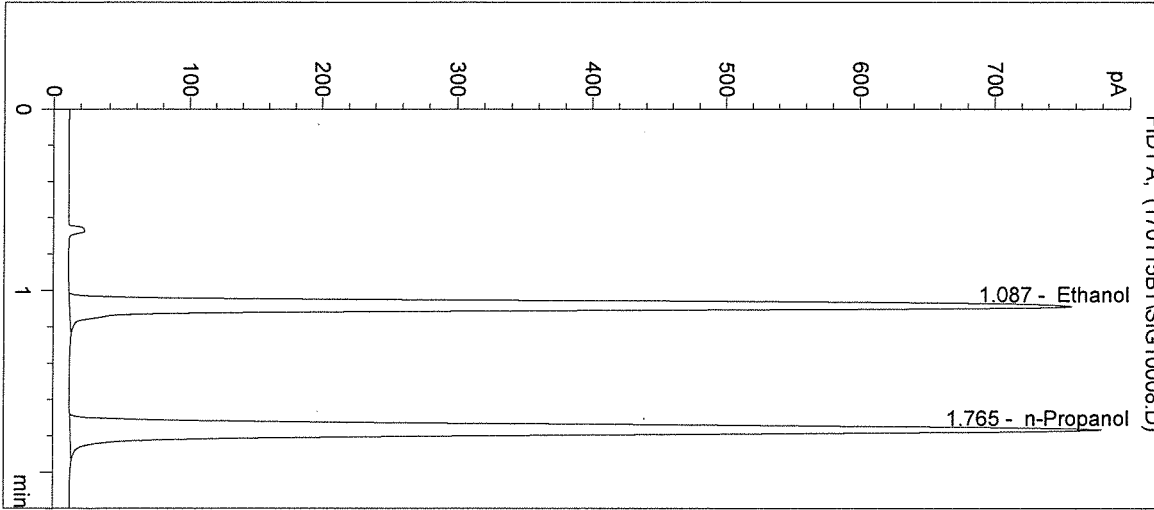


#	Compound	Peak Area	RT (min)
1	Ethanol	2564	1.087
2	n-Propanol	2914	1.765

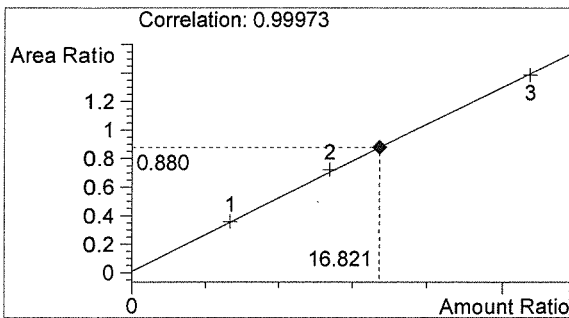

Ethanol 0.202 g/100mL

AWO



n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:43:34 AM

Sample Name: NEG CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 9

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

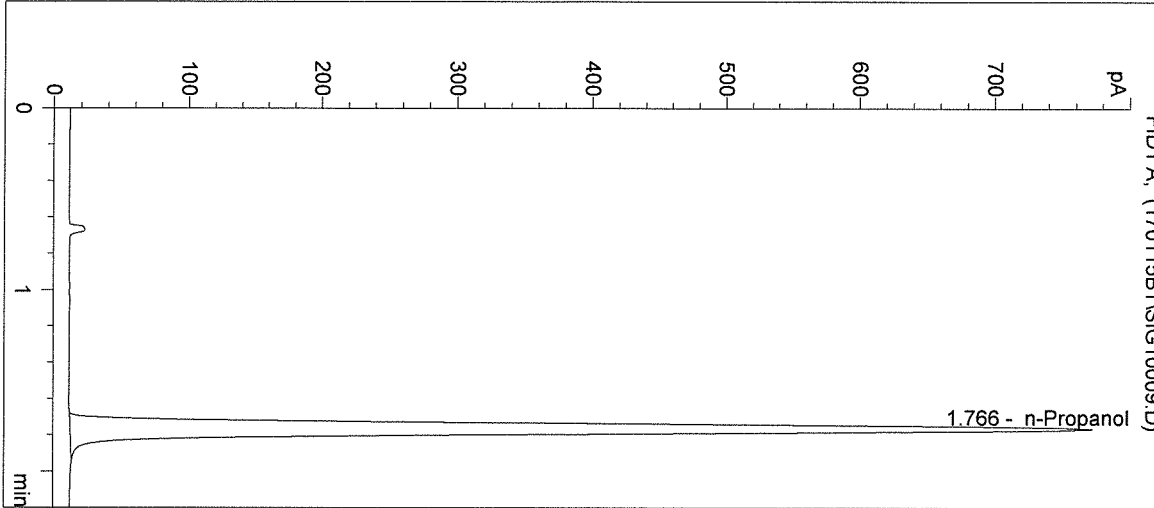


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2893	1.766

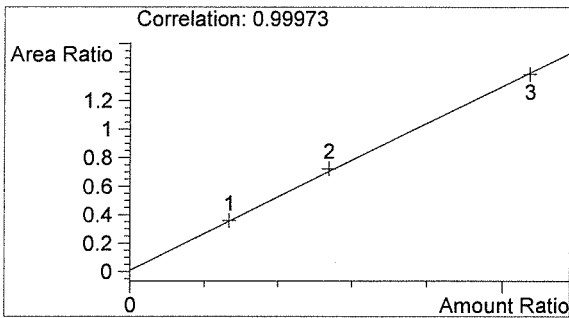

Ethanol 0.000 g/100mL

AW



n-Propanol 0.012 g/100mL

AW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:46:47 AM

Sample Name: QAP0.20 17007 #1

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 10

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

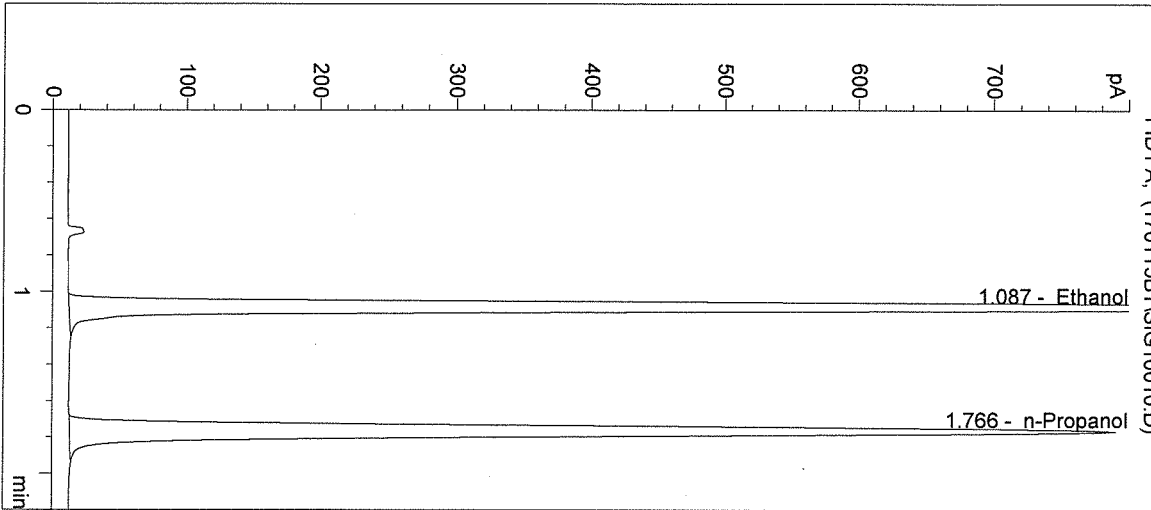


#	Compound	Peak Area	RT (min)
1	Ethanol	3226	1.087
2	n-Propanol	2952	1.766

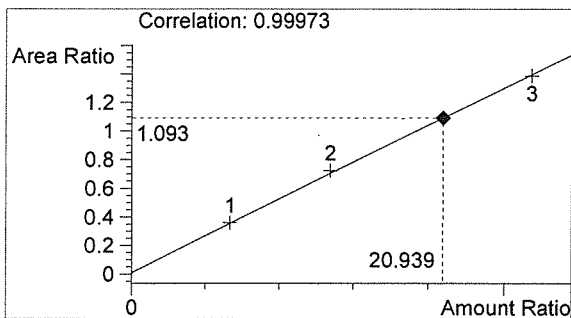

Ethanol 0.251 g/100mL

AWD

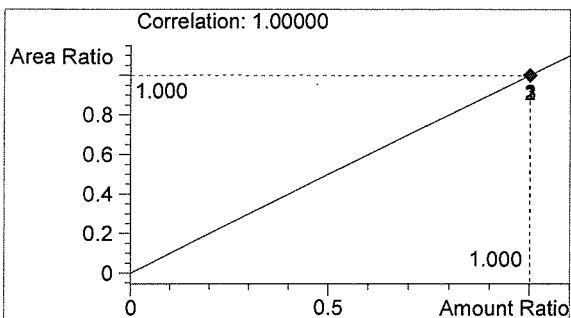

n-Propanol 0.012 g/100mL

VT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:50:00 AM

Sample Name: QAP0.20 17007 #2

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 11

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

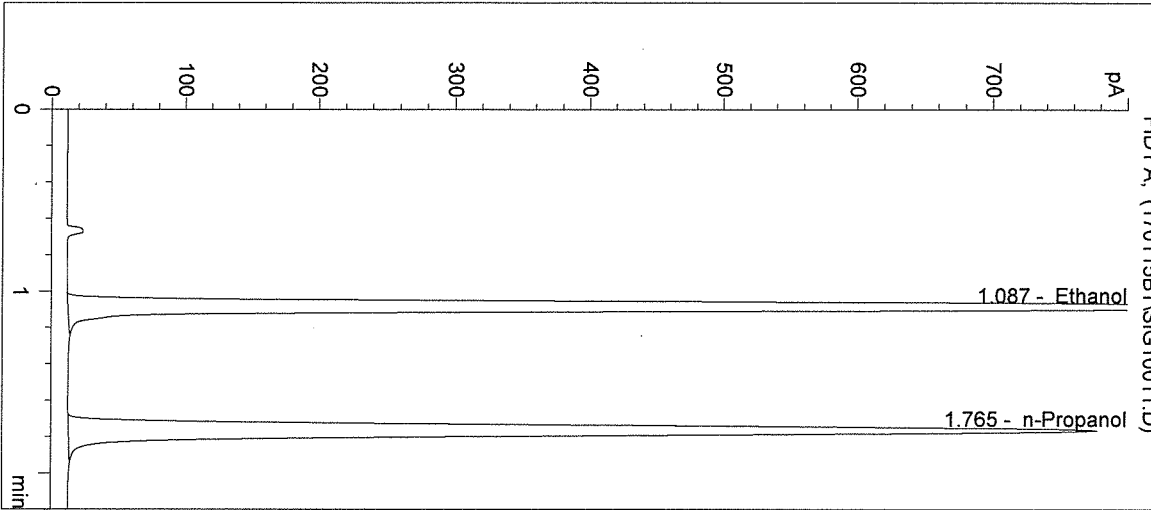


#	Compound	Peak Area	RT (min)
1	Ethanol	3154	1.087
2	n-Propanol	2904	1.765



Ethanol 0.250 g/100mL

AW



n-Propanol 0.012 g/100mL

AW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:53:14 AM

Sample Name: QAP0.20 17007 #3

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 12

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

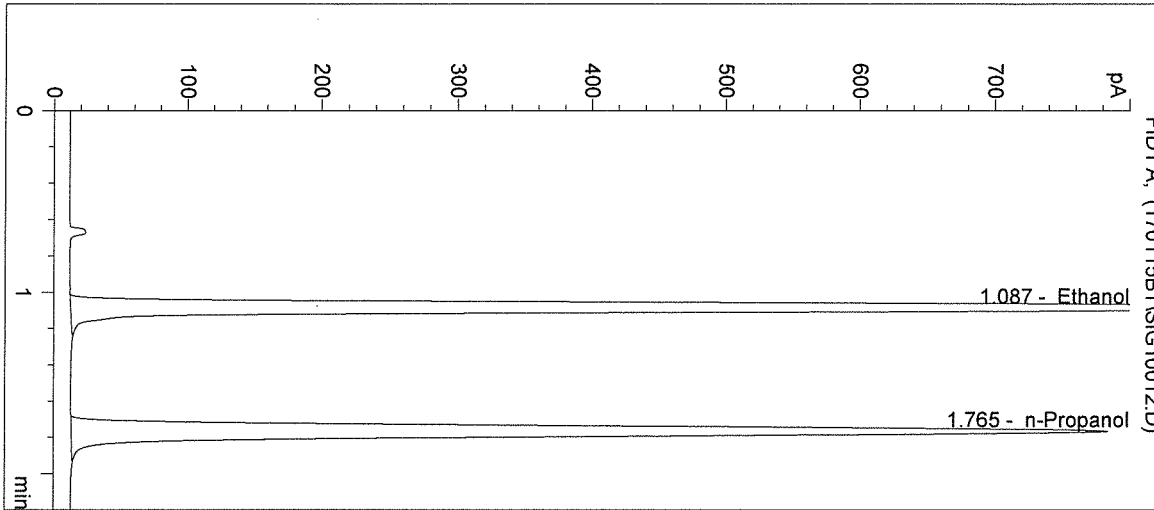


#	Compound	Peak Area	RT (min)
1	Ethanol	3200	1.087
2	n-Propanol	2927	1.765

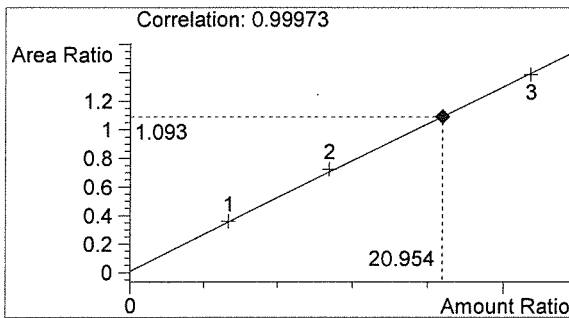

Ethanol 0.251 g/100mL

RAW

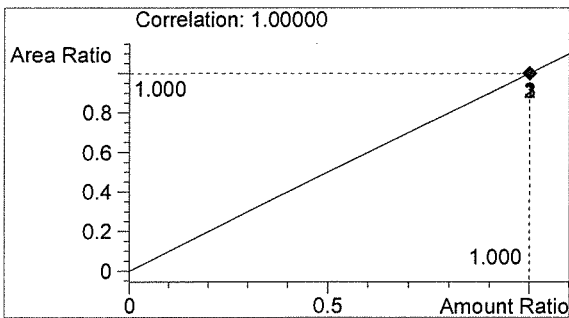

n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:56:27 AM

Sample Name: QAP0.20 17007 #4

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 13

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

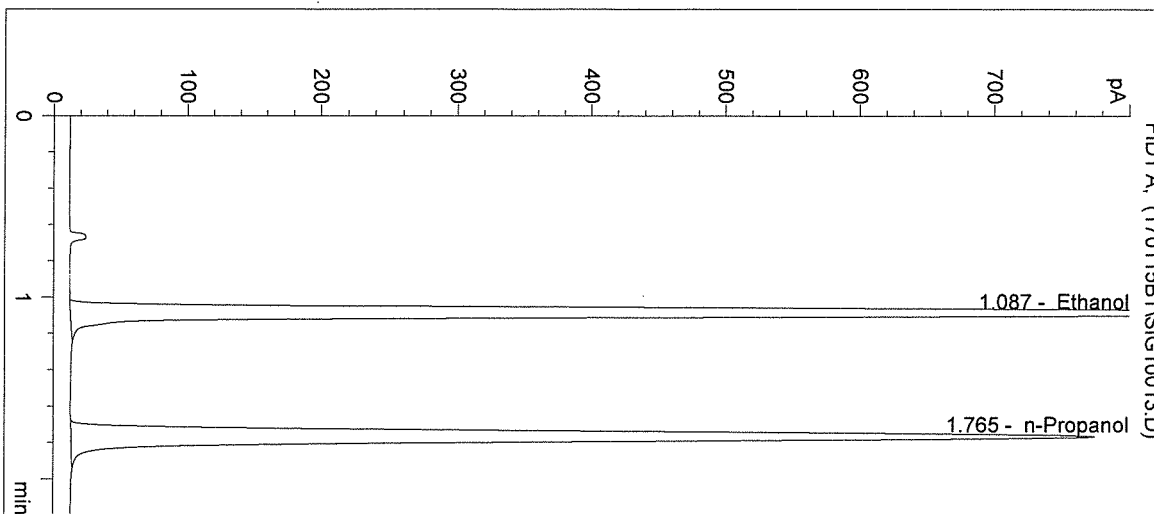


#	Compound	Peak Area	RT (min)
1	Ethanol	3143	1.087
2	n-Propanol	2891	1.765

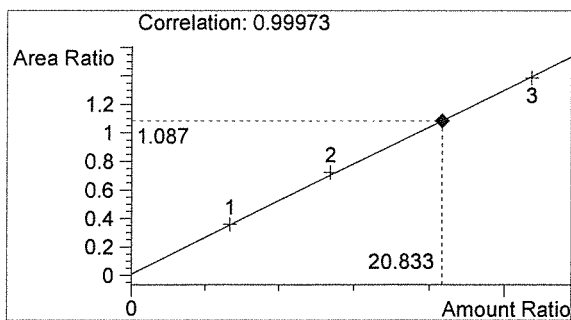

Ethanol 0.250 g/100mL

ALW

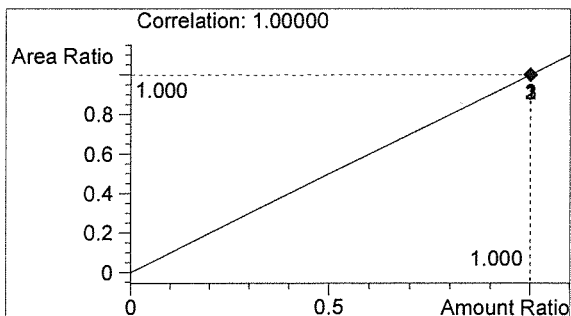

n-Propanol 0.012 g/100mL

MT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 9:59:40 AM

Sample Name: QAP0.20 17007 #5

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 14

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

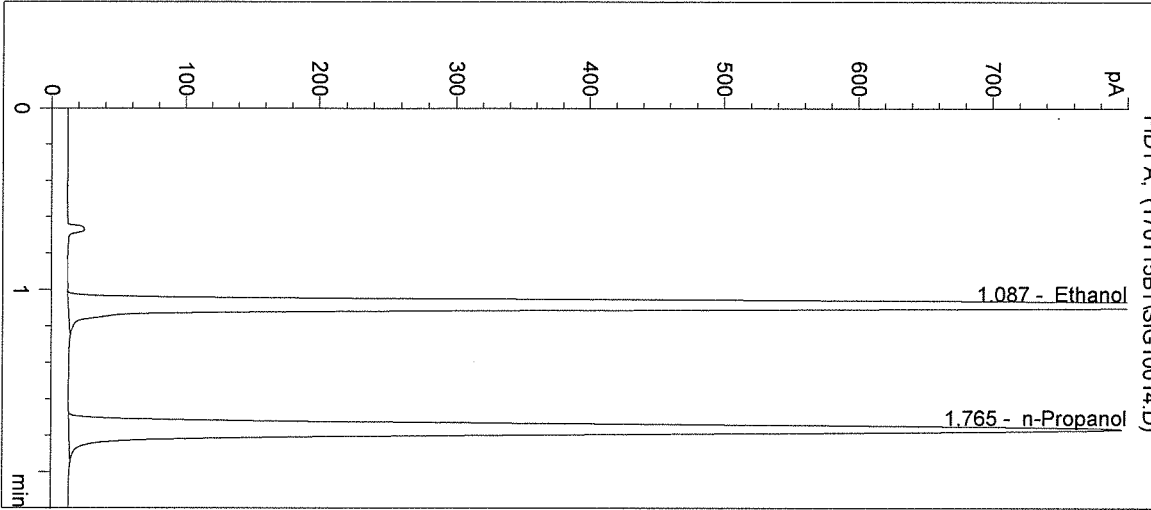


#	Compound	Peak Area	RT (min)
1	Ethanol	3234	1.087
2	n-Propanol	2975	1.765



Ethanol 0.250 g/100mL

AW



n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 10:02:53 AM

Sample Name: 0.10 CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 15

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: ~~15028~~ 17007
 1/17/17

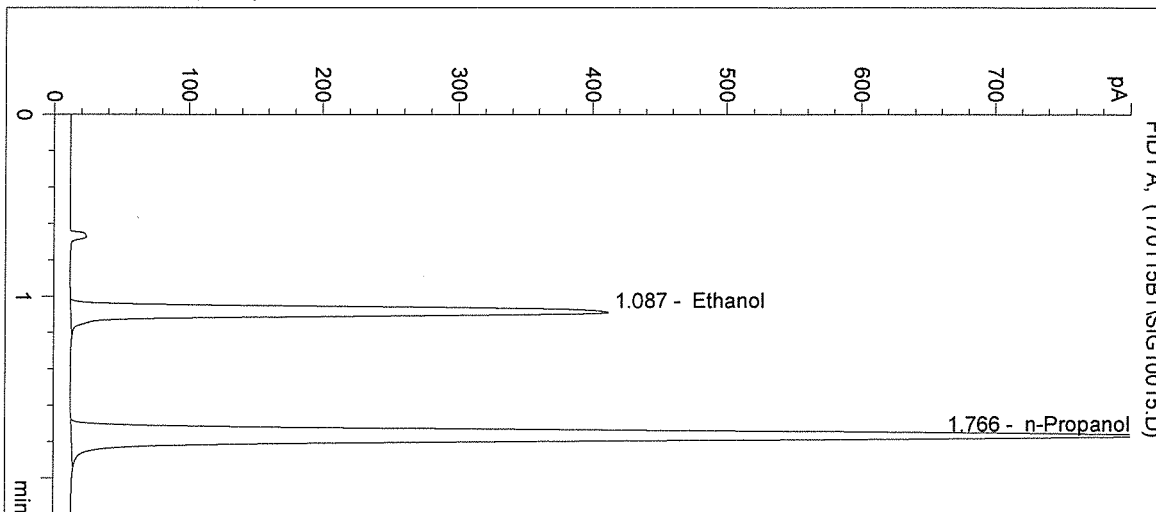


#	Compound	Peak Area	RT (min)
1	Ethanol	1376	1.087
2	n-Propanol	3084	1.766

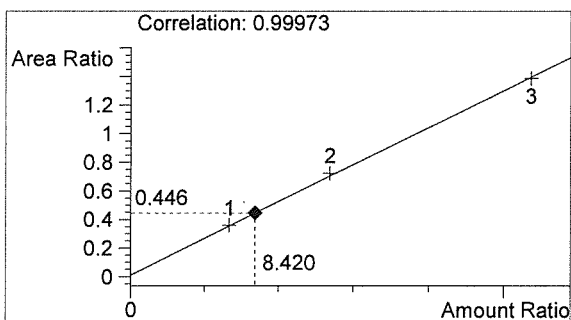

Ethanol 0.101 g/100mL

BLW

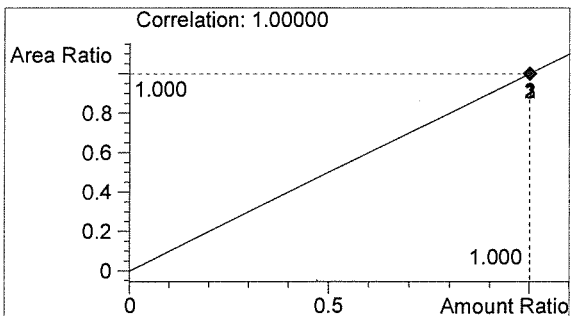

n-Propanol 0.012 g/100mL

BT

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 10:06:07 AM

Sample Name: NEG CTRL-BT

Instrument: HSGC#1


Operator: Brittany Thomas

Column: DB-ALC1


Location: Vial 16

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: ~~15028~~ 17007
 BT 1/17/17

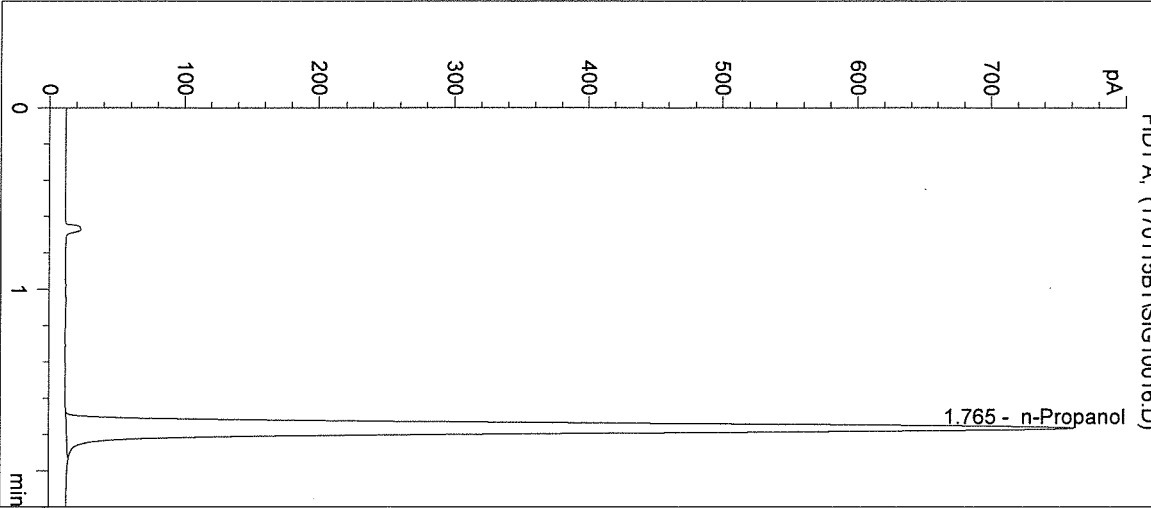


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2842	1.765



Ethanol 0.000 g/100mL

PLU



n-Propanol 0.012 g/100mL

BT

Sequence Parameters:

Operator: Katie Harris
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 170115KH
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

CAL 1 (0.079g/100mL) - LOT# E0916-01 - EXP 3/15/2017
 CAL 2 (0.158g/100mL) - LOT# E0916-02 - EXP 3/15/2017
 CAL 3 (0.316g/100mL) - LOT# E0916-03 - EXP 3/15/2017
 CTRL 1 (0.04g/100mL) - LOT# FN12181501 - EXP 12/2020
 CTRL 2 (0.10g/100mL) - LOT# FN08051301 - EXP 10/2018
 CTRL 3 (0.20g/100mL) - LOT# FN08101505 - EXP 02/2021
 n-Propanol ISTD - LOT# P1116 - Exp 02/23/2017

Standard data located in Batch File 17007

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	NEG CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	NEG CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	QAP0.20 17007 #1	SIMALC1	1	Sample		
11	Vial 11	QAP0.20 17007 #2	SIMALC1	1	Sample		
12	Vial 12	QAP0.20 17007 #3	SIMALC1	1	Sample		
13	Vial 13	QAP0.20 17007 #4	SIMALC1	1	Sample		
14	Vial 14	QAP0.20 17007 #5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	NEG CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	QAP0.08 17009 #1	SIMALC1	1	Sample		
18	Vial 18	QAP0.08 17009 #2	SIMALC1	1	Sample		
19	Vial 19	QAP0.08 17009 #3	SIMALC1	1	Sample		
20	Vial 20	QAP0.08 17009 #4	SIMALC1	1	Sample		
21	Vial 21	QAP0.08 17009 #5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	NEG CTRL	SIMALC1	1	Ctrl Samp		

17007
 BLU 1-31-17

Calibration Part:

KH

Sequence: C:\HPCHEM\1\SEQUENCE\KHQAP.S

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

17007
Rw01-31-17

KH

=====
Calibration Table
=====

Calib. Data Modified : Sunday, January 15, 2017 11:41:29 AM

Calculate : Internal Standard
Based on : Peak Area

Rel. Reference Window : 5.000 %
Abs. Reference Window : 0.050 min
Rel. Non-ref. Window : 5.000 %
Abs. Non-ref. Window : 0.050 min
Multiplier : 1.0000
Dilution : 1.0000
Sample Amount : 0.00000

Use Multiplier & Dilution Factor with ISTDs
Uncalibrated Peaks : not reported
Partial Calibration : No recalibration if peaks missing

Curve Type : Linear
Origin : Included
Weight : Equal

Recalibration Settings:
Average Response : No Update
Average Retention Time: No Update

Calibration Report Options :
Printout of recalibrations within a sequence:
Normal Report after Recalibration

Sample ISTD Information:

ISTD #	ISTD Amount [g/100mL]	Name
1	1.20000e-2	n-Propanol

Signal 1: FID1 A,

RetTime [min]	Lvl Sig	Amount [g/100mL]	Area	Amt/Area	Ref Grp	Name
1.087	1 1	8.00100e-2	1029.69141	7.77029e-5	1	Ethanol
		2 1.61200e-1	2010.12781	8.01939e-5		
		3 3.21790e-1	3914.76782	8.21990e-5		
1.766	1 1	1.20000e-2	2911.61377	4.12143e-6	I1	n-Propanol
		2 1.20000e-2	2882.90527	4.16247e-6		
		3 1.20000e-2	2859.59521	4.19640e-6		


17007
Rev 1-31-17

=====
Peak Sum Table
=====


No Entries in table
=====

KH

=====
Calibration Curves
=====

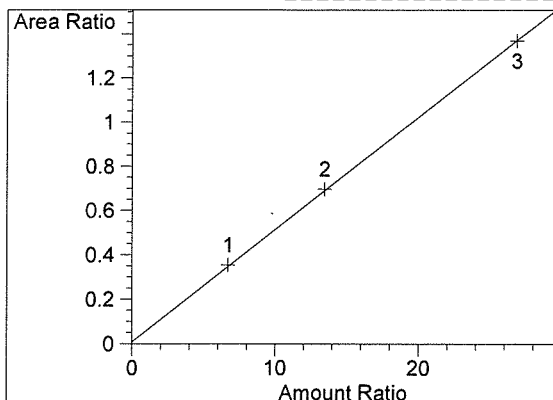

Ethanol at exp. RT: 1.087
FID1 A,
Correlation: 0.99993
Residual Std. Dev.: 0.00862
Formula: $y = mx + b$
m: 5.09308e-2
b: 7.59940e-3
x: Amount Ratio
y: Area Ratio

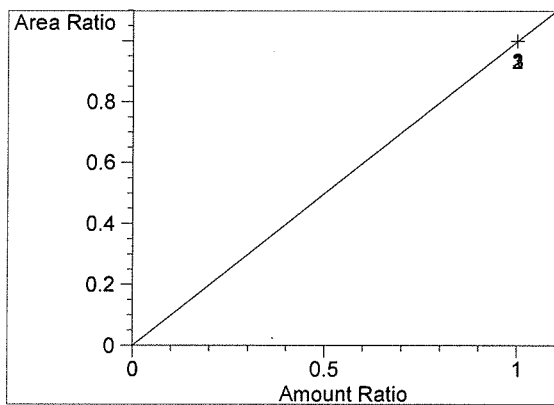

n-Propanol at exp. RT: 1.766
FID1 A,
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio


=====

17007
Rw01-31-17


KH

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:29:24 AM Sample Name: BLANK
Instrument: HSGC#1 Operator: Katie Harris
Column: DB-ALC1 Location: Vial 1
Method: C:\HPCHEM\1\METHODS\SIMALC1.M
Sample Info: 17007

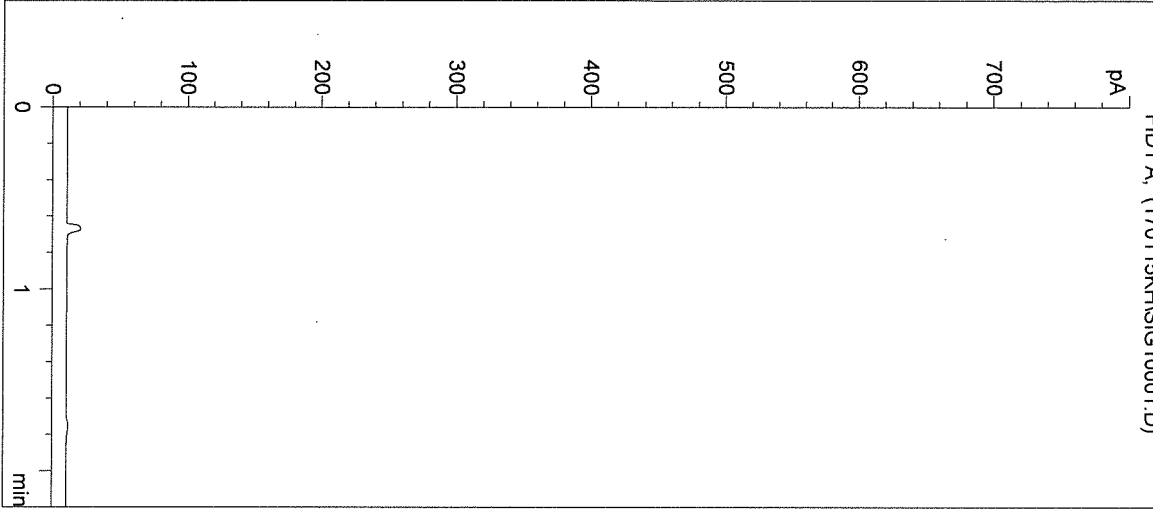


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	0	0.000

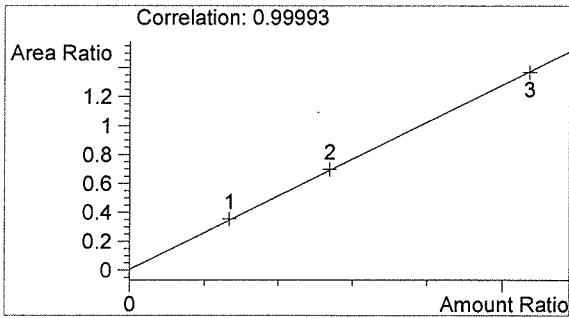

Ethanol 0.000 g/100mL

BW

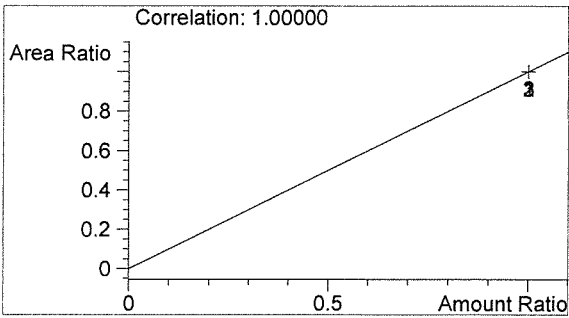

n-Propanol 0.000 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:32:41 AM

Sample Name: 0.079 CAL 1

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 2

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

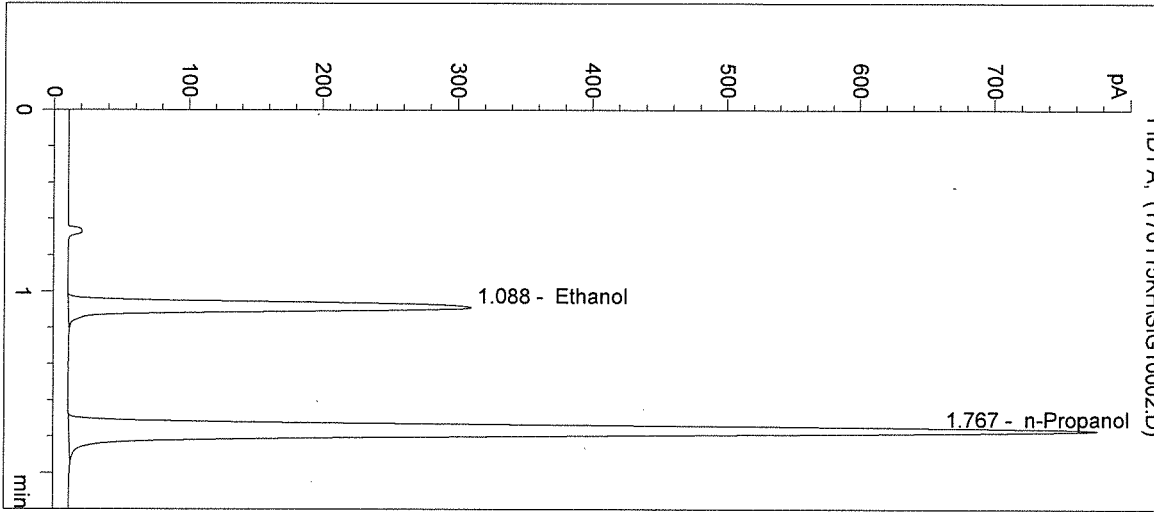


#	Compound	Peak Area	RT (min)
1	Ethanol	1030	1.088
2	n-Propanol	2912	1.767



Ethanol 0.082 g/100mL

PLW



n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:35:58 AM

Sample Name: 0.158 CAL 2

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 3

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

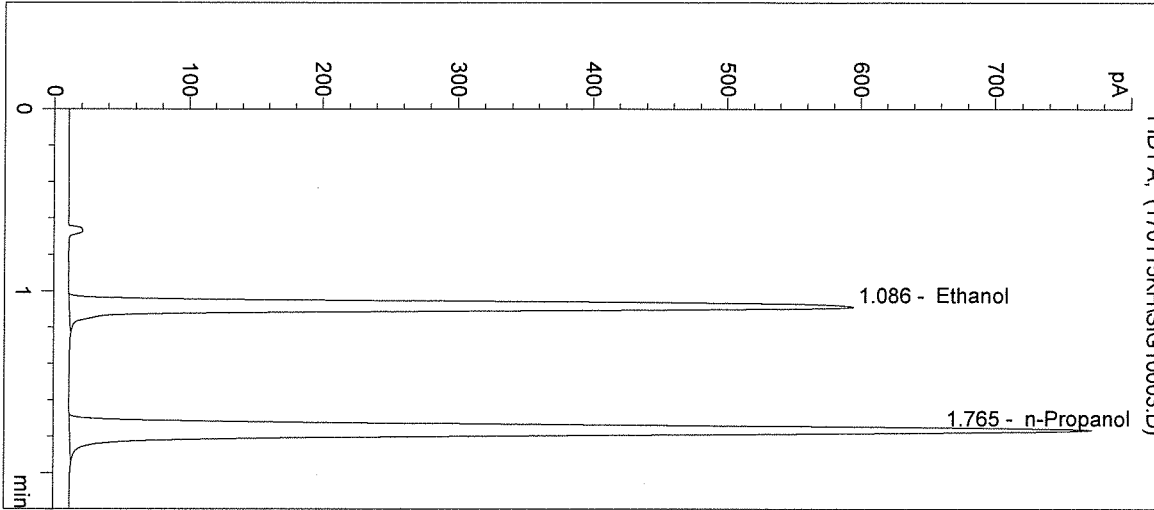


#	Compound	Peak Area	RT (min)
1	Ethanol	2010	1.086
2	n-Propanol	2883	1.765

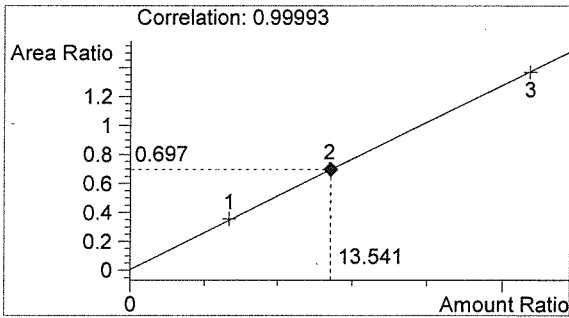

Ethanol 0.162 g/100mL

BW



n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:39:15 AM

Sample Name: 0.316 CAL 3

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 4

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

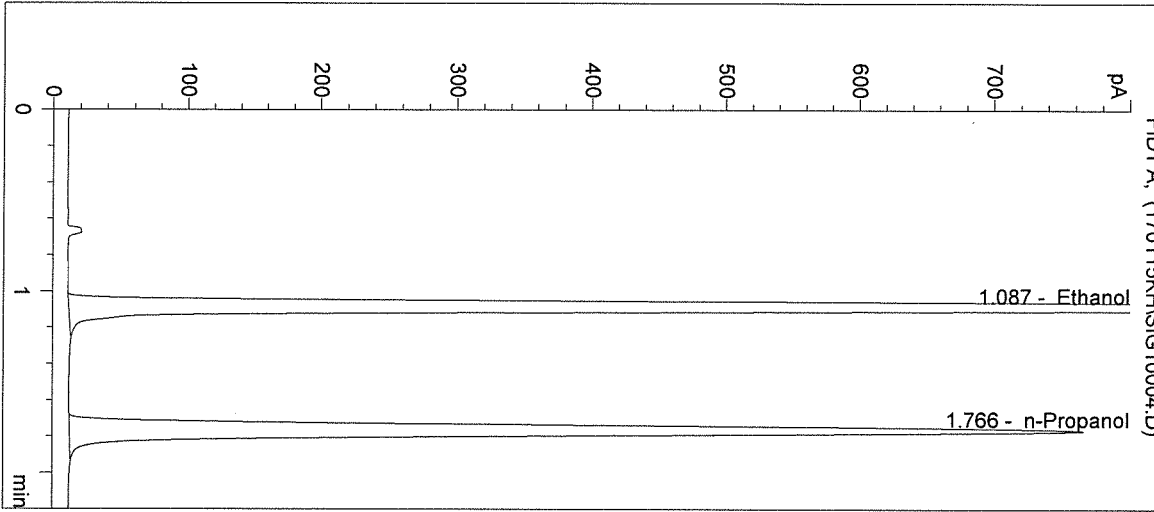


#	Compound	Peak Area	RT (min)
1	Ethanol	3915	1.087
2	n-Propanol	2860	1.766



Ethanol 0.321 g/100mL

AWO



n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:42:29 AM

Sample Name: NEG CTRL

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 5

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

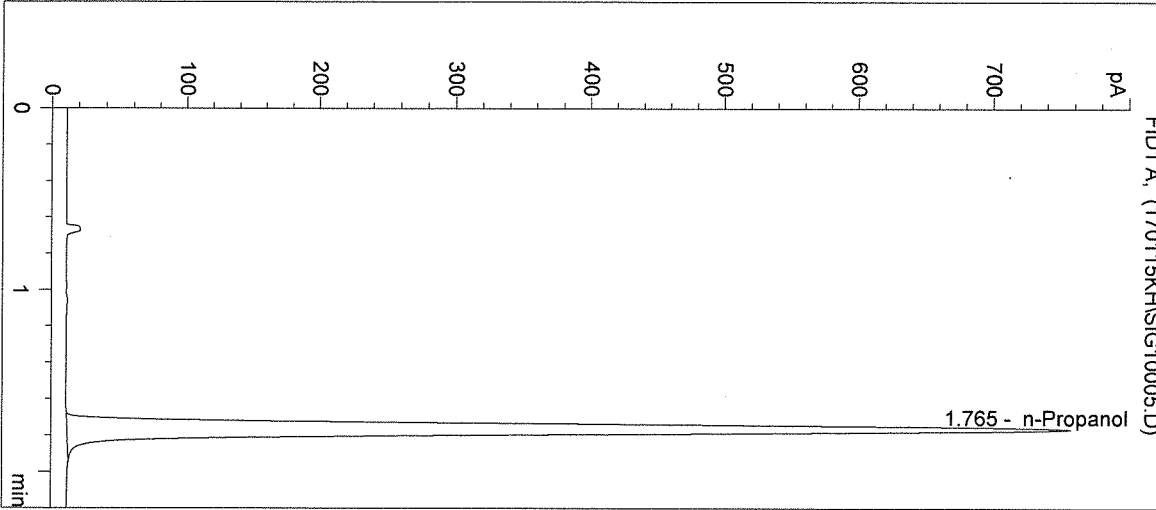


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2830	1.765

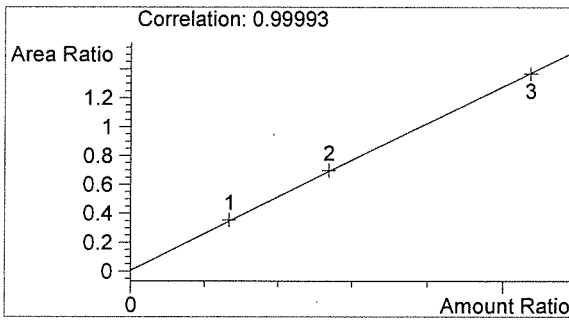

Ethanol 0.000 g/100mL

BW



n-Propanol 0.012 g/100mL

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:45:42 AM

Sample Name: 0.04 CTRL

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 6

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

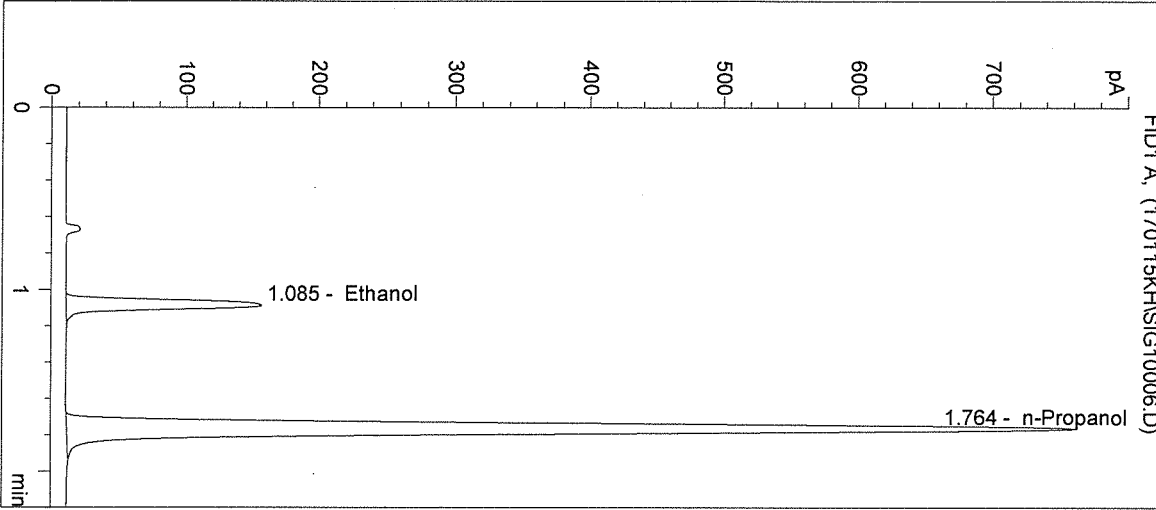


#	Compound	Peak Area	RT (min)
1	Ethanol	500	1.085
2	n-Propanol	2855	1.764

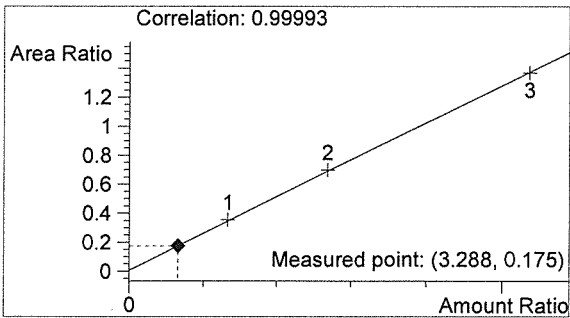

Ethanol 0.039 g/100mL

BLW

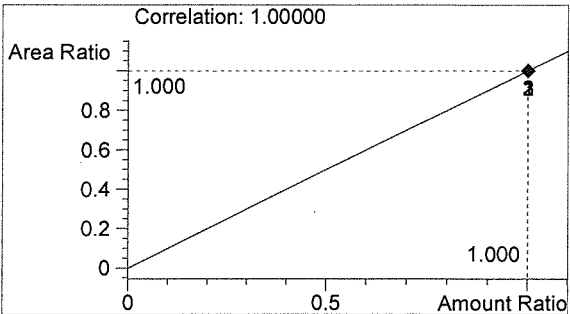

n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:48:56 AM

Sample Name: 0.10 CTRL

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 7

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

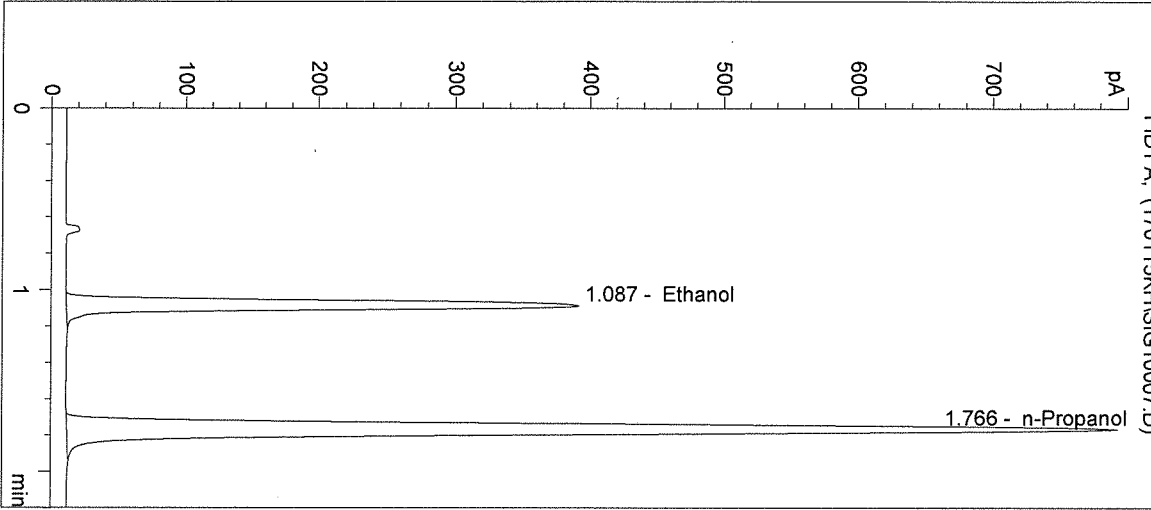


#	Compound	Peak Area	RT (min)
1	Ethanol	1309	1.087
2	n-Propanol	2973	1.766

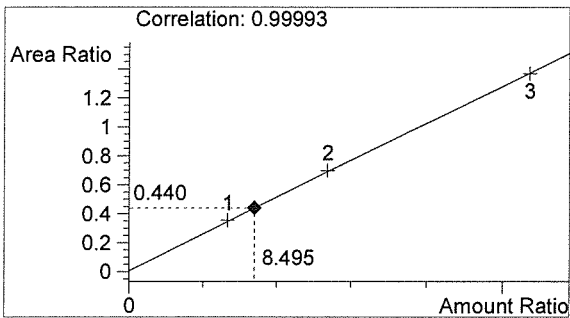

Ethanol 0.102 g/100mL

BWO

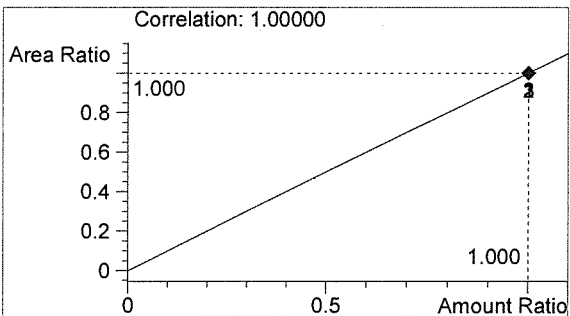

n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:52:09 AM

Sample Name: 0.20 CTRL

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 8

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

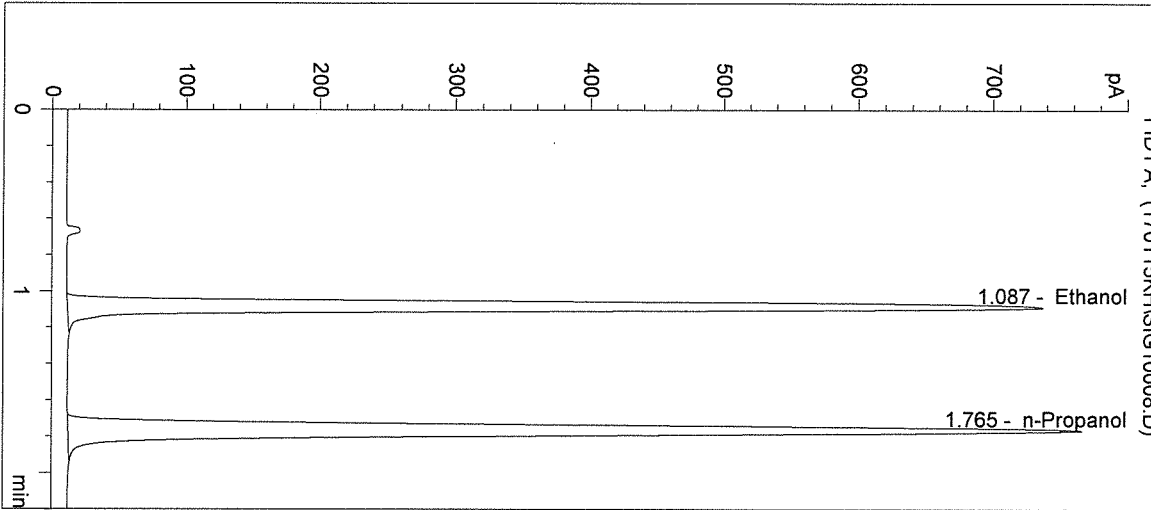


#	Compound	Peak Area	RT (min)
1	Ethanol	2495	1.087
2	n-Propanol	2868	1.765

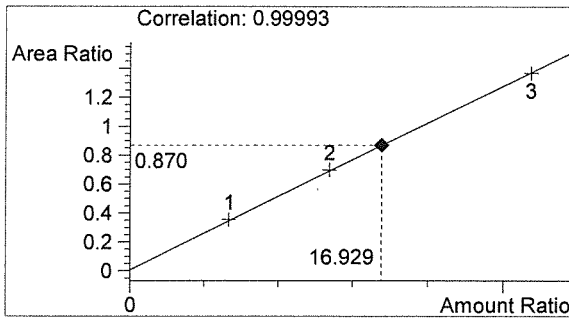

Ethanol 0.203 g/100mL

Buo



n-Propanol 0.012 g/100mL


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:55:22 AM
 Instrument: HSGC#1


Sample Name: NEG CTRL
 Operator: Katie Harris
 Location: Vial 9

Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

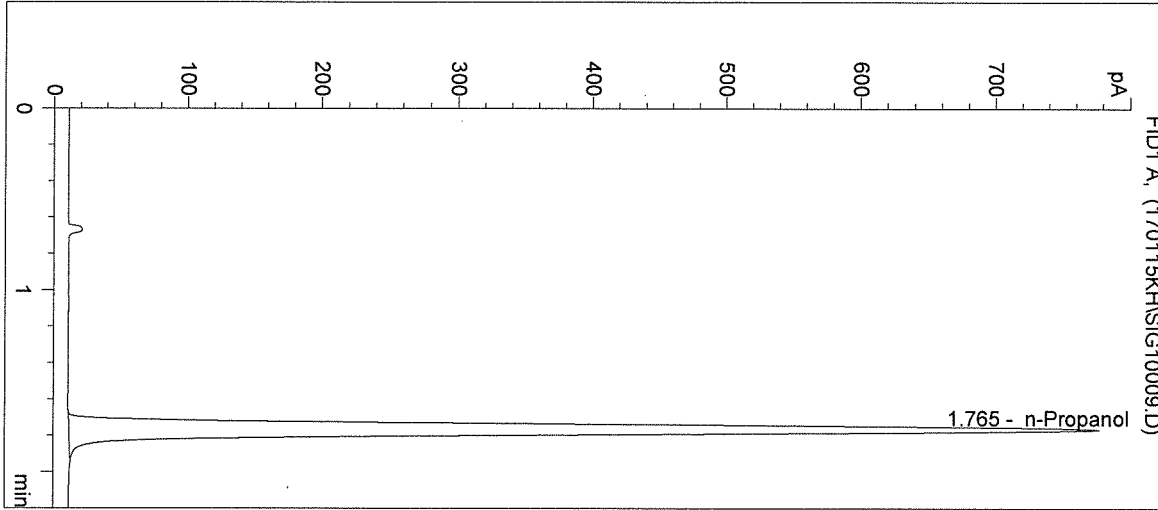


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2901	1.765



Ethanol 0.000 g/100mL

Buo

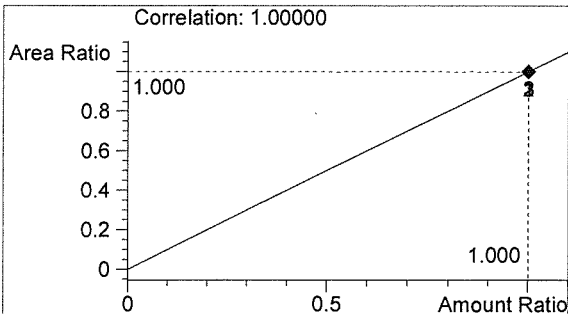

n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 11:58:35 AM

Sample Name: QAP0.20 17007 #1

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 10

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

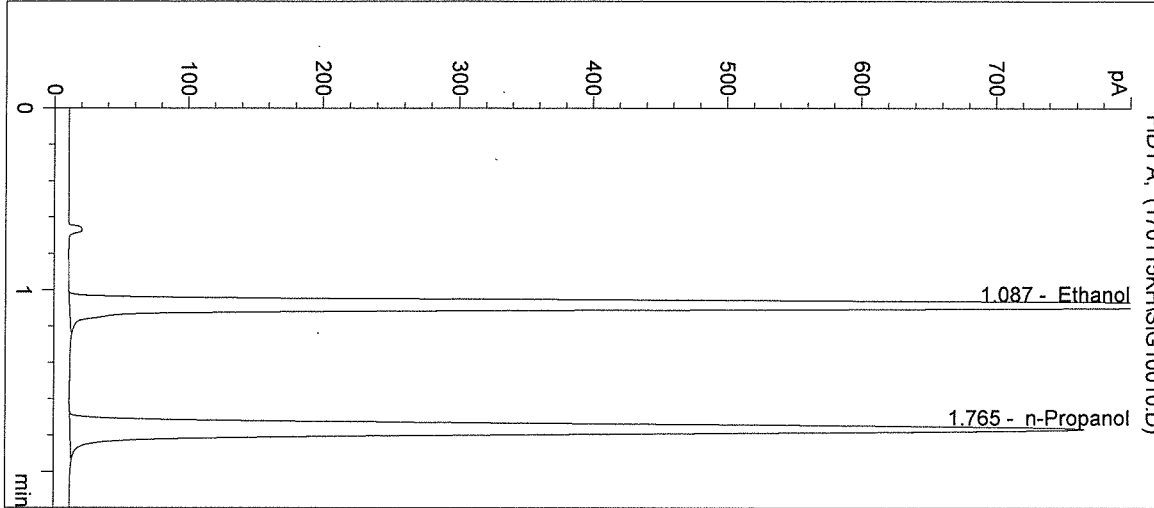


#	Compound	Peak Area	RT (min)
1	Ethanol	3089	1.087
2	n-Propanol	2860	1.765



Ethanol 0.253 g/100mL

PLW

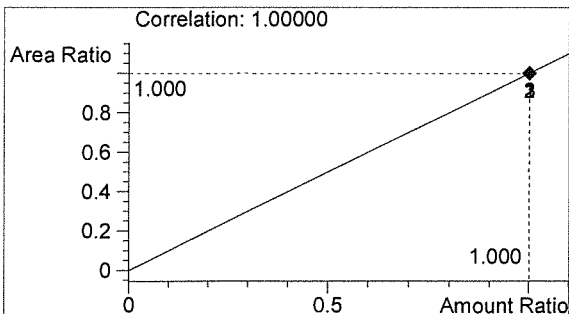

n-Propanol 0.012 g/100mL


KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/15/2017 12:01:48 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: QAP0.20 17007 #2
 Operator: Katie Harris
 Location: Vial 11

Sample Info:

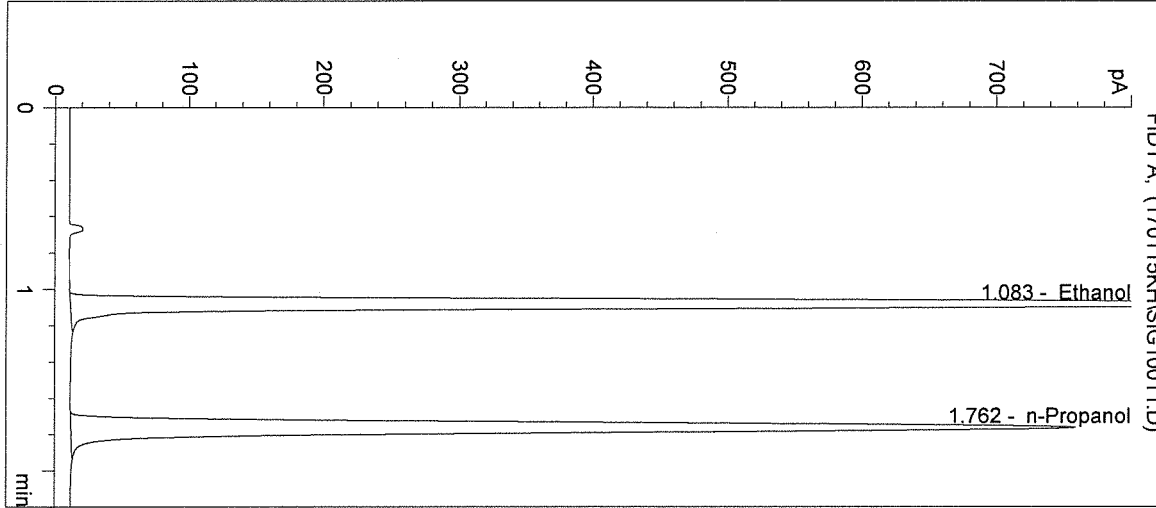


#	Compound	Peak Area	RT (min)
1	Ethanol	3025	1.083
2	n-Propanol	2828	1.762

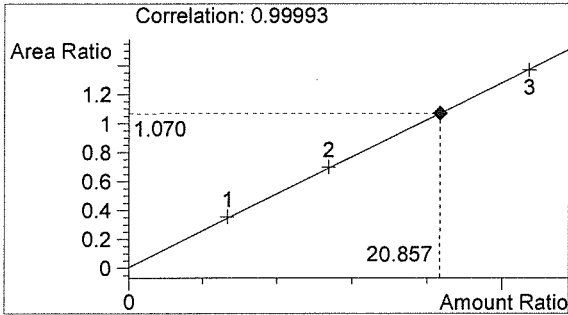

Ethanol 0.250 g/100mL

BW

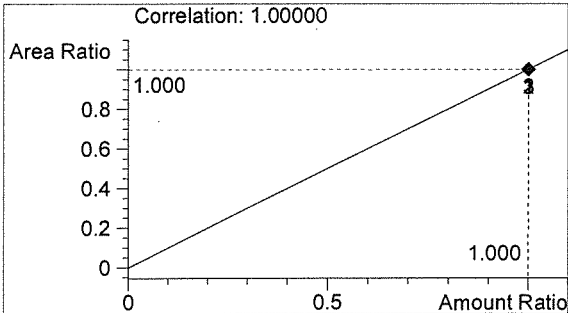

n-Propanol 0.012 g/100mL

KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 12:05:01 PM

Sample Name: QAP0.20 17007 #3

Instrument: HSGC#1


Operator: Katie Harris

Column: DB-ALC1


Location: Vial 12

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

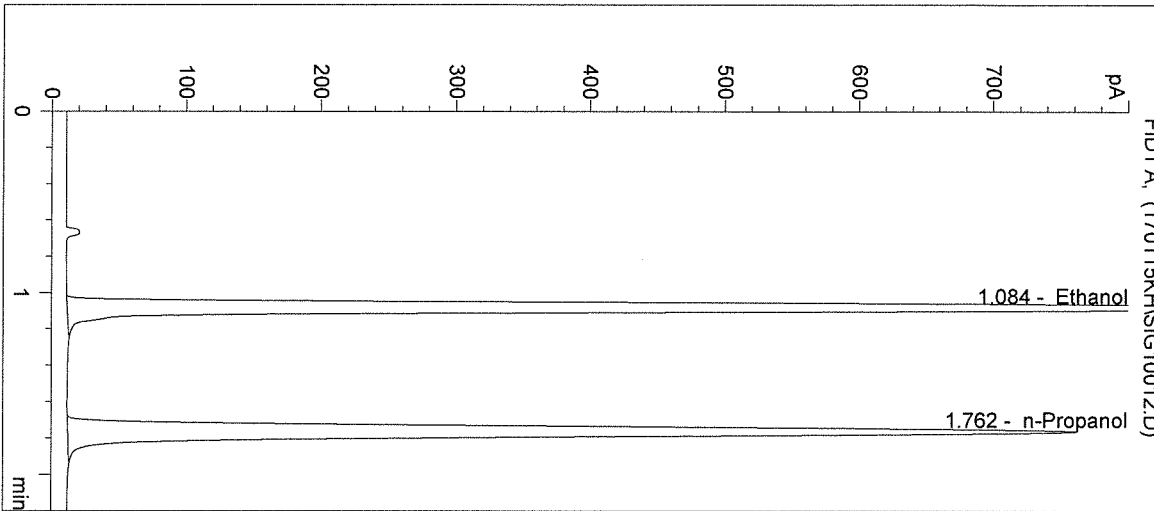


#	Compound	Peak Area	RT (min)
1	Ethanol	3038	1.084
2	n-Propanol	2826	1.762



Ethanol 0.251 g/100mL

BLW



n-Propanol 0.012 g/100mL


KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/15/2017 12:08:14 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: QAP0.20 17007 #4
 Operator: Katie Harris
 Location: Vial 13

Sample Info:

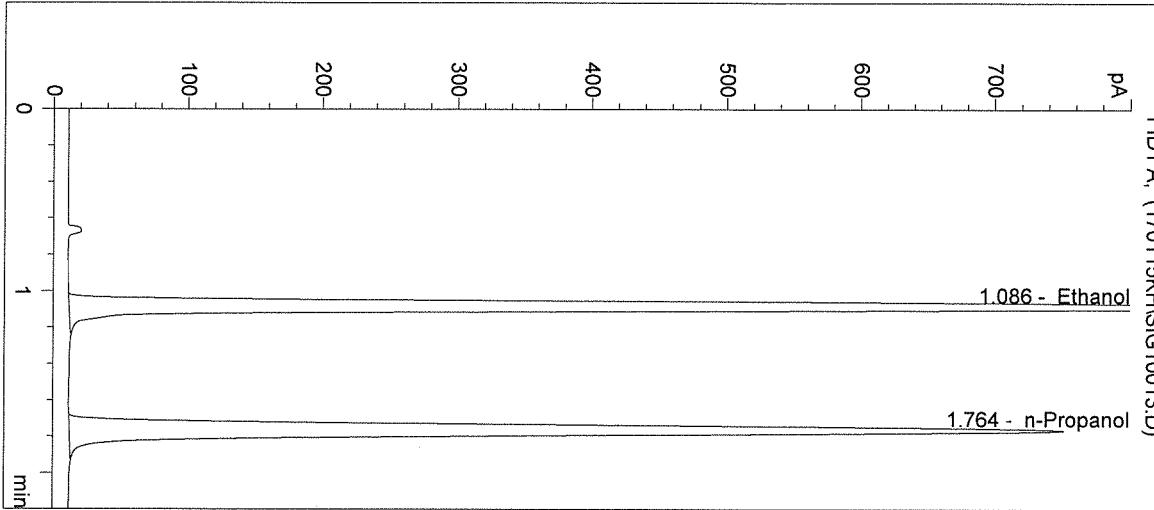


#	Compound	Peak Area	RT (min)
1	Ethanol	3034	1.086
2	n-Propanol	2805	1.764



Ethanol 0.253 g/100mL

BW

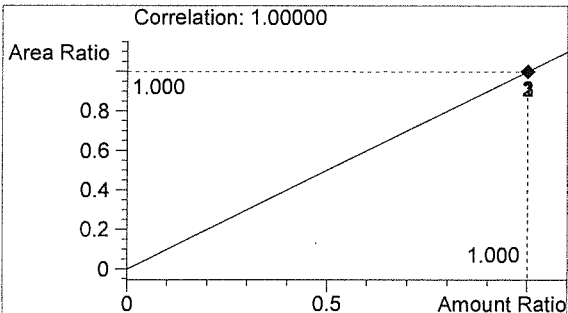

n-Propanol 0.012 g/100mL


KH

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/15/2017 12:11:28 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: QAP0.20 17007 #5
 Operator: Katie Harris
 Location: Vial 14

Sample Info:

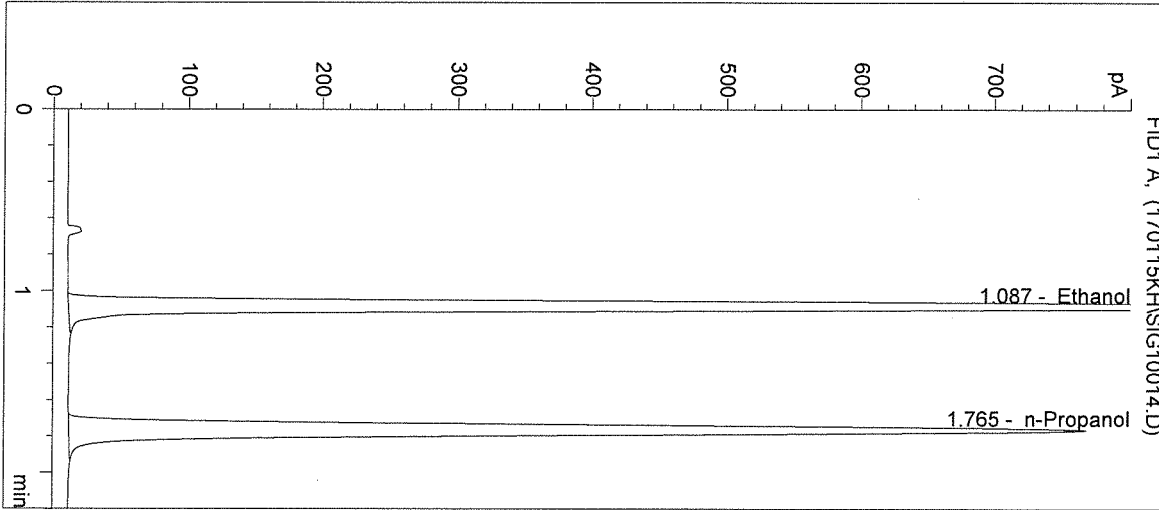


#	Compound	Peak Area	RT (min)
1	Ethanol	3103	1.087
2	n-Propanol	2870	1.765



Ethanol 0.253 g/100mL

BW

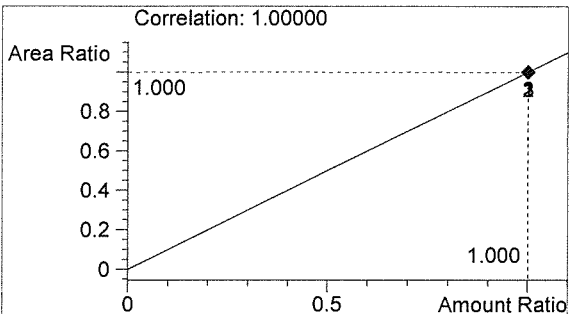

n-Propanol 0.012 g/100mL

KH


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 12:14:41 PM
 Instrument: HSGC#1


Sample Name: 0.10 CTRL
 Operator: Katie Harris
 Location: Vial 15

Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

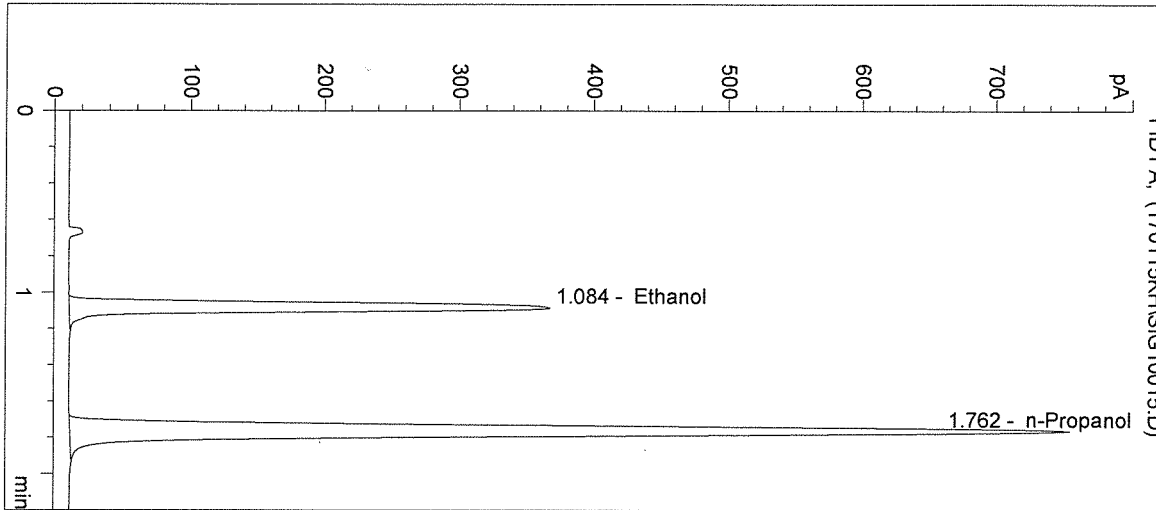


#	Compound	Peak Area	RT (min)
1	Ethanol	1214	1.084
2	n-Propanol	2802	1.762

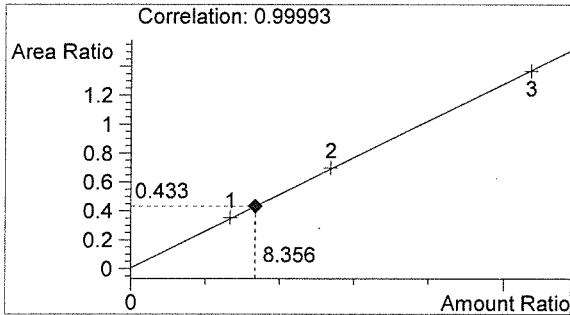

Ethanol 0.100 g/100mL

BW

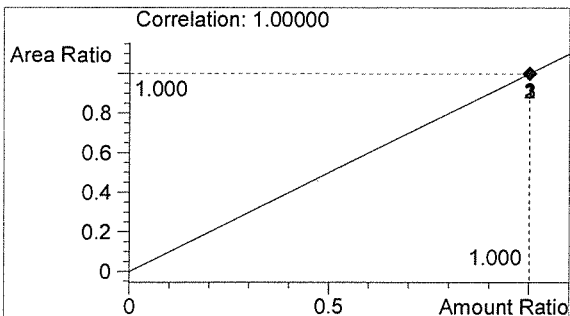

n-Propanol 0.012 g/100mL

KH


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/15/2017 12:17:54 PM
 Instrument: HSGC#1


Sample Name: NEG CTRL
 Operator: Katie Harris
 Location: Vial 16

Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

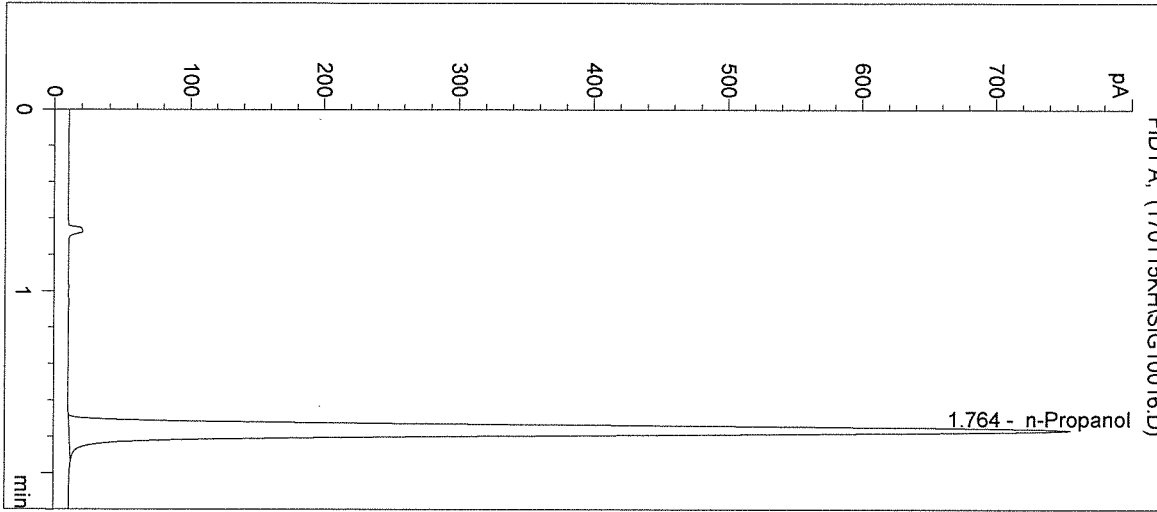


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2815	1.764

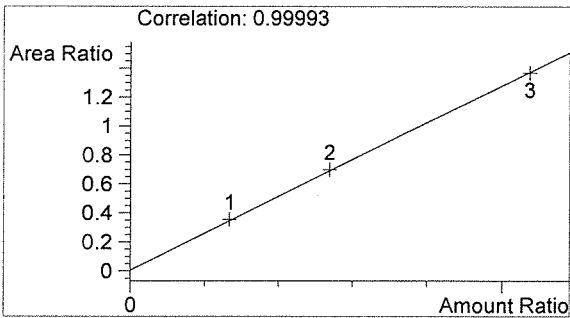

Ethanol 0.000 g/100mL

BW

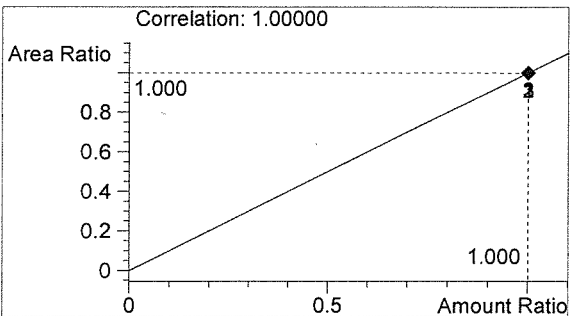

n-Propanol 0.012 g/100mL

KH

Sequence Parameters:

Operator: David Nguyen
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 170117DN
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

*1 value outside acceptable
 range for batch 17009,
 batch 17009 re-aliquotted
 & tested.
 1/17/17DN*

Sequence Comment:

CAL 1: 0.079 g/100mL - Lot: E0916-01 - X: 03/15/17
 CAL 2: 0.158 g/100mL - Lot: E0916-02 - X: 03/15/17
 CAL 3: 0.316 g/100mL - Lot: E0916-03 - X: 03/15/17

 CTRL 1: 0.04 g/100mL - Lot: FN12181501 - X: 12/2020
 CTRL 2: 0.10 g/100mL - Lot: FN08051301 - X: 10/2018
 CTRL 3: 0.20 g/100mL - Lot: FN08101505 - X: 02/2021

 n-Propanol ISTD - Lot: P1116 - X: 02/23/17

 Calibration vials 1-9 filed with 17007.

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	CAL 1 (0.079)	SIMALC1	1	Calib		
3	Vial 3	CAL 2 (0.158)	SIMALC1	1	Calib		
4	Vial 4	CAL 3 (0.316)	SIMALC1	1	Calib		
5	Vial 5	NEG CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	CTRL 1 (0.04)	SIMALC1	1	Ctrl Samp		
7	Vial 7	CTRL 2 (0.10)	SIMALC1	1	Ctrl Samp		
8	Vial 8	CTRL 3 (0.20)	SIMALC1	1	Ctrl Samp		
9	Vial 9	NEG CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	17007 #1	SIMALC1	1	Sample		
11	Vial 11	17007 #2	SIMALC1	1	Sample		
12	Vial 12	17007 #3	SIMALC1	1	Sample		
13	Vial 13	17007 #4	SIMALC1	1	Sample		
14	Vial 14	17007 #5	SIMALC1	1	Sample		
15	Vial 15	POS CTRL (0.10)	SIMALC1	1	Ctrl Samp		
16	Vial 16	NEG CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	17009 #1	SIMALC1	1	Sample		
18	Vial 18	17009 #2	SIMALC1	1	Sample		
19	Vial 19	17009 #3	SIMALC1	1	Sample		
20	Vial 20	17009 #4	SIMALC1	1	Sample		
21	Vial 21	17009 #5	SIMALC1	1	Sample		
22	Vial 22	POS CTRL (0.10)	SIMALC1	1	Ctrl Samp		
23	Vial 23	NEG CTRL	SIMALC1	1	Ctrl Samp		

*17007
 BU01-31-17*

DN

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update RF	Update RT	Interval
2	Vial 2	CAL 1 (0.079)	SIMALC1	1	Replace	Replace	
3	Vial 3	CAL 2 (0.158)	SIMALC1	2	Replace	Replace	
4	Vial 4	CAL 3 (0.316)	SIMALC1	3	Replace	Replace	

Sequence Table (Back Injector):

No entries - empty table!

17007
Blu 1.31.17

DN

=====
 Calibration Table
 =====

Calib. Data Modified : Tuesday, January 17, 2017 1:30:56 PM

Calculate : Internal Standard
 Based on : Peak Area

Rel. Reference Window : 5.000 %
 Abs. Reference Window : 0.050 min
 Rel. Non-ref. Window : 5.000 %
 Abs. Non-ref. Window : 0.050 min
 Multiplier : 1.0000
 Dilution : 1.0000
 Sample Amount : 0.00000

Use Multiplier & Dilution Factor with ISTDs
 Uncalibrated Peaks : not reported
 Partial Calibration : No recalibration if peaks missing

Curve Type : Linear
 Origin : Included
 Weight : Equal

Recalibration Settings:
 Average Response : No Update
 Average Retention Time: No Update

Calibration Report Options :
 Printout of recalibrations within a sequence:
 Normal Report after Recalibration

Sample ISTD Information:

ISTD #	ISTD Amount [g/100mL]	Name
1	1.20000e-2	n-Propanol

Signal 1: FID1 A,

RetTime [min]	Lvl Sig	Amount [g/100mL]	Area	Amt/Area	Ref Grp	Name
1.086	1 1	8.00100e-2	990.83179	8.07503e-5	1	Ethanol
	2	1.61200e-1	1999.22754	8.06311e-5		
	3	3.21790e-1	3908.70508	8.23265e-5		
1.764	1 1	1.20000e-2	2862.81689	4.19168e-6	I1	n-Propanol
	2	1.20000e-2	2894.69043	4.14552e-6		
	3	1.20000e-2	2843.25146	4.22052e-6		


17007
 Buo1-31-17

=====
 Peak Sum Table
 =====


No Entries in table
 =====

DN

=====
Calibration Curves
=====

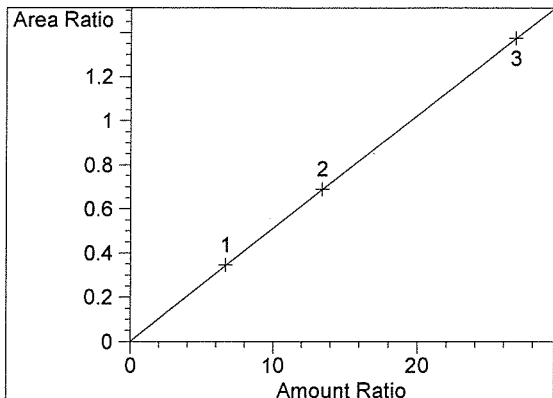

Ethanol at exp. RT: 1.086
FID1 A,
Correlation: 0.99999
Residual Std. Dev.: 0.00241
Formula: $y = mx + b$
m: 5.12191e-2
b: 2.11495e-3
x: Amount Ratio
y: Area Ratio

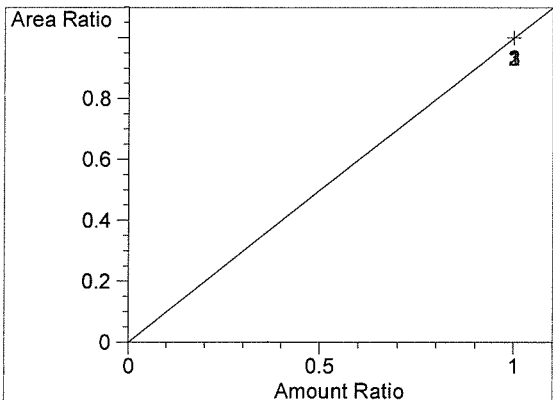

n-Propanol at exp. RT: 1.764
FID1 A,
Correlation: 1.00000
Residual Std. Dev.: 0.00000
Formula: $y = mx + b$
m: 1.00000
b: 0.00000
x: Amount Ratio
y: Area Ratio

=====

17007
Paw 1-31-17

DN


Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:18:52 PM
Instrument: HSGC#1


Sample Name: BLANK
Operator: David Nguyen
Location: Vial 1

Column: DB-ALC1
Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

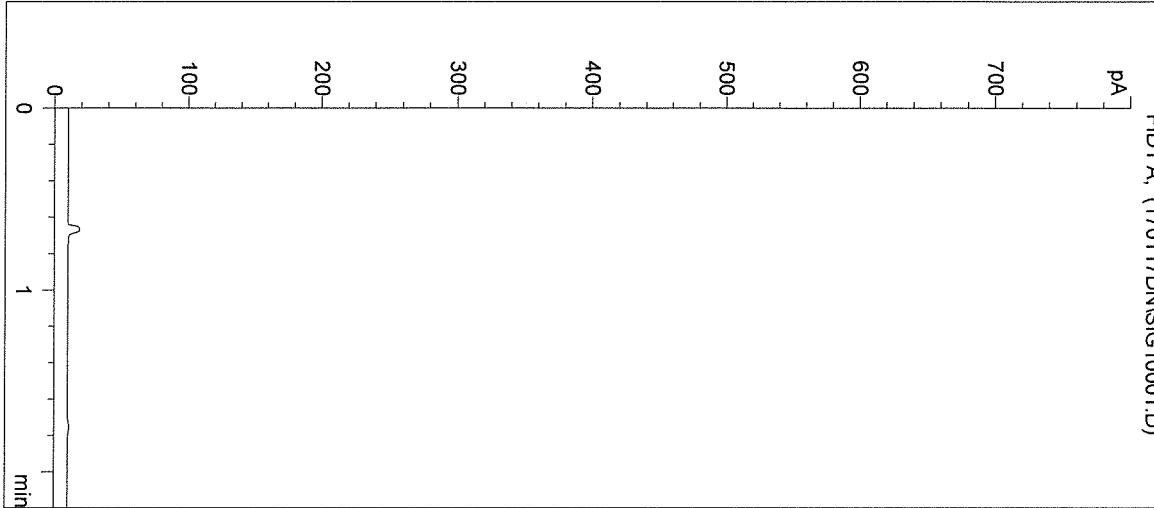


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	0	0.000



Ethanol 0.000 g/100mL

BLW



n-Propanol 0.000 g/100mL


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/17/2017 1:22:09 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info: CAL 1: 0.079 g/100mL
 17007

Sample Name: CAL 1 (0.079)
 Operator: David Nguyen
 Location: Vial 2

->

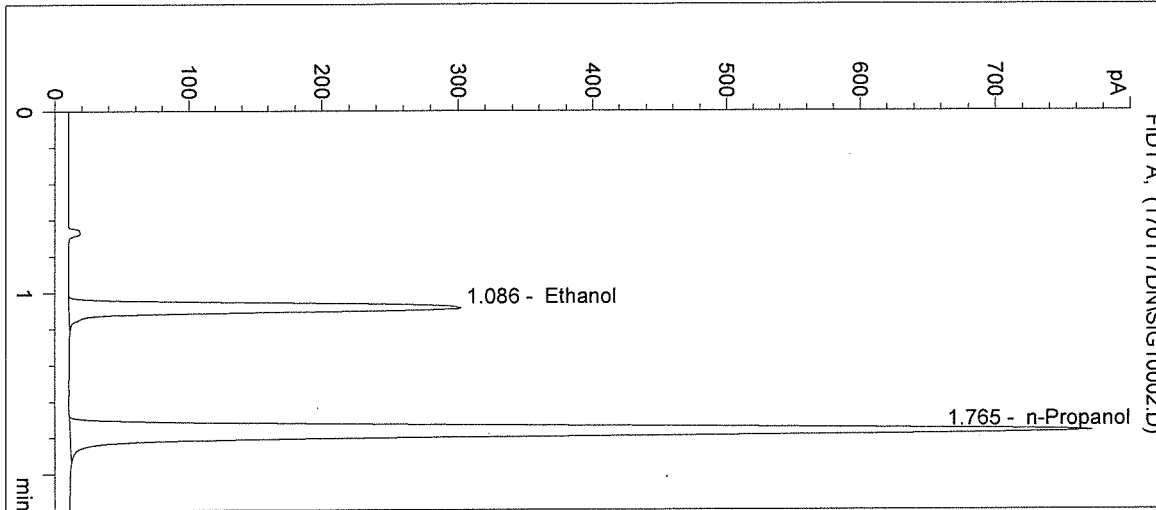


#	Compound	Peak Area	RT (min)
1	Ethanol	991	1.086
2	n-Propanol	2863	1.765

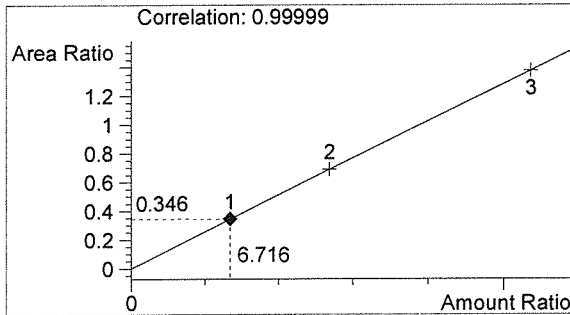

Ethanol 0.081 g/100mL

BLW

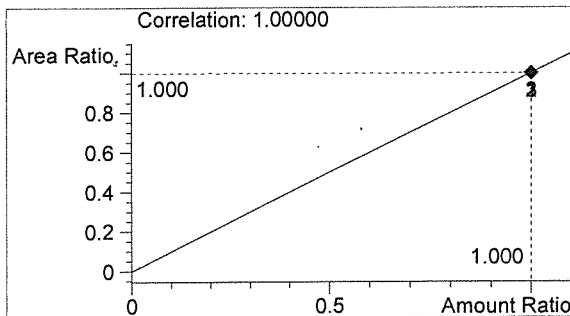


n-Propanol 0.012 g/100mL

DN


Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:25:26 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info: CAL 2: 0.158 g/100mL
 17007

Sample Name: CAL 2 (0.158)
 Operator: David Nguyen
 Location: Vial 3

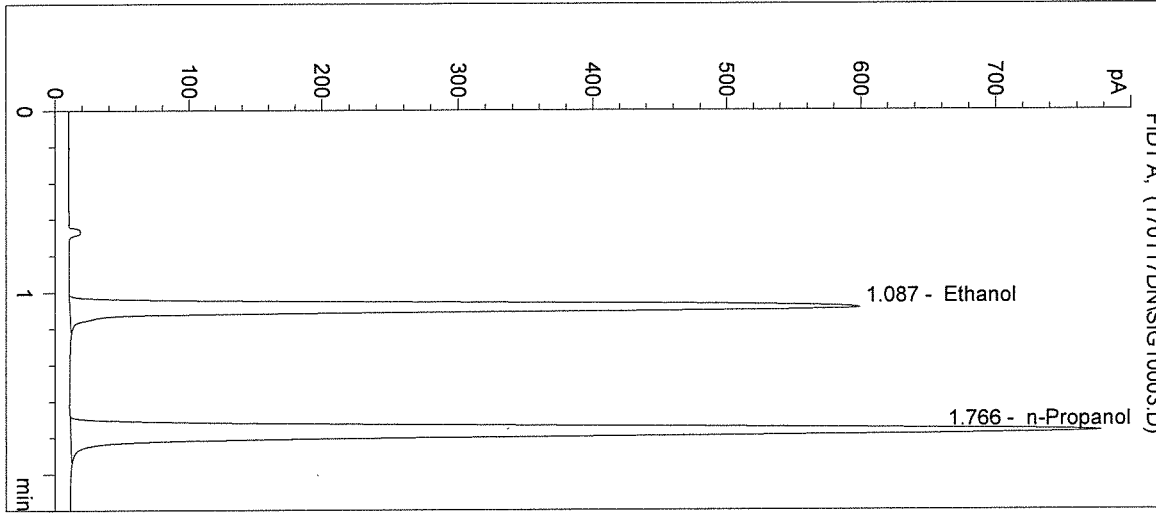


#	Compound	Peak Area	RT (min)
1	Ethanol	1999	1.087
2	n-Propanol	2895	1.766

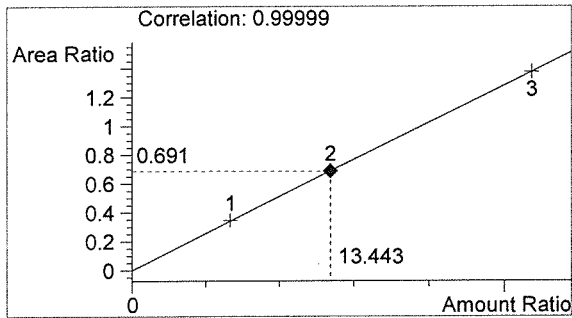

Ethanol 0.161 g/100mL

AWD

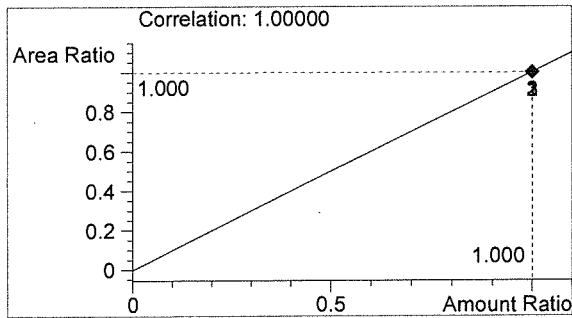

n-Propanol 0.012 g/100mL


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/17/2017 1:28:43 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info: CAL 3: 0.316 g/100mL
 17007

Sample Name: CAL 3 (0.316)
 Operator: David Nguyen
 Location: Vial 4

->

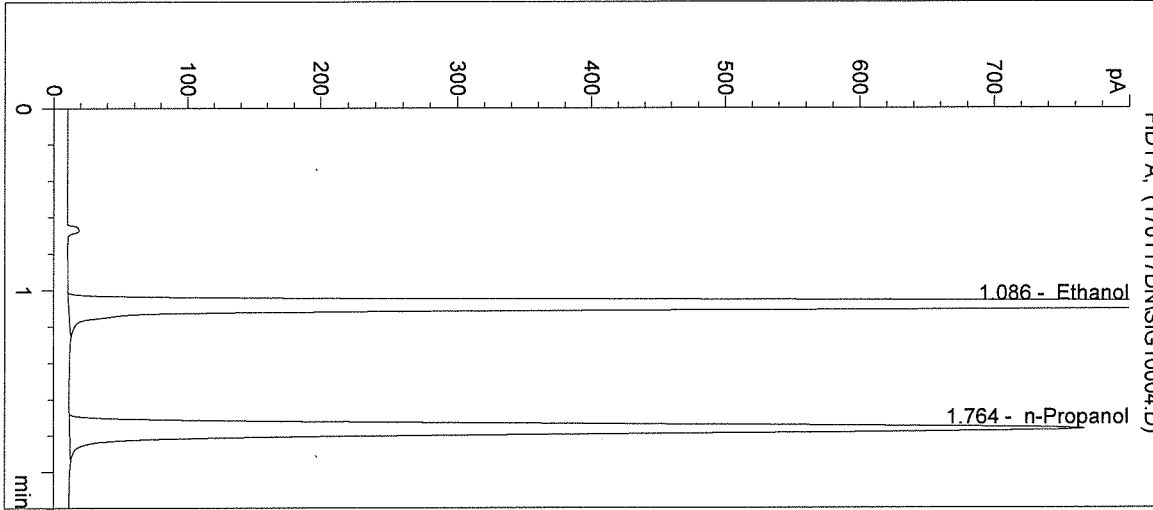


#	Compound	Peak Area	RT (min)
1	Ethanol	3909	1.086
2	n-Propanol	2843	1.764

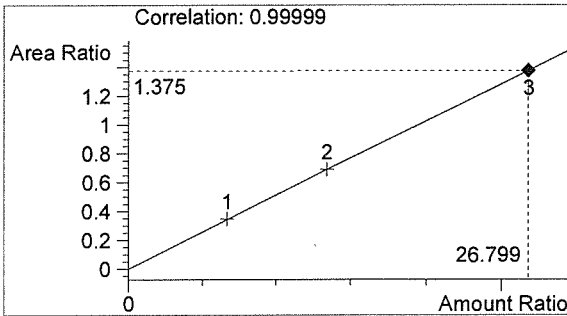

Ethanol 0.322 g/100mL

BW

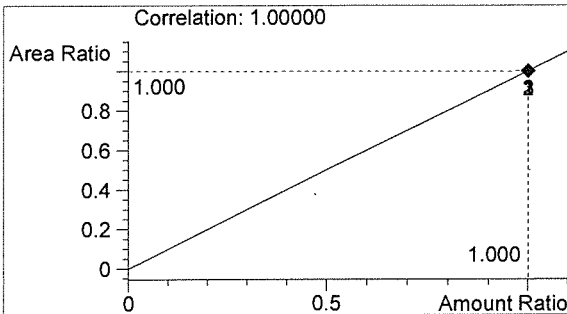


n-Propanol 0.012 g/100mL


DN

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:31:56 PM Sample Name: NEG CTRL
Instrument: HSGC#1 Operator: David Nguyen
Column: DB-ALC1 Location: Vial 5
Method: C:\HPCHEM\1\METHODS\SIMALC1.M
Sample Info: 17007

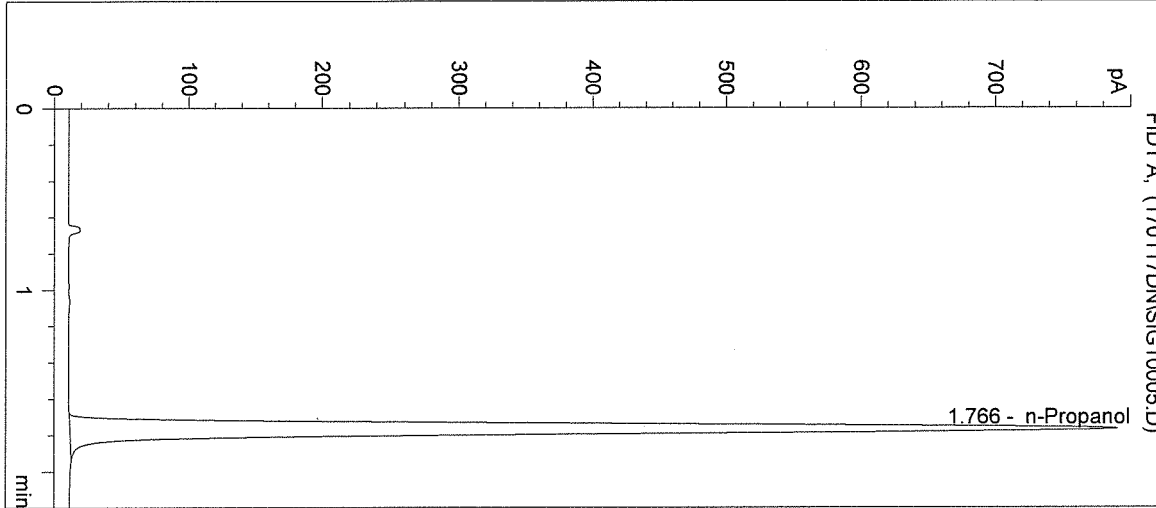


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2944	1.766



Ethanol 0.000 g/100mL

AWO

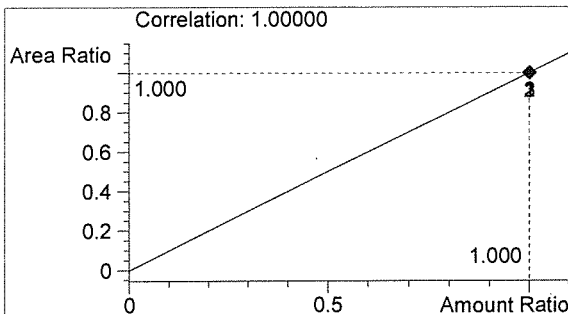


n-Propanol 0.012 g/100mL

DN


Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:35:09 PM
Instrument: HSGC#1
Column: DB-ALC1
Method: C:\HPCHEM\1\METHODS\SIMALC1.M
Sample Info: CTRL 1: 0.04 g/100mL
17007

Sample Name: CTRL 1 (0.04)
Operator: David Nguyen
Location: Vial 6

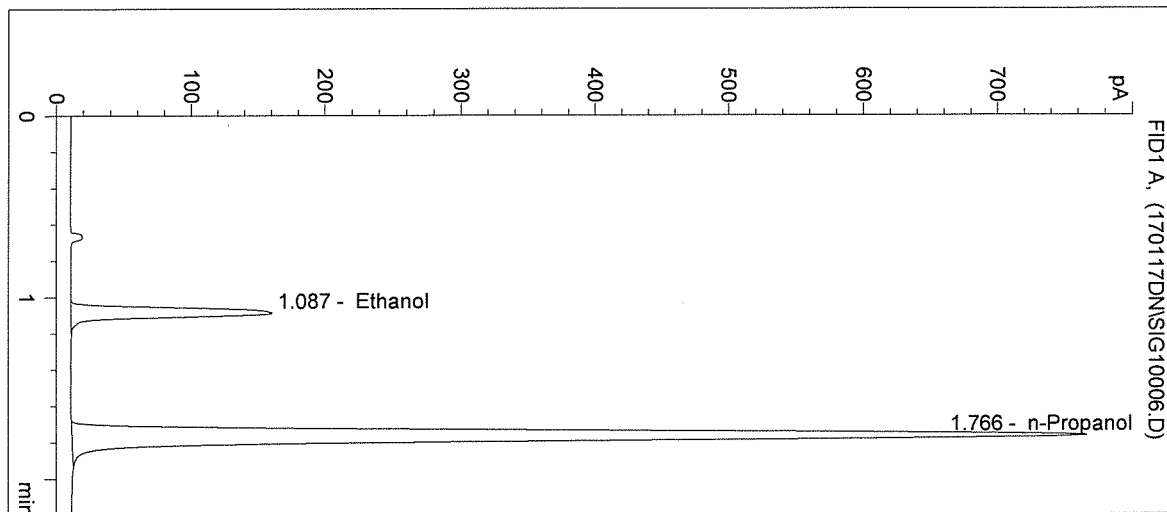


#	Compound	Peak Area	RT (min)
1	Ethanol	506	1.087
2	n-Propanol	2843	1.766

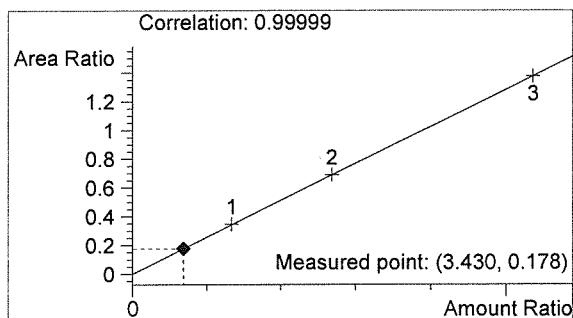

Ethanol 0.041 g/100mL

BW

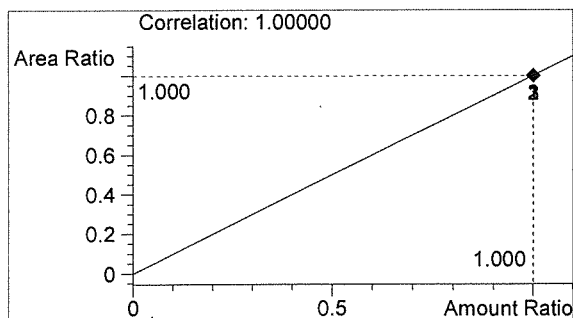


n-Propanol 0.012 g/100mL

DN


Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:38:23 PM Sample Name: CTRL 2 (0.10)
Instrument: HSGC#1 Operator: David Nguyen
Column: DB-ALC1 Location: Vial 7
Method: C:\HPCHEM\1\METHODS\SIMALC1.M
Sample Info: CTRL 2: 0.10 g/100mL
17007

->

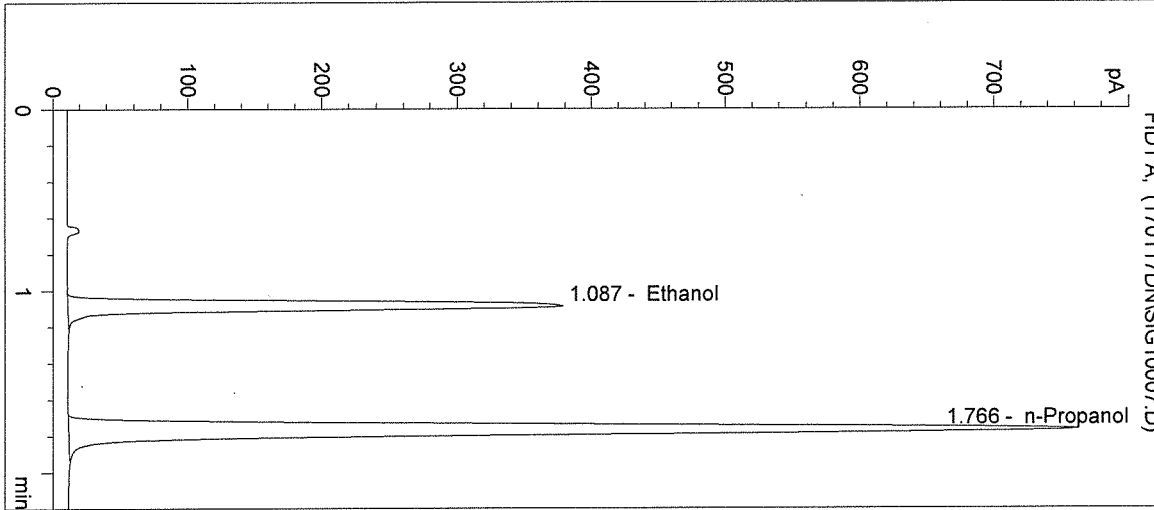


#	Compound	Peak Area	RT (min)
1	Ethanol	1243	1.087
2	n-Propanol	2828	1.766

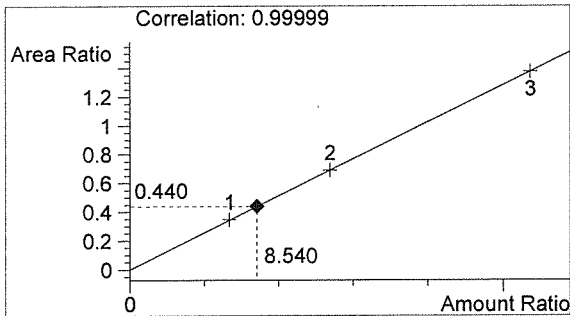

Ethanol 0.102 g/100mL

AWO

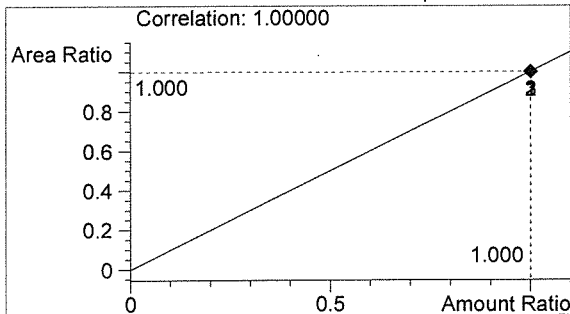

n-Propanol 0.012 g/100mL


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/17/2017 1:41:36 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info: CTRL 3: 0.20 g/100mL
 17007

Sample Name: CTRL 3 (0.20)
 Operator: David Nguyen
 Location: Vial 8

->

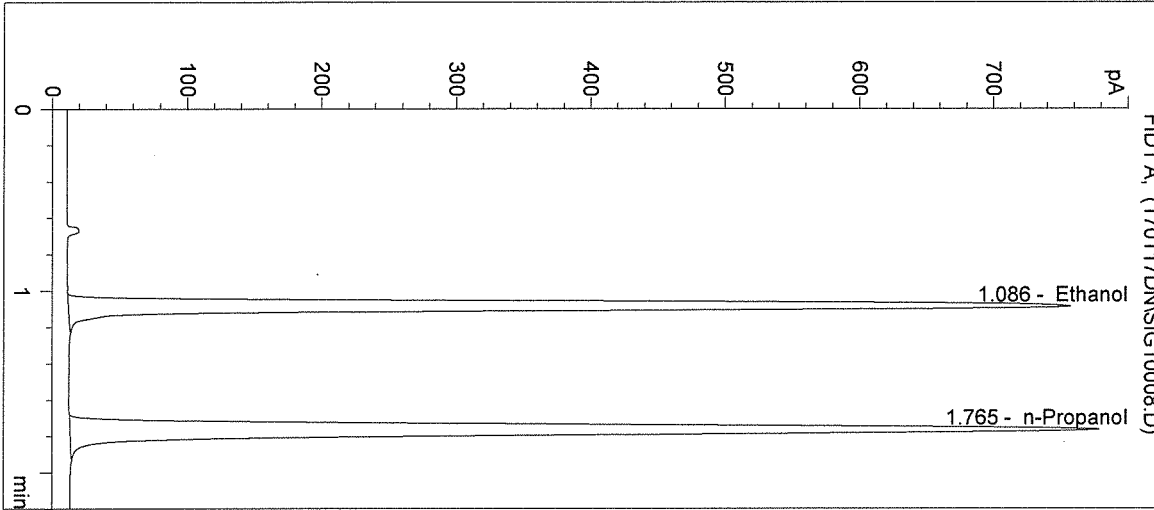


#	Compound	Peak Area	RT (min)
1	Ethanol	2520	1.086
2	n-Propanol	2880	1.765

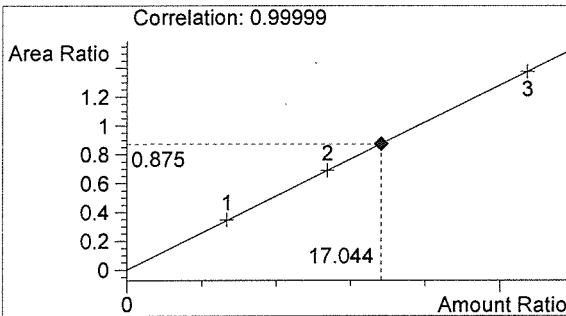

Ethanol 0.205 g/100mL

BLW

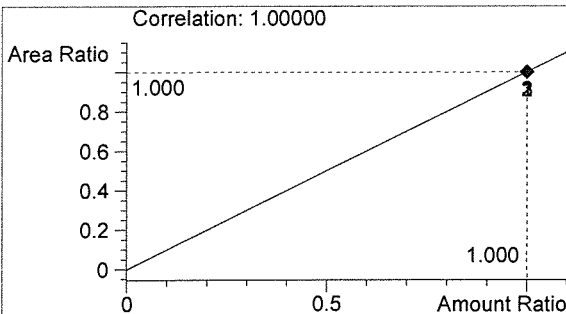

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:44:49 PM

Sample Name: NEG CTRL

Instrument: HSGC#1


Operator: David Nguyen

Column: DB-ALC1


Location: Vial 9

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

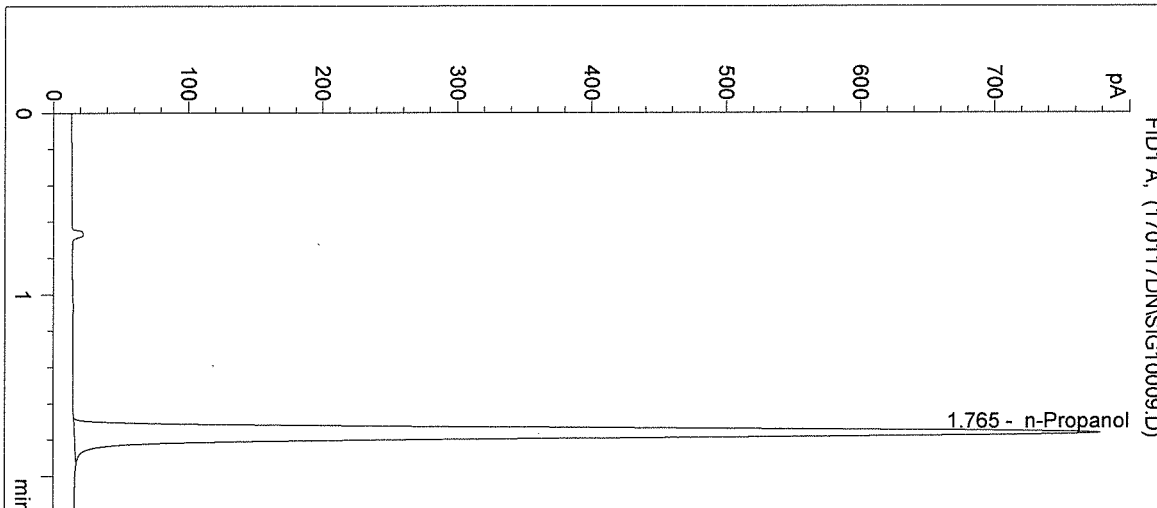


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2871	1.765



Ethanol 0.000 g/100mL

BLW



n-Propanol 0.012 g/100mL


DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/17/2017 1:48:03 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: 17007 #1
 Operator: David Nguyen
 Location: Vial 10

Sample Info:

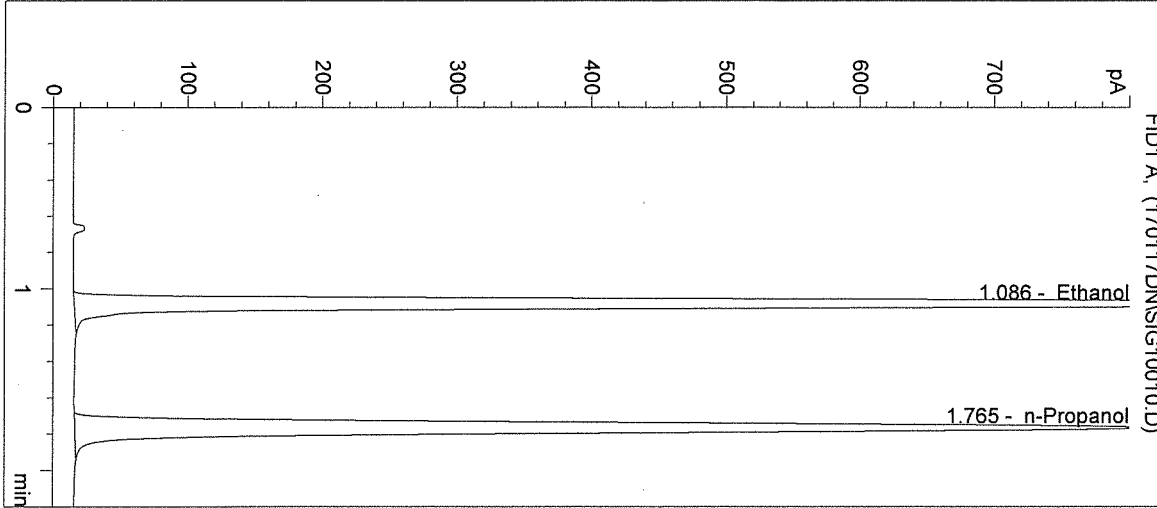


#	Compound	Peak Area	RT (min)
1	Ethanol	3251	1.086
2	n-Propanol	3004	1.765

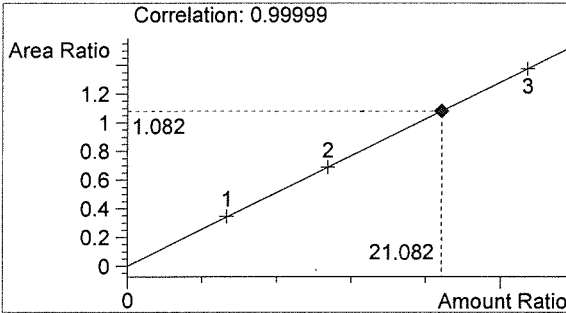

Ethanol 0.253 g/100mL

BW

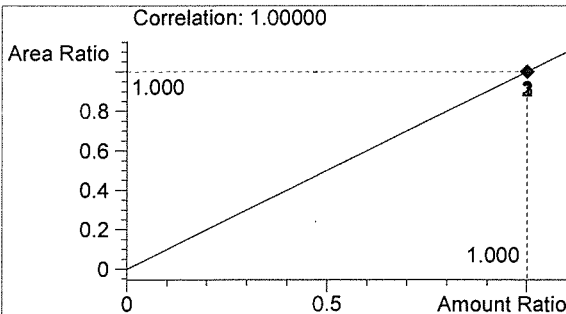

n-Propanol 0.012 g/100mL


D

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134


Inj. Date: 1/17/2017 1:51:15 PM
 Instrument: HSGC#1
 Column: DB-ALC1
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Name: 17007 #2
 Operator: David Nguyen
 Location: Vial 11

Sample Info:

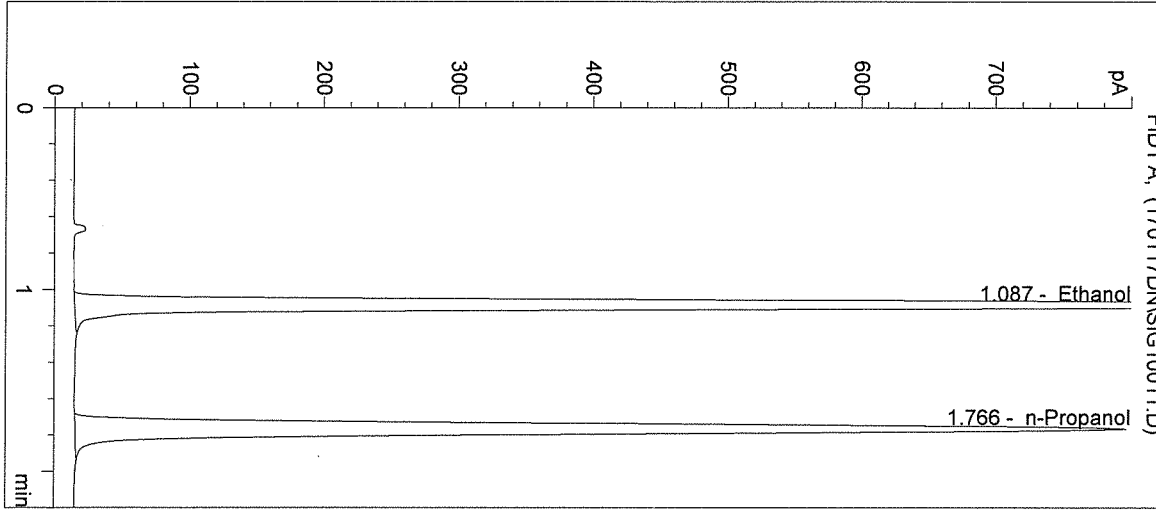


#	Compound	Peak Area	RT (min)
1	Ethanol	3230	1.087
2	n-Propanol	2942	1.766

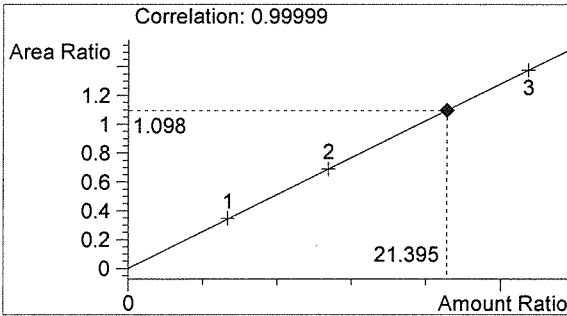

Ethanol 0.257 g/100mL

AWO

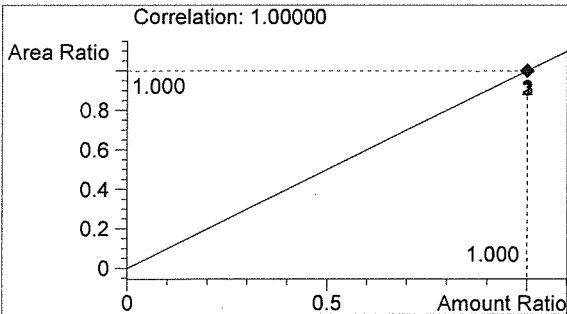

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:54:29 PM

Sample Name: 17007 #3

Instrument: HSGC#1


Operator: David Nguyen

Column: DB-ALC1


Location: Vial 12

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

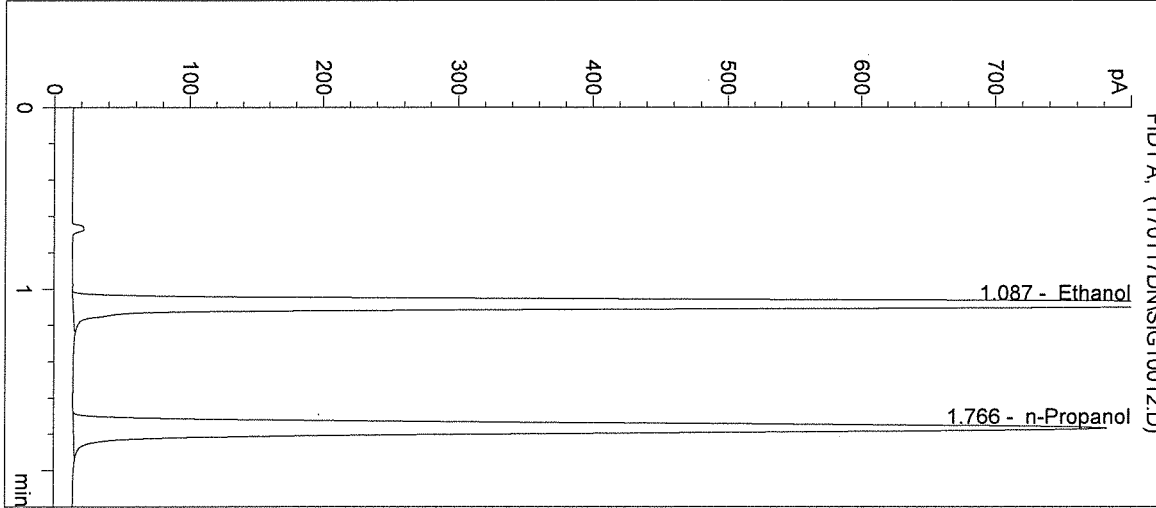


#	Compound	Peak Area	RT (min)
1	Ethanol	3151	1.087
2	n-Propanol	2890	1.766

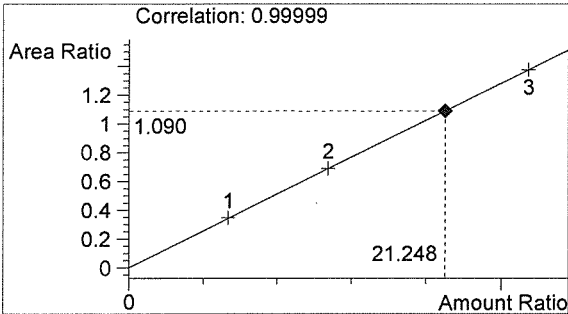

Ethanol 0.255 g/100mL

BLW

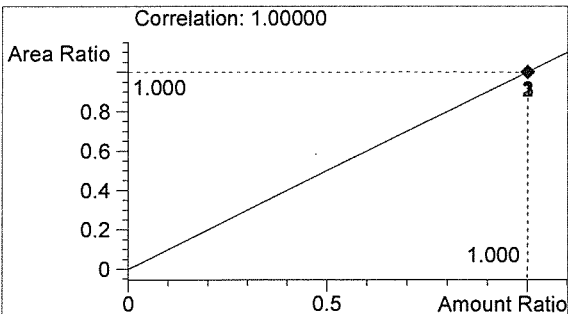

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 1:57:42 PM

Sample Name: 17007 #4

Instrument: HSGC#1


Operator: David Nguyen

Column: DB-ALC1


Location: Vial 13

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

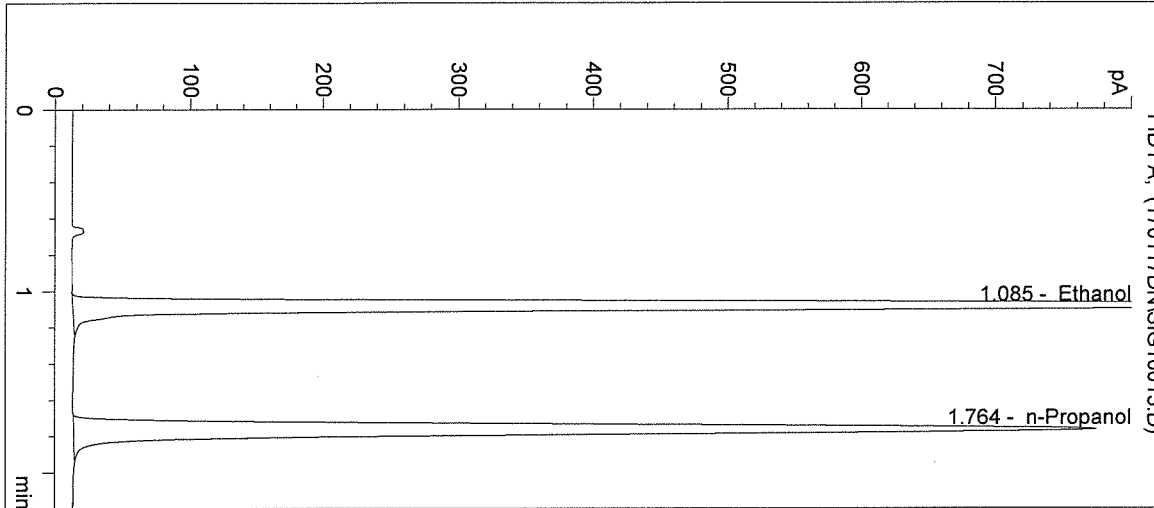


#	Compound	Peak Area	RT (min)
1	Ethanol	3082	1.085
2	n-Propanol	2855	1.764

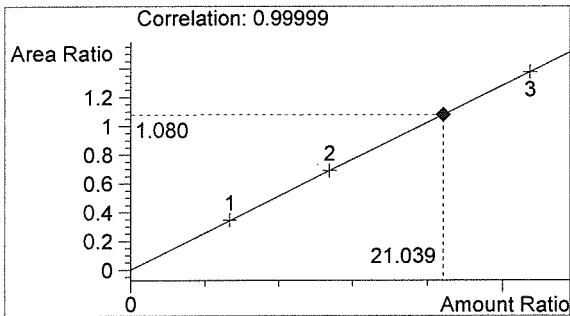

Ethanol 0.252 g/100mL

BLW

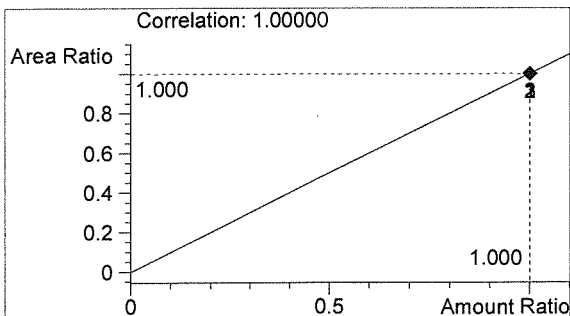

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 2:00:55 PM

Sample Name: 17007 #5

Instrument: HSGC#1


Operator: David Nguyen

Column: DB-ALC1


Location: Vial 14

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

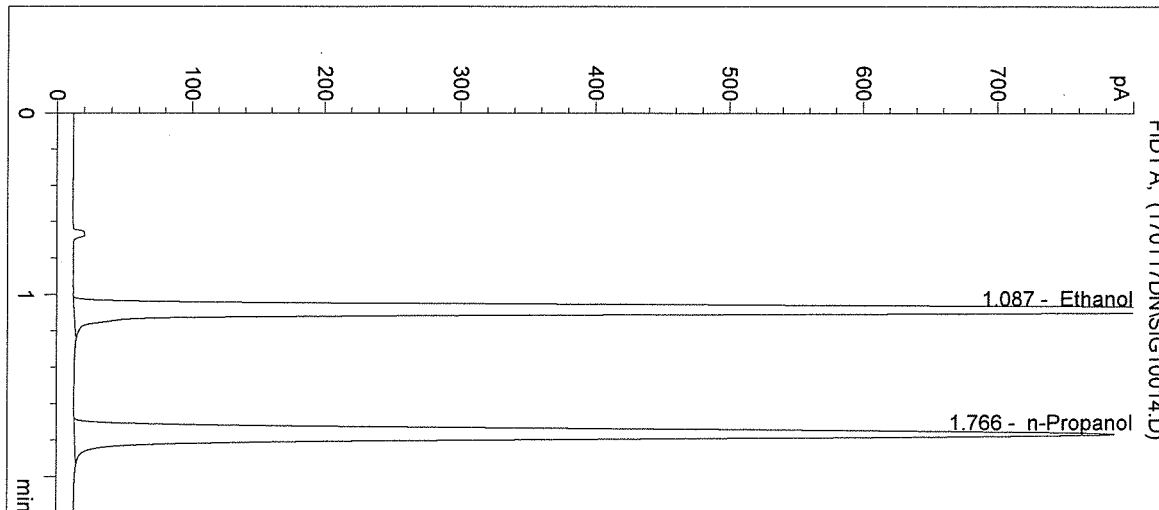


#	Compound	Peak Area	RT (min)
1	Ethanol	3192	1.087
2	n-Propanol	2916	1.766

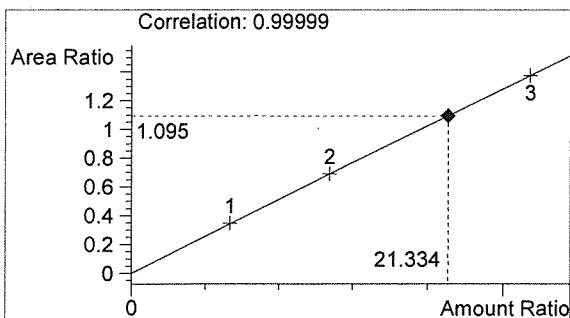

Ethanol 0.256 g/100mL

AWD

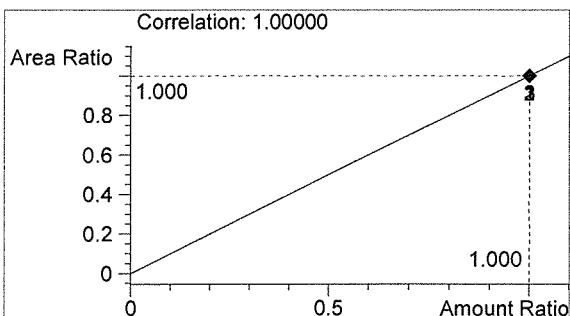

n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 2:04:08 PM

Sample Name: POS CTRL (0.10)

Instrument: HSGC#1

Operator: David Nguyen

Column: DB-ALC1


Location: Vial 15

Method: C:\HPCHEM\1\METHODS\SIMALC1.M


Sample Info: POS CTRL: 0.10 g/100mL

17007

->

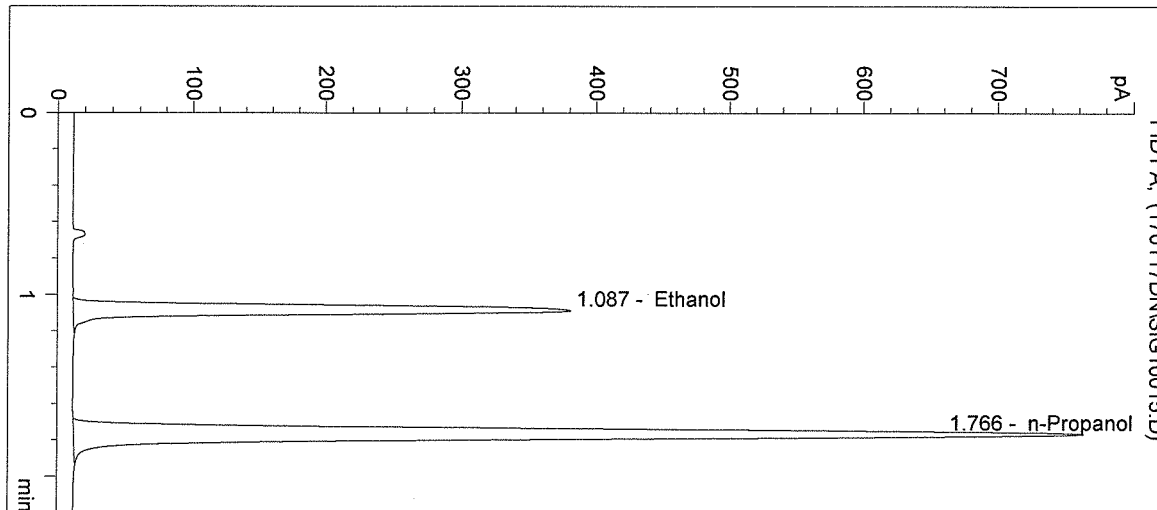


#	Compound	Peak Area	RT (min)
1	Ethanol	1247	1.087
2	n-Propanol	2828	1.766

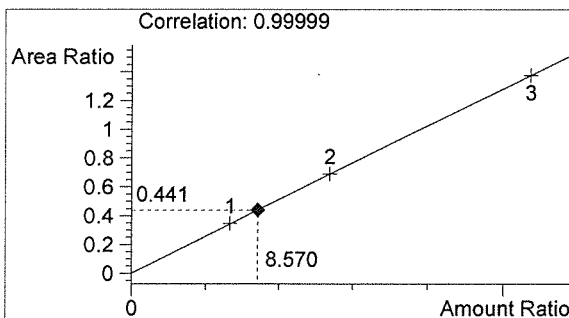

Ethanol 0.103 g/100mL

BLW



n-Propanol 0.012 g/100mL

DN

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 1/17/2017 2:07:21 PM

Sample Name: NEG CTRL

Instrument: HSGC#1


Operator: David Nguyen

Column: DB-ALC1


Location: Vial 16

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17007

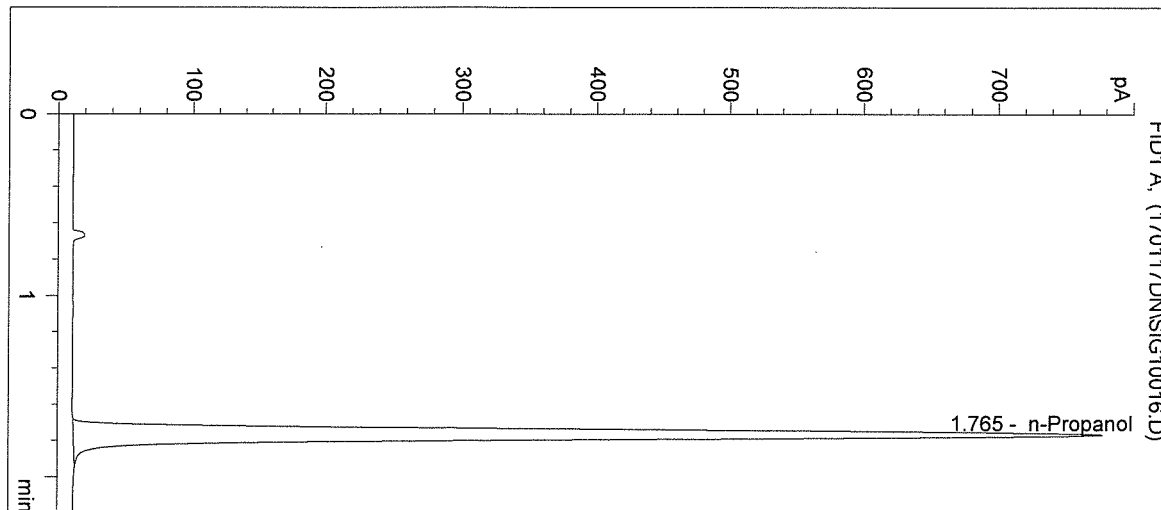


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2884	1.765

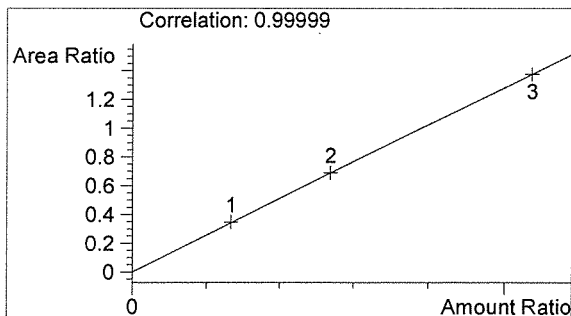

Ethanol 0.000 g/100mL

AWO

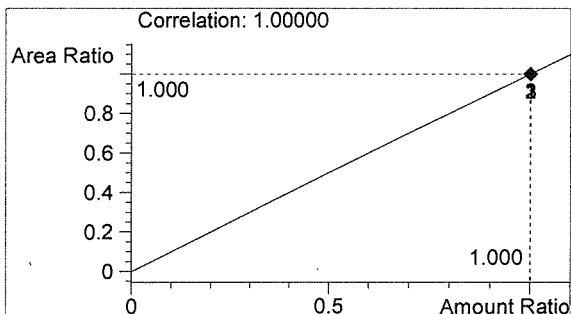

n-Propanol 0.012 g/100mL

DN