



QUALITY ASSURANCE PROCEDURE SOLUTION TEST REPORT

BATCH REPORT: 17027

CUSTOMER INFORMATION

Washington State Patrol – Breath Test Program
811 East Roanoke SEATTLE, WA 98102

TESTING PROCEDURE USED: TLD Technical Manual, Chapter 4.0 Certification of Simulator Solutions;
Headspace-Gas Chromatography.

TESTING ITEM INFORMATION

TARGET VAPOR CONCENTRATION: 0.08 g/210L
DATE PREPARED: 03/10/2017
BATCH UNITS: g/100mL

IDENTITY: QAP Solution
PREPARED BY: Lyndsey Knoy

	LK	AG	CM
1	0.101	0.100	0.099
2	0.101	0.100	0.100
3	0.100	0.100	0.101
4	0.101	0.100	0.100
5	0.101	0.100	0.100
C	0.101	0.102	0.100

ETHANOL CONTROL INFORMATION

LOT NUMBER: FN08051301 EXPIRATION: 10/2018 CONCENTRATION: 0.10 g/100mL

RESULTS OF TESTING

AVERAGE SOLUTION CONCENTRATION: 0.1003 g/100mL PRECISION CV (%): 0.59
STANDARD DEVIATION: 0.00059 NUMBER OF TESTS: 15

EQUIVALENT VAPOR CONCENTRATION: **0.0815 g/210L**
EXPANDED UNCERTAINTY: ± 0.0020 (k=2, 95.45% confidence interval)

WASHINGTON STATE PATROL – TOXICOLOGY LABORATORY DIVISION

Brianne E. O'Reilly
Brianne E. O'Reilly Technical Lead

3.15.17
DATE REPORT ISSUED


ANALYST	NAME	THIS TESTING WAS PERFORMED BY:		DATE TESTED
		SIGNATURE		
LK	Lyndsey Knoy	<u>Lyndsey Knoy</u>		03/10/2017
AG	Andrew Gingras	<u>Andrew Gingras</u>		03/10/2017
CM	Christie Mitchell-Mata	<u>Christie Mitchell-Mata</u>		03/13/2017

SIMULATOR SOLUTION DATA ENTRY REVIEW

Reviewer/s: Amanda M. Black Date: 3-20-17
Location: WSP-FUSB Seattle, WA Solution Batch Number: 17027

	YES	NO	N/A
Analysis dates do not precede preparation date:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Declarations signed and properly dated:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Data entry corresponds to all chromatograms:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
All signatures present on Test Report:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Average solution concentration correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Standard deviation correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
CV (%) correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Equivalent vapor concentration correct:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
All chromatograms and sequences included in file:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Ethanol control information present: (lot # present & used within expiration)	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Complies with accuracy and precision requirements established by the State Toxicologist:	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Comments:

Reviewer Signature:  Date: 3-20-17

Washington State Patrol - Toxicology Laboratory Division
QAP Test Report Calculation Record

QAP Solution Batch #: 17027

Date Prepared: 3/10/2017

Analyst:	LK	AG	CM
Date Tested:	3/10/2017	3/10/2017	3/13/2017
Instrument:	HSGC #1	HSGC #1	HSGC #1
1	0.101	0.100	0.099
2	0.101	0.100	0.100
3	0.100	0.100	0.101
4	0.101	0.100	0.100
5	0.101	0.100	0.100
C	0.101	0.102	0.100

CV^2_{COA}	$CV^2_{QAP\ Solution}$	$CV^2_{Control}$	$CV^2_{Part\ Coef}$
0.0000084100	0.0000023367	0.0000326765	0.0001016326

Ethanol Control Lot #: FN08051301
Control Uncertainty (%): 0.29

Average Solution Concentration: 0.1003 g/100mL
Standard Deviation: 0.00059 g/100mL
Precision CV (%): 0.59
Equivalent Vapor Concentration: 0.0815 g/210L
Combined Standard Uncertainty (\pm): 0.0010 g/210L
Expanded Uncertainty (\pm): 0.0020 coverage factor (k) =2 (95.45% level of confidence)

Calculations performed by: Brianne E. O'Reilly Brianne O'Reilly 3.14.17
Name Signature Date

Calculations verified by: Amanda M. Black [Signature] 3.20.17 Method: Hand calculation
Name Signature Date

Tech. review performed by: Brianne E. O'Reilly Brianne O'Reilly 3.14.17
Name Signature Date

SOLUTION CERTIFICATE REVIEW

Please check that the data on your chromatograms is the data entered into the Test Report, that the date to the right of your name is the date that you tested the solution, and then sign the Test Report.

Please initial and date below to affirm that you have:

- 1) Checked your data
- 2) Checked the date to the right of your name on the Test Report
- 3) Signed the Test Report

	Initials	Date
Amanda Chandler		
Andrew Gingras	<i>AG</i>	3/15/17
Asa Louis		
Brittany Thomas		
Christie Mitchell-Mata	<i>CM</i>	3/15/17
Christopher Johnston		
David Nguyen		
Dawn Sklerov		
Elizabeth Wehner		
Justin Knoy		
Katie Harris		
Lyndsey Knoy	<i>LK</i>	3.15.17
Naziha Nuwayhid		
Rebecca Flaherty		

17027

Batch # _____

BW 3.14.17

JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.08 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 17027**


I, Lyndsey Knoy, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Chemistry.

The quality assurance procedure (QAP) solution, Lot Number 17027, was prepared in the Washington State Toxicology Laboratory on 3/10/2017. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 3/10/2018.

Seattle, WA

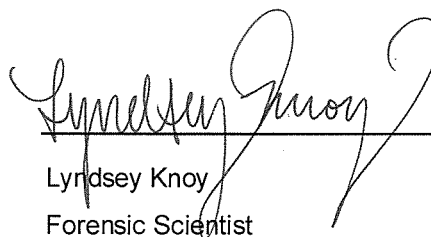 3.15.17
Lyndsey Knoy Date
Forensic Scientist



JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.08 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 17027**

I, Andrew Gingras, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BS degree in Cell and Molecular Biology and MS degree in Forensic Science.

The quality assurance procedure (QAP) solution, Lot Number 17027, was prepared in the Washington State Toxicology Laboratory on 3/10/2017. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 3/10/2018.

Seattle, WA

 3/15/2017

Andrew Gingras
Forensic Scientist

Date



JAY INSLEE
Governor



JOHN R. BATISTE
Chief

STATE OF WASHINGTON
WASHINGTON STATE PATROL
WASHINGTON STATE TOXICOLOGY LABORATORY

2203 Airport Way South, Suite 360 • Seattle, Washington 98134-2027 • (206) 262-6100 • FAX (206) 262-6145

**0.08 g/210 L QUALITY ASSURANCE PROCEDURE SOLUTION
CERTIFICATION FOR LOT 17027**

I, Christie Mitchell-Mata, do certify under penalty of perjury that:

I am employed by the Washington State Toxicology Laboratory, and my responsibilities include the preparation and certification of alcohol solutions for use with evidential breath test instruments.

I possess the following qualifications: BA degree in Chemistry, MFS degree in Forensic Science.

The quality assurance procedure (QAP) solution, Lot Number 17027, was prepared in the Washington State Toxicology Laboratory on 3/10/2017. I tested this solution and it was found to conform to those standards established by the State Toxicologist for the certification of simulator solution. It shall not be used to perform a quality assurance procedure after 3/10/2018.

Seattle, WA

 3/15/17

Christie Mitchell-Mata

Date

Forensic Toxicologist



FILE A COPY IN THE BATCH FILE FOR EACH SOLUTION LISTED ON THE WORKSHEET

Preparation Date: 3.10.17 Expiration Date: 3.10.18 Initials of Preparer: LKLot # of 200-proof Ethanol used in preparation: 2FE01309Date the 200-proof Ethanol bottle was opened: 3.7.17

After opening, each bottle of 200-proof Ethanol is approved for use for 6 months unless an extension is approved by the State Toxicologist. This timeframe applies to the 200-proof Ethanol only, not to simulator solutions which have a 1 year expiration.

Environmental conditions verified as acceptable:

Simulator Solution	Volume of Ethanol (mL)	Volume of Deionized Water (L)		Batch Number
QAP 0.04	11.2	18	<input checked="" type="checkbox"/>	<u>17026</u>
QAP 0.08	22.4	18	<input checked="" type="checkbox"/>	<u>17027</u>
QAP 0.10	28.1	18	<input checked="" type="checkbox"/>	<u>17028</u>
QAP 0.15	42.1	18	<input checked="" type="checkbox"/>	<u>17029</u>
QAP 0.20	56.1	18	<input type="checkbox"/>	
ESS	66.5	52	<input type="checkbox"/>	

Stir bar is rotating Stirred for minimum 30 minutes; 2 hours for ESS Spigot purged Aliquot taken Batch labeled, packaged and sealed 3.10.17
Date

If different ethanol lot numbers are used in the preparation of solutions, record them and the corresponding solution batch numbers in the comments section.

Comments:

_____*Imelda Murray*
Analyst Signature3.10.17
Date17027
BLW 3.14.17

Sequence Parameters:

Operator: Lyndsey Knoy
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 170310LK
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

Ethanol Calibrator 1 0.079 g/100 mL, E0217-01 - Exp. 08/21/17
 Ethanol Calibrator 2 0.158 g/100 mL, E0217-02 - Exp. 08/21/17
 Ethanol Calibrator 3 0.316 g/100 mL, E0217-03 - Exp. 08/21/17

 0.04 Control - Lot #FN12181501 - Exp. 12/2020
 0.10 Control - Lot #FN08051301 - Exp. 10/2018
 0.20 Control - Lot #FN08101505 - Exp. 02/2021

 ISTD Lot#P0117 - Exp. 04/20/2017

 Calibration 1-9 filed with 17026

17027
 BLW 3.14.17

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	Negative CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	Negative CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	17026 #1	SIMALC1	1	Sample		
11	Vial 11	17026 #2	SIMALC1	1	Sample		
12	Vial 12	17026 #3	SIMALC1	1	Sample		
13	Vial 13	17026 #4	SIMALC1	1	Sample		
14	Vial 14	17026 #5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	Negative CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	17027 #1	SIMALC1	1	Sample		
18	Vial 18	17027 #2	SIMALC1	1	Sample		
19	Vial 19	17027 #3	SIMALC1	1	Sample		
20	Vial 20	17027 #4	SIMALC1	1	Sample		
21	Vial 21	17027 #5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	Negative CTRL	SIMALC1	1	Ctrl Samp		
24	Vial 24	17028 #1	SIMALC1	1	Sample		

for

for

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
25	Vial 25	17028 #2	SIMALC1	1	Sample		
26	Vial 26	17028 #3	SIMALC1	1	Sample		
27	Vial 27	17028 #4	SIMALC1	1	Sample		
28	Vial 28	17028 #5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL	SIMALC1	1	Ctrl Samp		
30	Vial 30	Negative CTRL	SIMALC1	1	Ctrl Samp		
31	Vial 31	17029 #1	SIMALC1	1	Sample		
32	Vial 32	17029 #2	SIMALC1	1	Sample		
33	Vial 33	17029 #3	SIMALC1	1	Sample		
34	Vial 34	17029 #4	SIMALC1	1	Sample		
35	Vial 35	17029 #5	SIMALC1	1	Sample		
36	Vial 36	0.10 CTRL	SIMALC1	1	Ctrl Samp		
37	Vial 37	Negative CTRL	SIMALC1	1	Ctrl Samp		
38	Vial 38	17030 #1	SIMALC1	1	Sample		
39	Vial 39	17030 #2	SIMALC1	1	Sample		
40	Vial 40	17030 #3	SIMALC1	1	Sample		
41	Vial 41	17030 #4	SIMALC1	1	Sample		
42	Vial 42	17030 #5	SIMALC1	1	Sample		
43	Vial 43	0.10 CTRL	SIMALC1	1	Ctrl Samp		
44	Vial 44	Negative CTRL	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):


No entries - empty table!

17027
Bw 3.14.17


JK

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 12:00:28 PM Sample Name: 17027 #1
 Instrument: HSGC#1 Operator: Lyndsey Knoy
 Column: DB-ALC1 Location: Vial 17
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info:

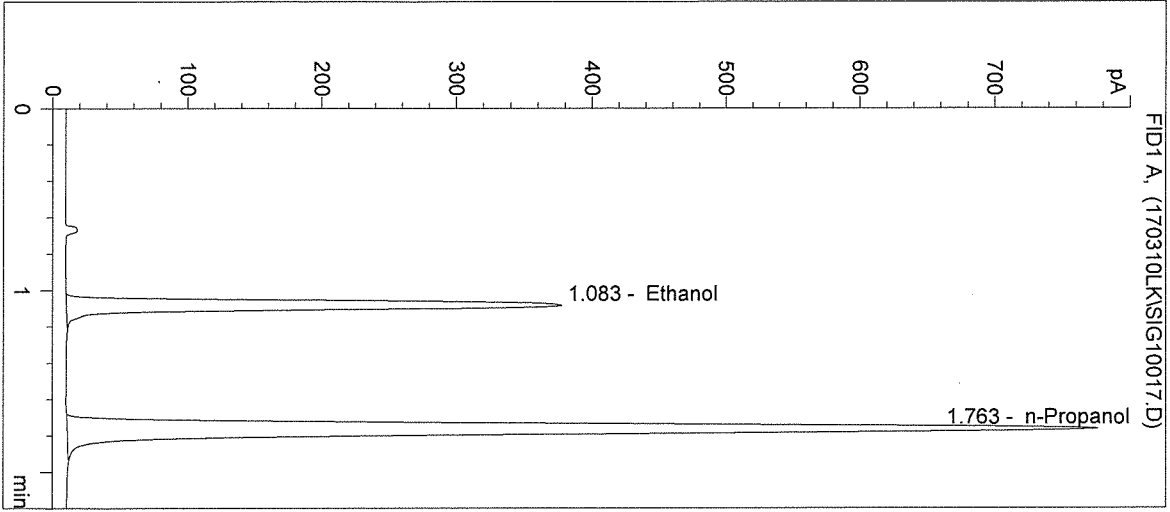


#	Compound	Peak Area	RT (min)
1	Ethanol	1226	1.083
2	n-Propanol	2872	1.763

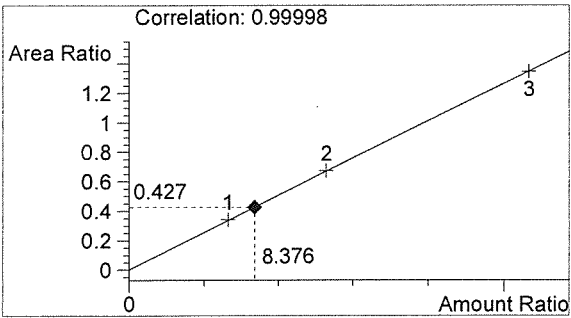

Ethanol 0.101 g/100mL

AWD

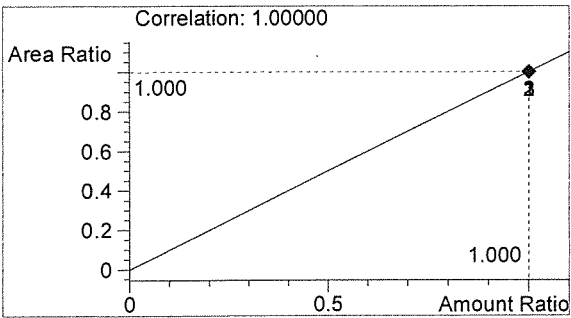

n-Propanol 0.012 g/100mL

fw

Inj. Date: 3/10/2017 12:03:42 PM

Sample Name: 17027 #2

Instrument: HSGC#1


Operator: Lyndsey Knoy

Column: DB-ALC1


Location: Vial 18

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

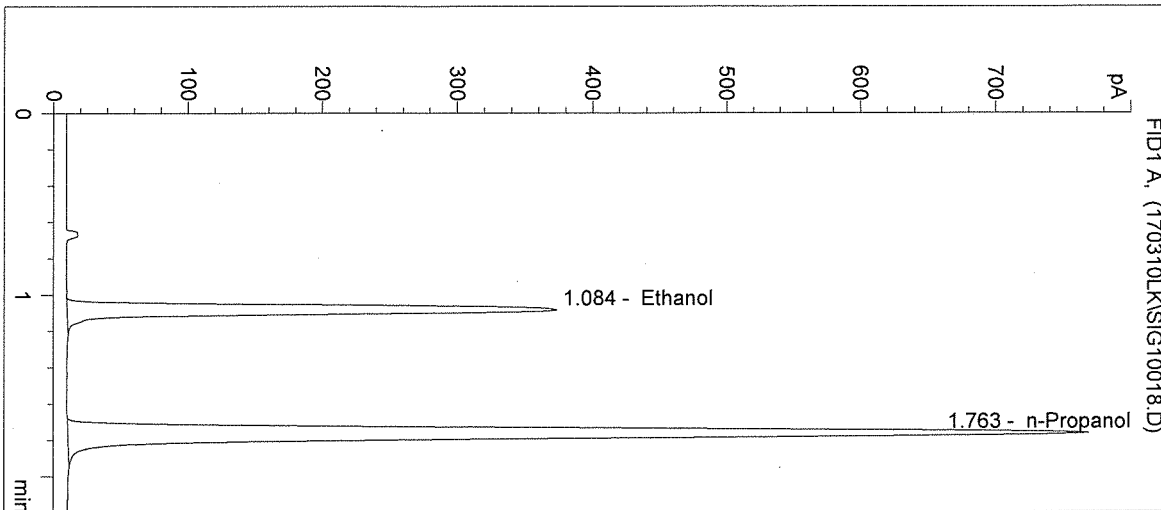


#	Compound	Peak Area	RT (min)
1	Ethanol	1218	1.084
2	n-Propanol	2852	1.763

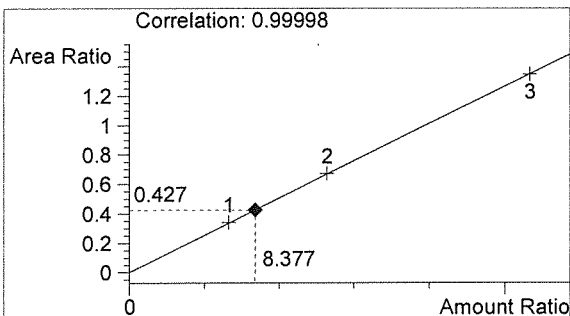

Ethanol 0.101 g/100mL

AW

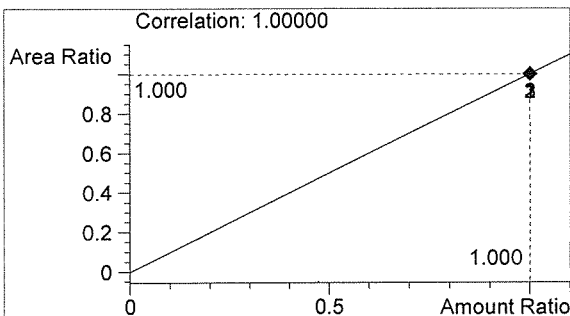


n-Propanol 0.012 g/100mL


AW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 12:06:55 PM Sample Name: 17027 #3
 Instrument: HSGC#1 Operator: Lyndsey Knoy
 Column: DB-ALC1 Location: Vial 19
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info:

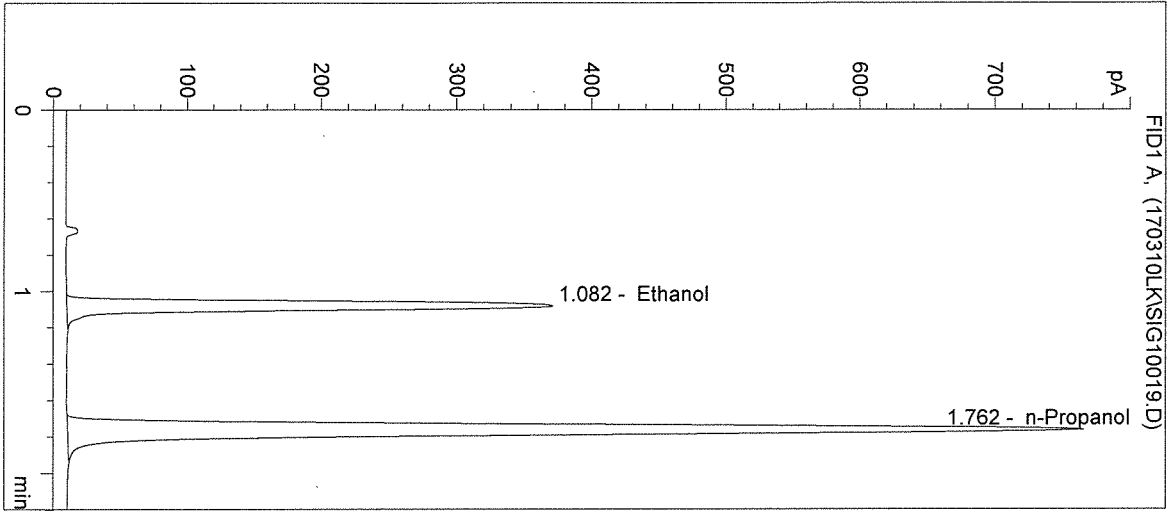


#	Compound	Peak Area	RT (min)
1	Ethanol	1205	1.082
2	n-Propanol	2826	1.762

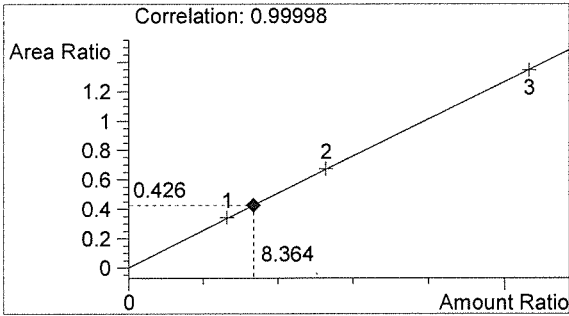

Ethanol 0.100 g/100mL

BW

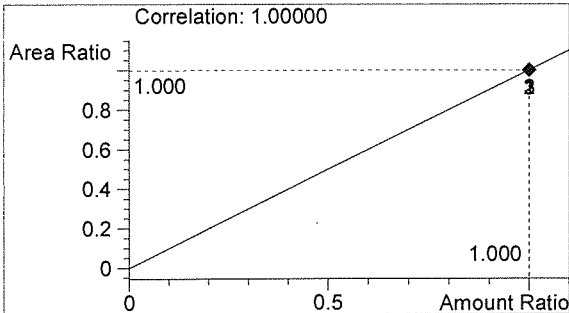

n-Propanol 0.012 g/100mL

JK

Inj. Date: 3/10/2017 12:10:08 PM

Sample Name: 17027 #4

Instrument: HSGC#1


Operator: Lyndsey Knoy

Column: DB-ALC1


Location: Vial 20

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

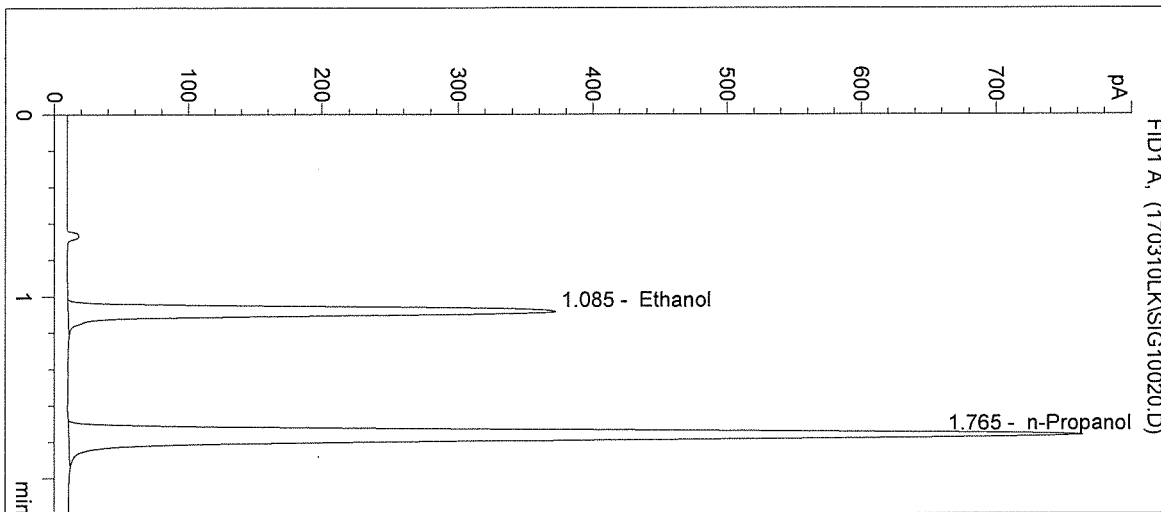


#	Compound	Peak Area	RT (min)
1	Ethanol	1221	1.085
2	n-Propanol	2841	1.765

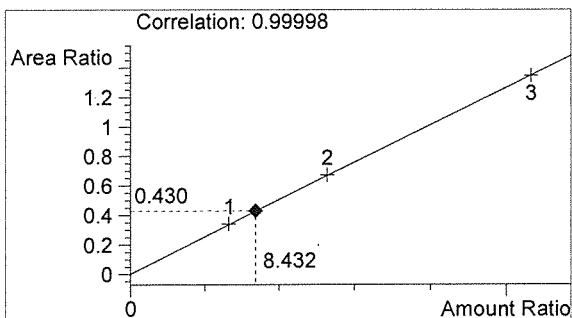

Ethanol 0.101 g/100mL

AWO

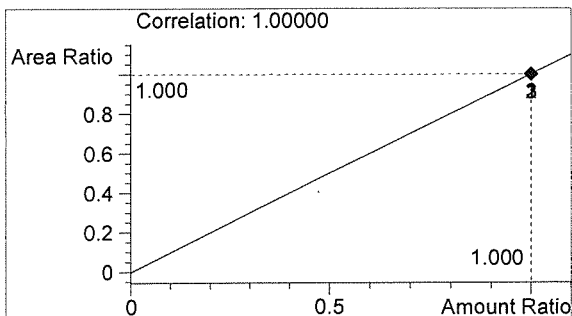


n-Propanol 0.012 g/100mL


JK

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 12:13:21 PM Sample Name: 17027 #5
 Instrument: HSGC#1 Operator: Lyndsey Knoy
 Column: DB-ALC1 Location: Vial 21
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info:

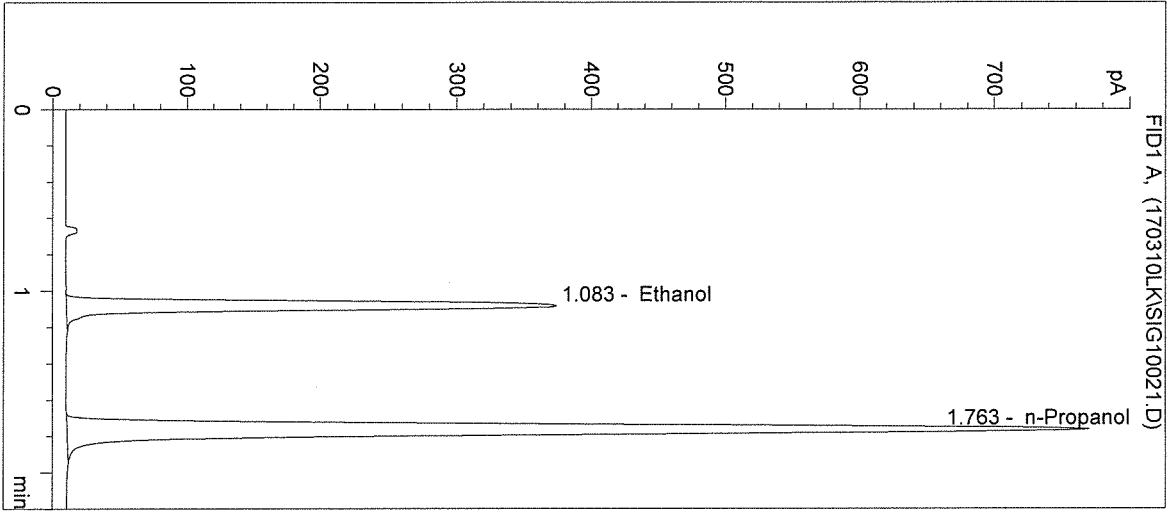


#	Compound	Peak Area	RT (min)
1	Ethanol	1216	1.083
2	n-Propanol	2846	1.763

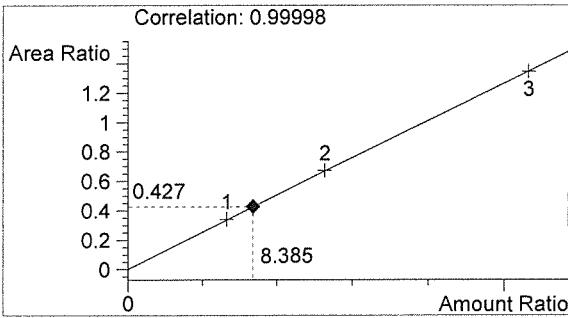

Ethanol 0.101 g/100mL

AW

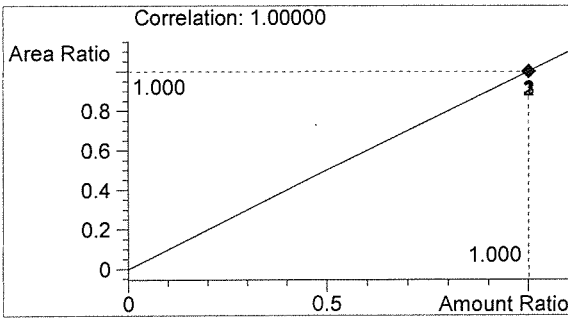


n-Propanol 0.012 g/100mL


JK

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 12:16:34 PM Sample Name: 0.10 CTRL
 Instrument: HSGC#1 Operator: Lyndsey Knoy
 Column: DB-ALC1 Location: Vial 22
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info: 17027

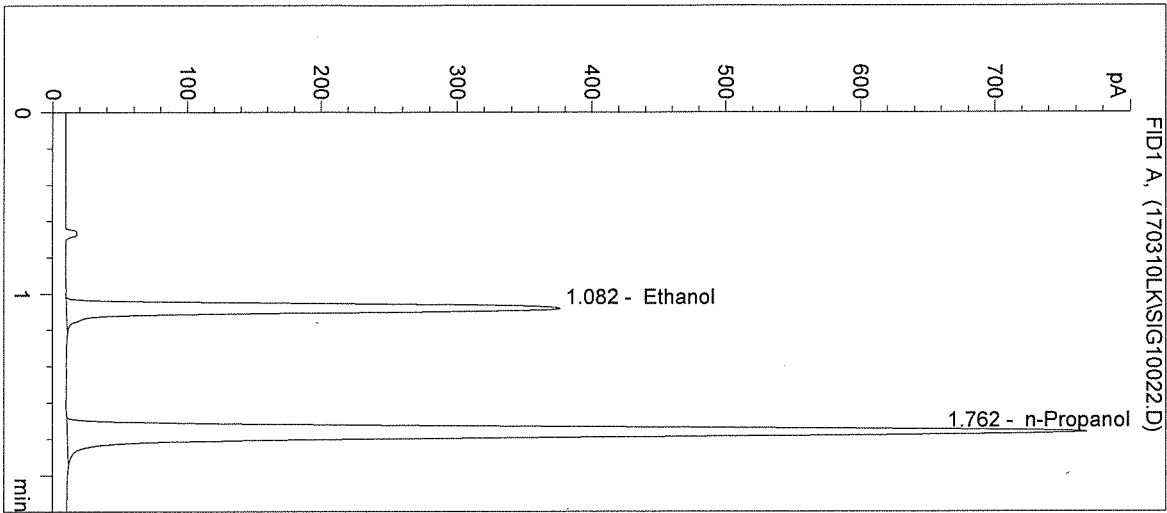


#	Compound	Peak Area	RT (min)
1	Ethanol	1225	1.082
2	n-Propanol	2847	1.762

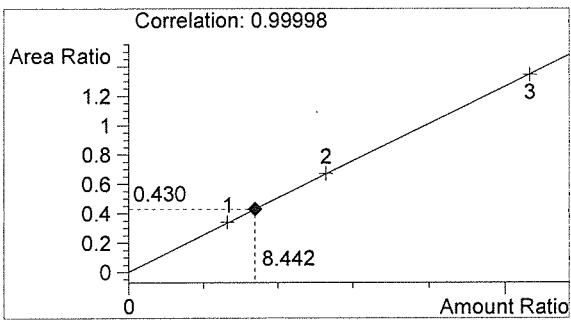

Ethanol 0.101 g/100mL

AW

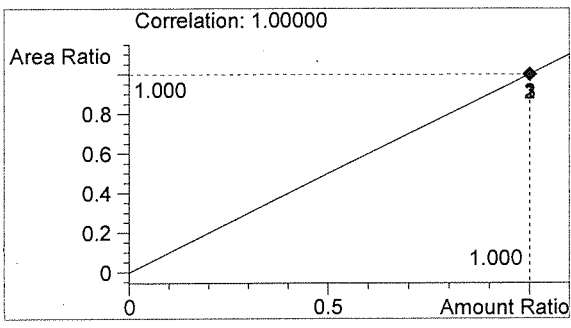


n-Propanol 0.012 g/100mL


JK

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 12:19:48 PM Sample Name: Negative CTRL
Instrument: HSGC#1 Operator: Lyndsey Knoy
Column: DB-ALC1 Location: Vial 23
Method: C:\HPCHEM\1\METHODS\SIMALC1.M
Sample Info: 17027

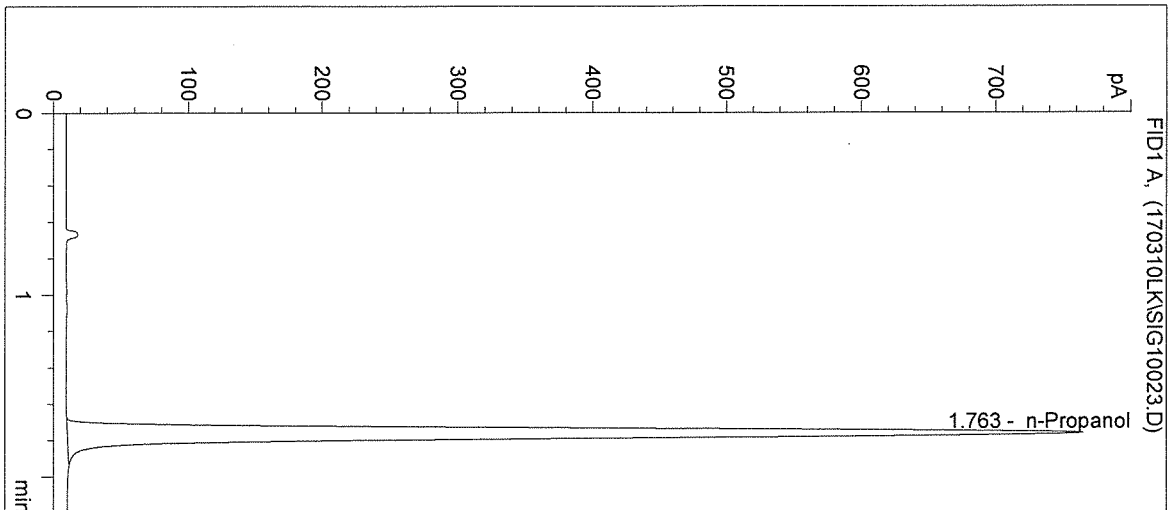


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2834	1.763

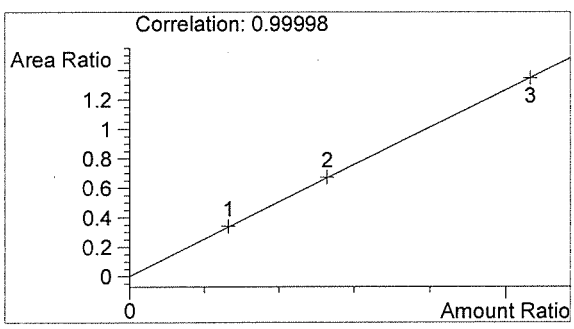

Ethanol 0.000 g/100mL

PLW

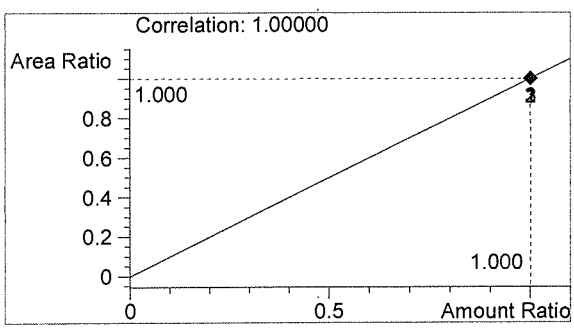

n-Propanol 0.012 g/100mL

JK

Sequence Parameters:

Operator: Andrew Gingras
 Data File Naming: Prefix/Counter
 Signal 1 Prefix: SIG1
 Counter: 0001
 Signal 2 Prefix: SIG2
 Counter: 0001
 Data Directory: C:\HPCHEM\1\DATA\
 Data Subdirectory: 170310A2
 Part of Methods to run: According to Runtime Checklist
 Barcode Reader: not used
 Shutdown Cmd/Macro: none

Sequence Comment:

Ethanol Calibrator 1 0.079 g/100 mL, E0217-01 - Exp. 08/21/17
 Ethanol Calibrator 2 0.158 g/100 mL, E0217-02 - Exp. 08/21/17
 Ethanol Calibrator 3 0.316 g/100 mL, E0217-03 - Exp. 08/21/17

 0.04 Control - Lot #FN12181501 - Exp. 12/2020
 0.10 Control - Lot #FN08051301 - Exp. 10/2018
 0.20 Control - Lot #FN08101505 - Exp. 02/2021

 ISTD Lot#P0117 - Exp. 04/20/2017

 Calibration 1-9 filed with 17026
 Diluter #3

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	Negative CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	Negative CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	17026 #1	SIMALC1	1	Sample		
11	Vial 11	17026 #2	SIMALC1	1	Sample		
12	Vial 12	17026 #3	SIMALC1	1	Sample		
13	Vial 13	17026 #4	SIMALC1	1	Sample		
14	Vial 14	17026 #5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	Negative CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	17027 #1	SIMALC1	1	Sample		
18	Vial 18	17027 #2	SIMALC1	1	Sample		
19	Vial 19	17027 #3	SIMALC1	1	Sample		
20	Vial 20	17027 #4	SIMALC1	1	Sample		
21	Vial 21	17027 #5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	Negative CTRL	SIMALC1	1	Ctrl Samp		

17027
 Buo 3-14-17

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
24	Vial 24	17028 #1	SIMALC1	1	Sample		
25	Vial 25	17028 #2	SIMALC1	1	Sample		
26	Vial 26	17028 #3	SIMALC1	1	Sample		
27	Vial 27	17028 #4	SIMALC1	1	Sample		
28	Vial 28	17028 #5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL	SIMALC1	1	Ctrl Samp		
30	Vial 30	Negative CTRL	SIMALC1	1	Ctrl Samp		
31	Vial 31	17029 #1	SIMALC1	1	Sample		
32	Vial 32	17029 #2	SIMALC1	1	Sample		
33	Vial 33	17029 #3	SIMALC1	1	Sample		
34	Vial 34	17029 #4	SIMALC1	1	Sample		
35	Vial 35	17029 #5	SIMALC1	1	Sample		
36	Vial 36	0.10 CTRL	SIMALC1	1	Ctrl Samp		
37	Vial 37	Negative CTRL	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

17027
Bao 3.14.17

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 2:47:39 PM

Sample Name: 17027 #1

Instrument: HSGC#1


Operator: Andrew Gingras

Column: DB-ALC1


Location: Vial 17

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

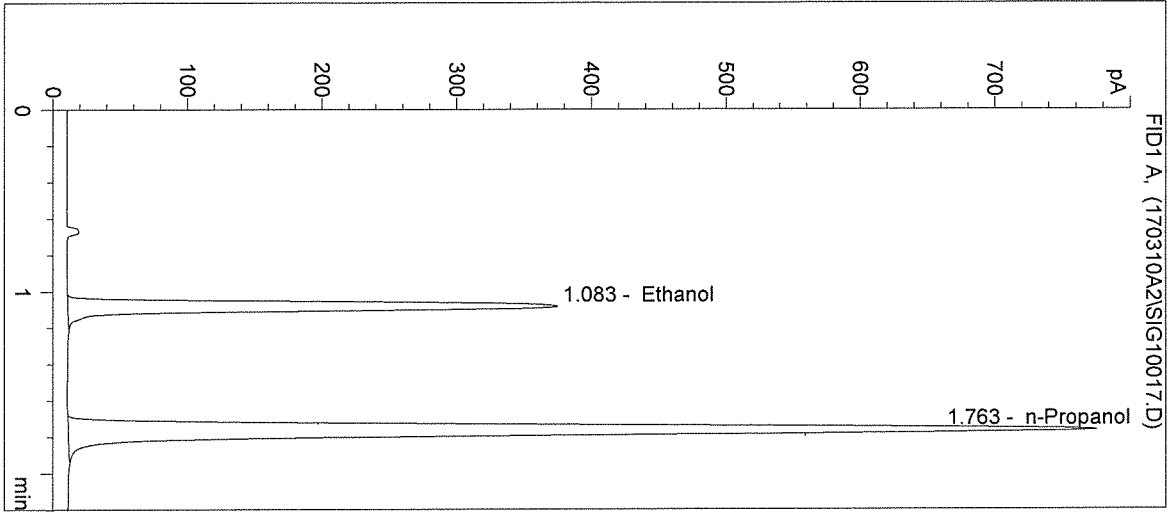


#	Compound	Peak Area	RT (min)
1	Ethanol	1217	1.083
2	n-Propanol	2864	1.763

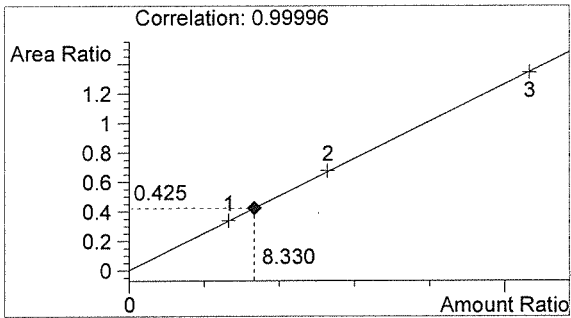

Ethanol 0.100 g/100mL

ALW

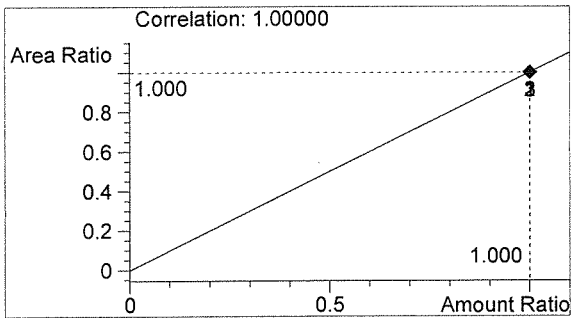

n-Propanol 0.012 g/100mL

AB

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 2:50:52 PM

Sample Name: 17027 #2

Instrument: HSGC#1


Operator: Andrew Gingras

Column: DB-ALC1


Location: Vial 18

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

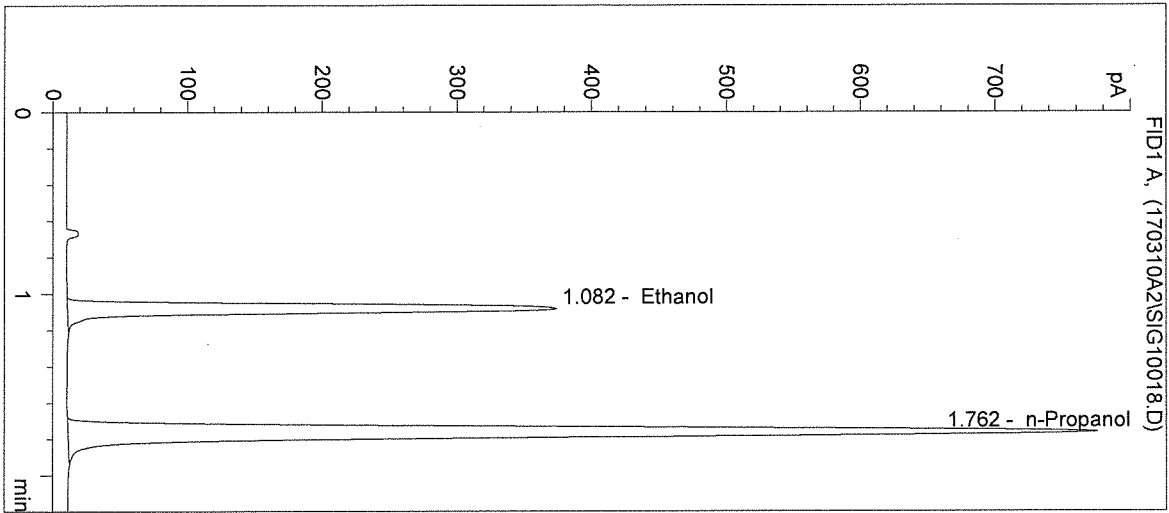


#	Compound	Peak Area	RT (min)
1	Ethanol	1214	1.082
2	n-Propanol	2860	1.762

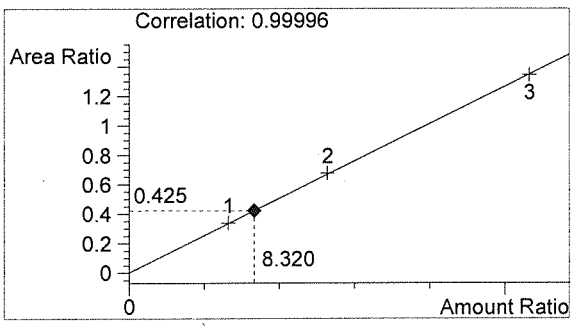

Ethanol 0.100 g/100mL

RAW

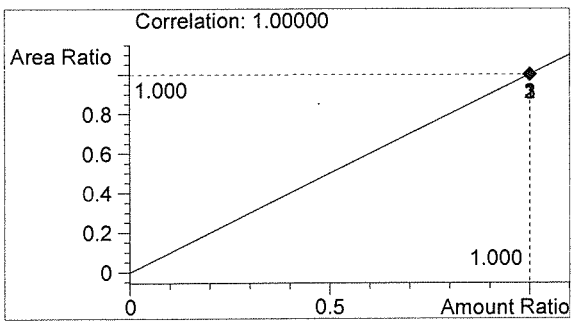


n-Propanol 0.012 g/100mL


AB

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 2:54:06 PM Sample Name: 17027 #3
 Instrument: HSGC#1 Operator: Andrew Gingras
 Column: DB-ALC1 Location: Vial 19
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info:

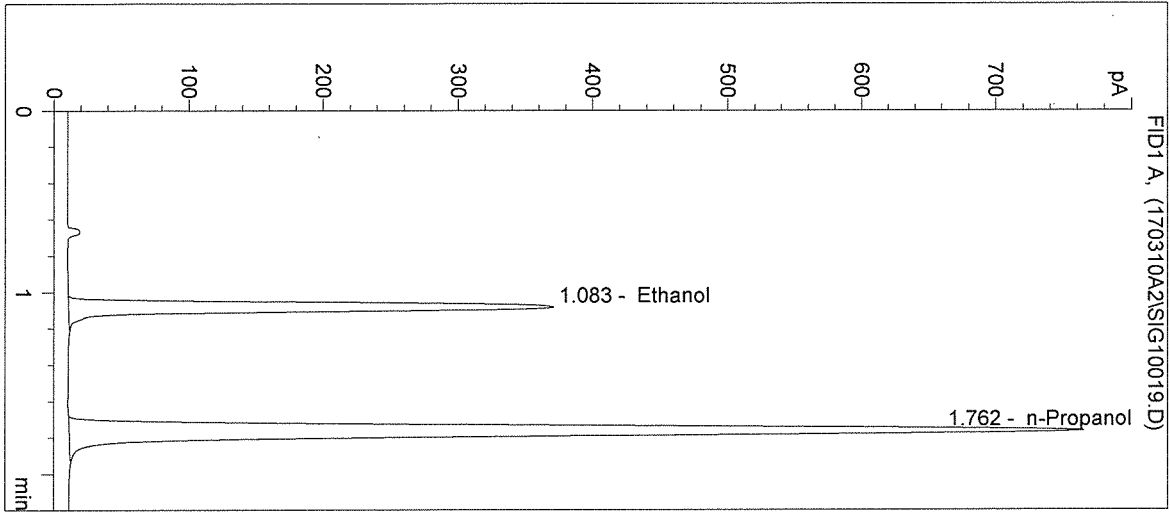


#	Compound	Peak Area	RT (min)
1	Ethanol	1202	1.083
2	n-Propanol	2830	1.762

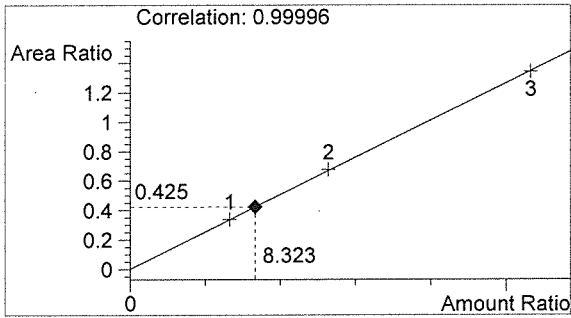

Ethanol 0.100 g/100mL

AW

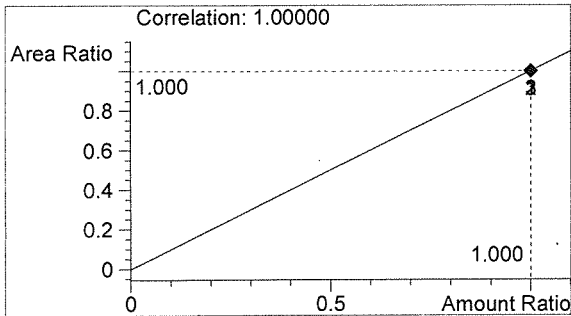


n-Propanol 0.012 g/100mL


JB

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 2:57:19 PM Sample Name: 17027 #4
 Instrument: HSGC#1 Operator: Andrew Gingras
 Column: DB-ALC1 Location: Vial 20
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info:

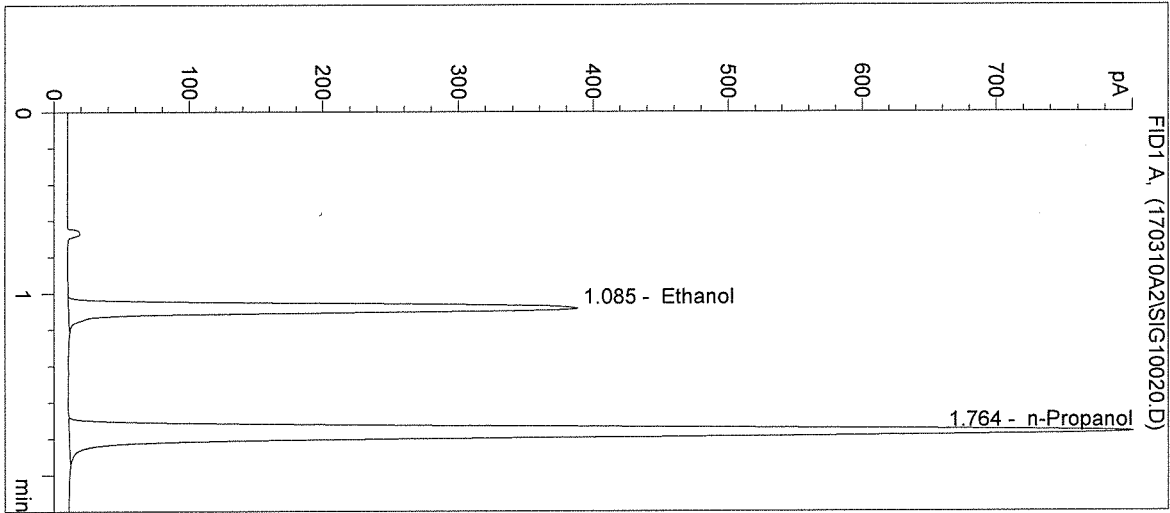


#	Compound	Peak Area	RT (min)
1	Ethanol	1269	1.085
2	n-Propanol	2977	1.764

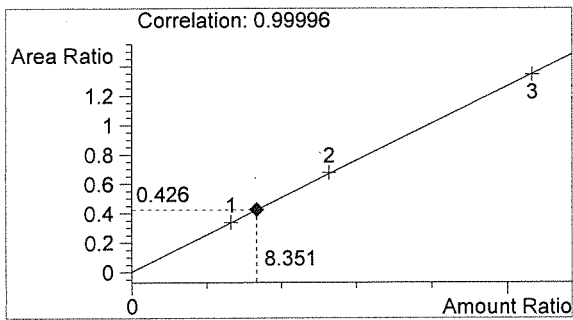

Ethanol 0.100 g/100mL

PHUO

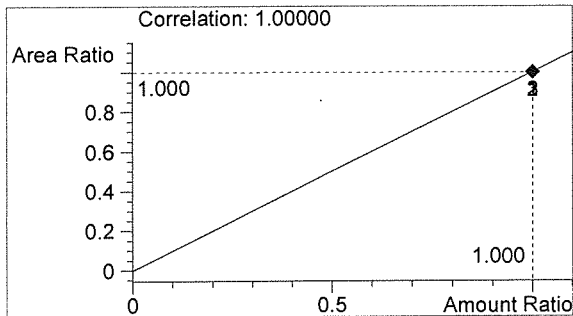

n-Propanol 0.012 g/100mL

AG

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 3:00:32 PM

Sample Name: 17027 #5

Instrument: HSGC#1


Operator: Andrew Gingras

Column: DB-ALC1


Location: Vial 21

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

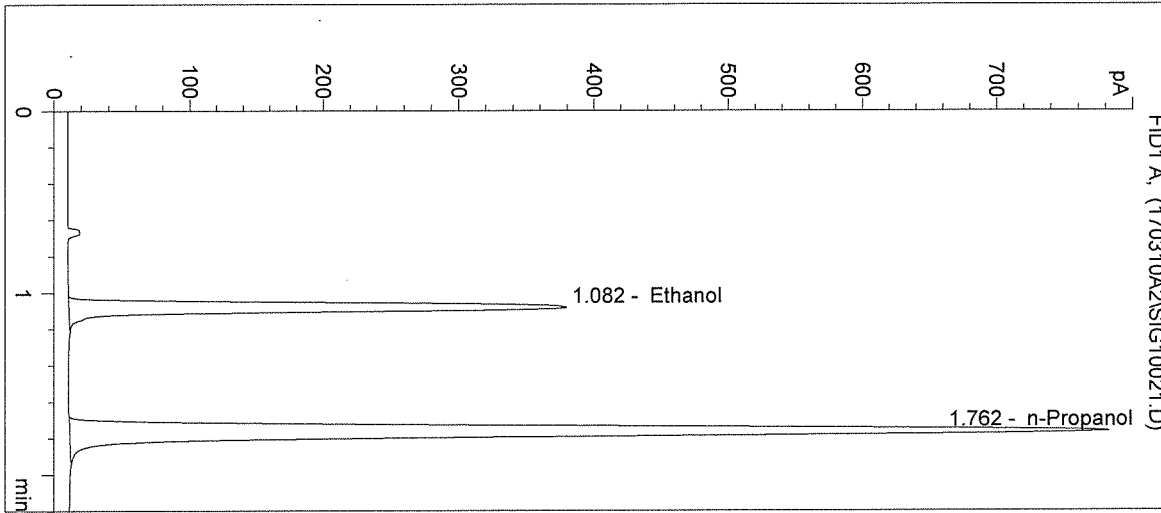


#	Compound	Peak Area	RT (min)
1	Ethanol	1234	1.082
2	n-Propanol	2900	1.762

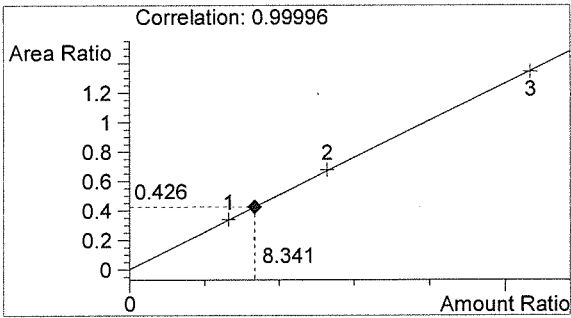

Ethanol 0.100 g/100mL

ALW

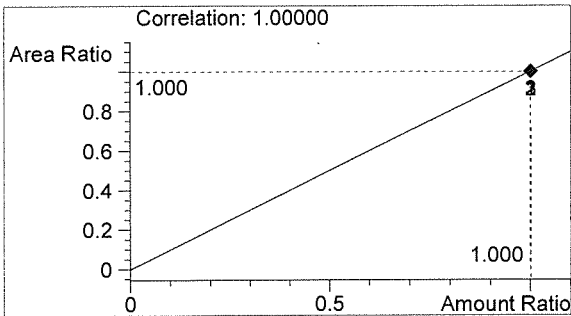


n-Propanol 0.012 g/100mL


AG

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 3:03:45 PM Sample Name: 0.10 CTRL
 Instrument: HSGC#1 Operator: Andrew Gingras
 Column: DB-ALC1 Location: Vial 22
 Method: C:\HPCHEM\1\METHODS\SIMALC1.M
 Sample Info: 17027

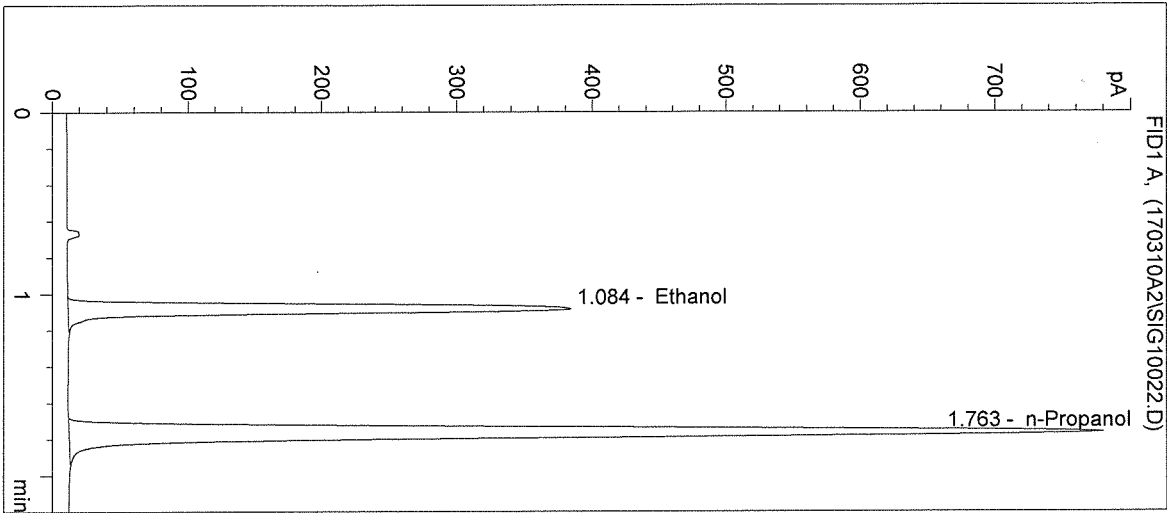


#	Compound	Peak Area	RT (min)
1	Ethanol	1256	1.084
2	n-Propanol	2897	1.763

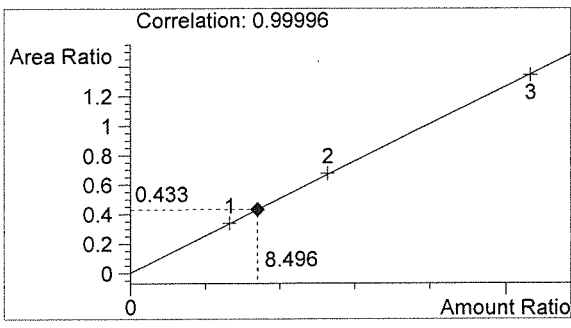

Ethanol 0.102 g/100mL

ALW

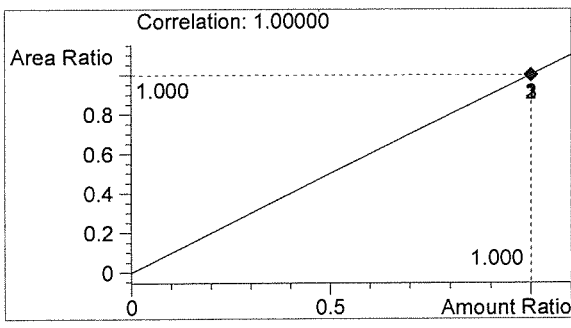

n-Propanol 0.012 g/100mL

AG

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/10/2017 3:06:59 PM

Sample Name: Negative CTRL

Instrument: HSGC#1


Operator: Andrew Gingras

Column: DB-ALC1


Location: Vial 23

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17027

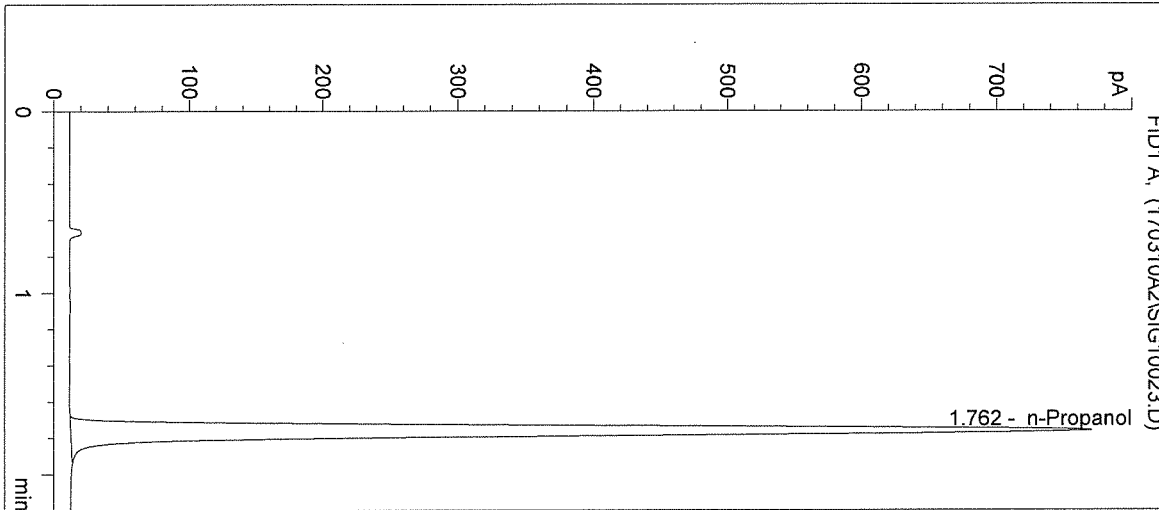


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2847	1.762

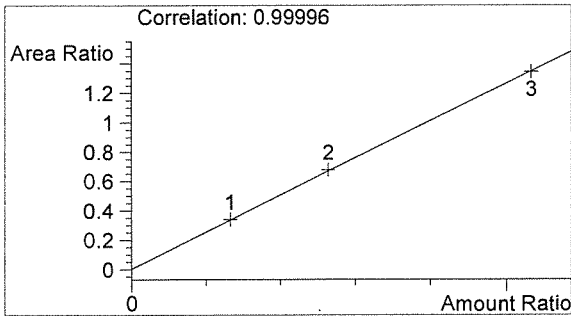

Ethanol 0.000 g/100mL

AW

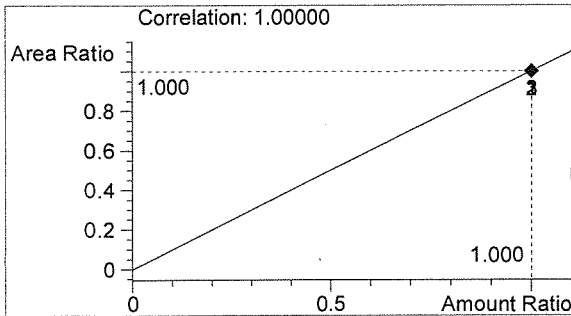

n-Propanol 0.012 g/100mL

JB

Sequence Parameters:

Operator: Christie Mitchell-Mata

Data File Naming: Prefix/Counter

Signal 1 Prefix: SIG1
Counter: 0001

Signal 2 Prefix: SIG2
Counter: 0001

Data Directory: C:\HPCHEM\1\DATA\

Data Subdirectory: 170313CM

Part of Methods to run: According to Runtime Checklist

Barcode Reader: not used

Shutdown Cmd/Macro: none

Sequence Comment:

Ethanol Calibrator 1 0.079 g/100 mL, E0217-01 - Exp. 08/21/17
 Ethanol Calibrator 2 0.158 g/100 mL, E0217-02 - Exp. 08/21/17
 Ethanol Calibrator 3 0.316 g/100 mL, E0217-03 - Exp. 08/21/17

0.04 Control - Lot #FN12181501 - Exp. 12/2020
 0.10 Control - Lot #FN08051301 - Exp. 10/2018
 0.20 Control - Lot #FN08101505 - Exp. 02/2021

ISTD Lot#P0117 - Exp. 04/20/2017

Calibration 1-9 filed with 17026

Sequence Table (Front Injector):

Method and Injection Info Part:

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
1	Vial 1	BLANK	SIMALC1	1	Sample		
2	Vial 2	0.079 CAL 1	SIMALC1	1	Calib		
3	Vial 3	0.158 CAL 2	SIMALC1	1	Calib		
4	Vial 4	0.316 CAL 3	SIMALC1	1	Calib		
5	Vial 5	Negative CTRL	SIMALC1	1	Ctrl Samp		
6	Vial 6	0.04 CTRL	SIMALC1	1	Ctrl Samp		
7	Vial 7	0.10 CTRL	SIMALC1	1	Ctrl Samp		
8	Vial 8	0.20 CTRL	SIMALC1	1	Ctrl Samp		
9	Vial 9	Negative CTRL	SIMALC1	1	Ctrl Samp		
10	Vial 10	17026 #1	SIMALC1	1	Sample		
11	Vial 11	17026 #2	SIMALC1	1	Sample		
12	Vial 12	17026 #3	SIMALC1	1	Sample		
13	Vial 13	17026 #4	SIMALC1	1	Sample		
14	Vial 14	17026 #5	SIMALC1	1	Sample		
15	Vial 15	0.10 CTRL	SIMALC1	1	Ctrl Samp		
16	Vial 16	Negative CTRL	SIMALC1	1	Ctrl Samp		
17	Vial 17	17027 #1	SIMALC1	1	Sample		
18	Vial 18	17027 #2	SIMALC1	1	Sample		
19	Vial 19	17027 #3	SIMALC1	1	Sample		
20	Vial 20	17027 #4	SIMALC1	1	Sample		
21	Vial 21	17027 #5	SIMALC1	1	Sample		
22	Vial 22	0.10 CTRL	SIMALC1	1	Ctrl Samp		
23	Vial 23	Negative CTRL	SIMALC1	1	Ctrl Samp		
24	Vial 24	17028 #1	SIMALC1	1	Sample		

17027
P0103.14.17

CM

Line	Location	SampleName	Method	Inj	SampleType	InjVolume	DataFile
25	Vial 25	17028 #2	SIMALC1	1	Sample		
26	Vial 26	17028 #3	SIMALC1	1	Sample		
27	Vial 27	17028 #4	SIMALC1	1	Sample		
28	Vial 28	17028 #5	SIMALC1	1	Sample		
29	Vial 29	0.10 CTRL	SIMALC1	1	Ctrl Samp		
30	Vial 30	Negative CTRL	SIMALC1	1	Ctrl Samp		
31	Vial 31	17029 #1	SIMALC1	1	Sample		
32	Vial 32	17029 #2	SIMALC1	1	Sample		
33	Vial 33	17029 #3	SIMALC1	1	Sample		
34	Vial 34	17029 #4	SIMALC1	1	Sample		
35	Vial 35	17029 #5	SIMALC1	1	Sample		
36	Vial 36	0.10 CTRL	SIMALC1	1	Ctrl Samp		
37	Vial 37	Negative CTRL	SIMALC1	1	Ctrl Samp		

Calibration Part:

Line	Location	SampleName	Method	CalLev	Update	RF	Update	RT	Interval
2	Vial 2	0.079 CAL 1	SIMALC1	1	Replace		Replace		
3	Vial 3	0.158 CAL 2	SIMALC1	2	Replace		Replace		
4	Vial 4	0.316 CAL 3	SIMALC1	3	Replace		Replace		

Sequence Table (Back Injector):

No entries - empty table!

17027
Paw 3.14.17

Paw 3.14.17
~~17031304~~

M

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:14:31 PM

Sample Name: 17027 #1

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 17

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

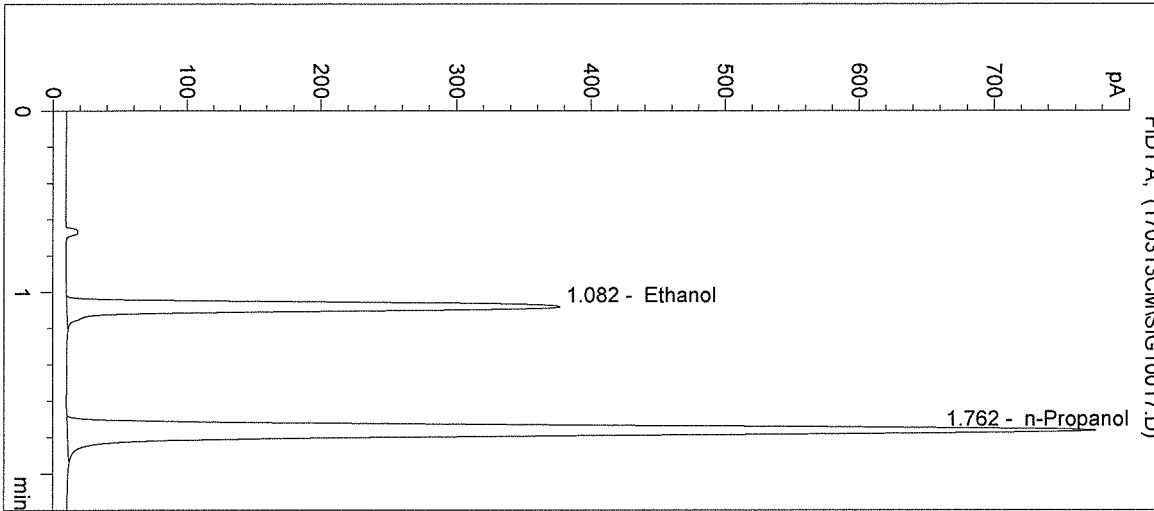


#	Compound	Peak Area	RT (min)
1	Ethanol	1221	1.082
2	n-Propanol	2863	1.762

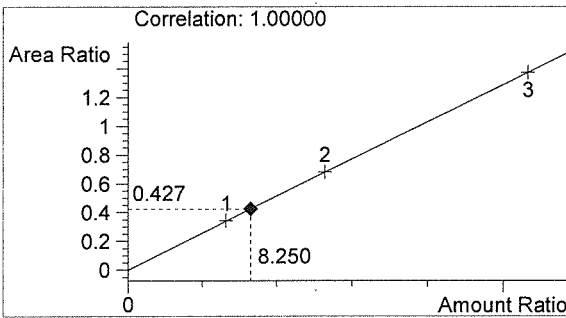

Ethanol 0.099 g/100mL

Also

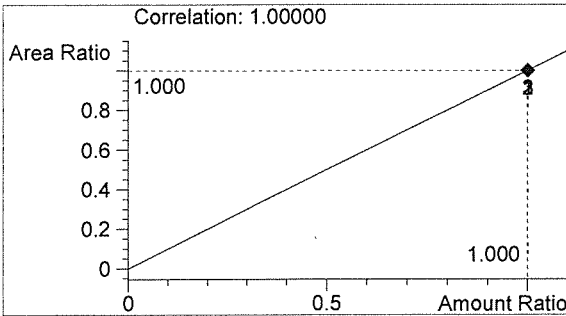

n-Propanol 0.012 g/100mL

M

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:17:44 PM

Sample Name: 17027 #2

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 18

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

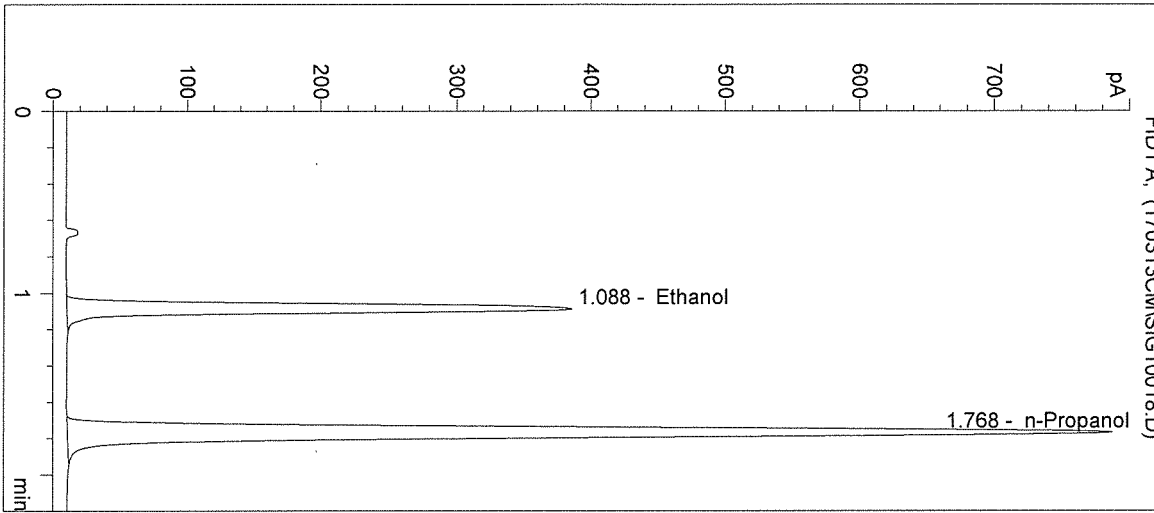


#	Compound	Peak Area	RT (min)
1	Ethanol	1275	1.088
2	n-Propanol	2956	1.768

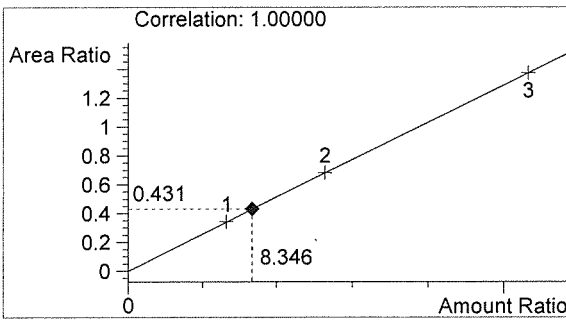

Ethanol 0.100 g/100mL

AW

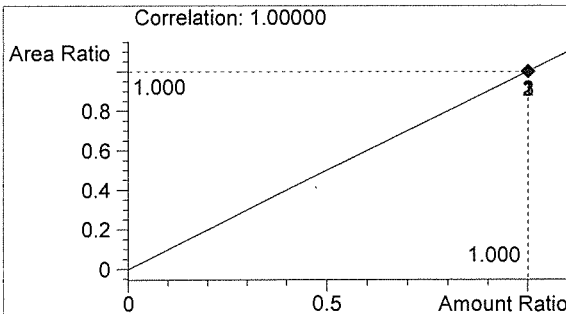

n-Propanol 0.012 g/100mL

AW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:20:57 PM

Sample Name: 17027 #3

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 19

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

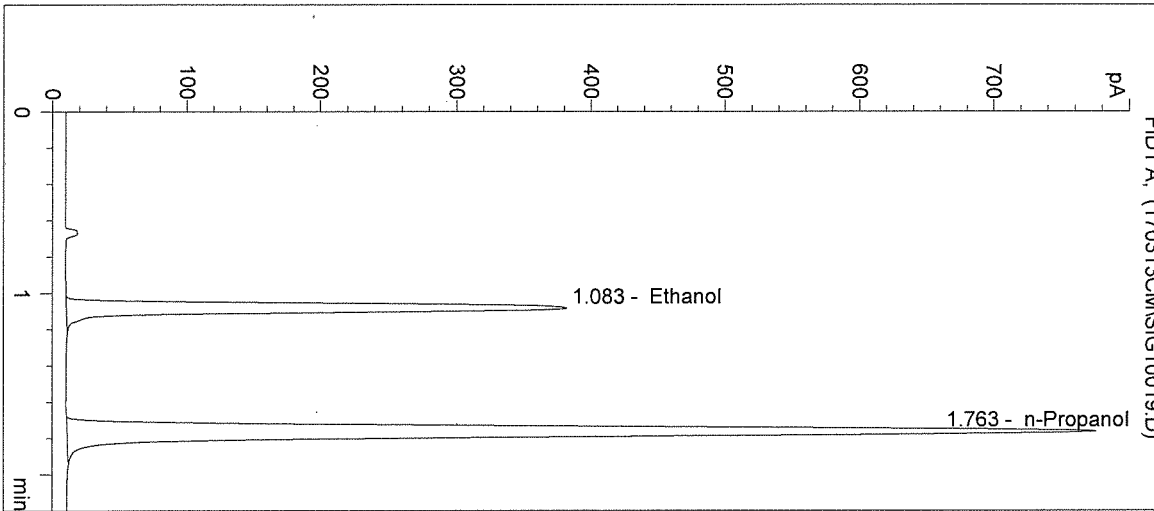


#	Compound	Peak Area	RT (min)
1	Ethanol	1243	1.083
2	n-Propanol	2864	1.763

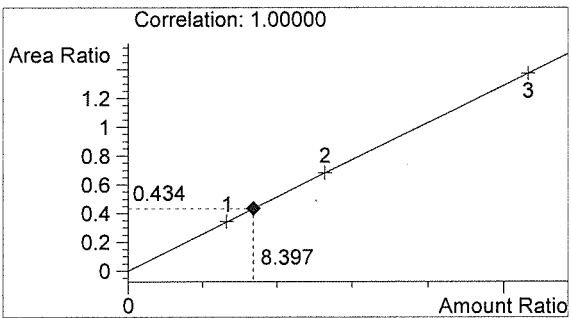

Ethanol 0.101 g/100mL

AWD

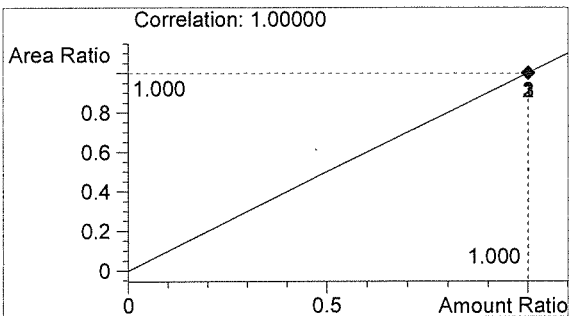

n-Propanol 0.012 g/100mL

AW

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:24:10 PM

Sample Name: 17027 #4

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 20

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

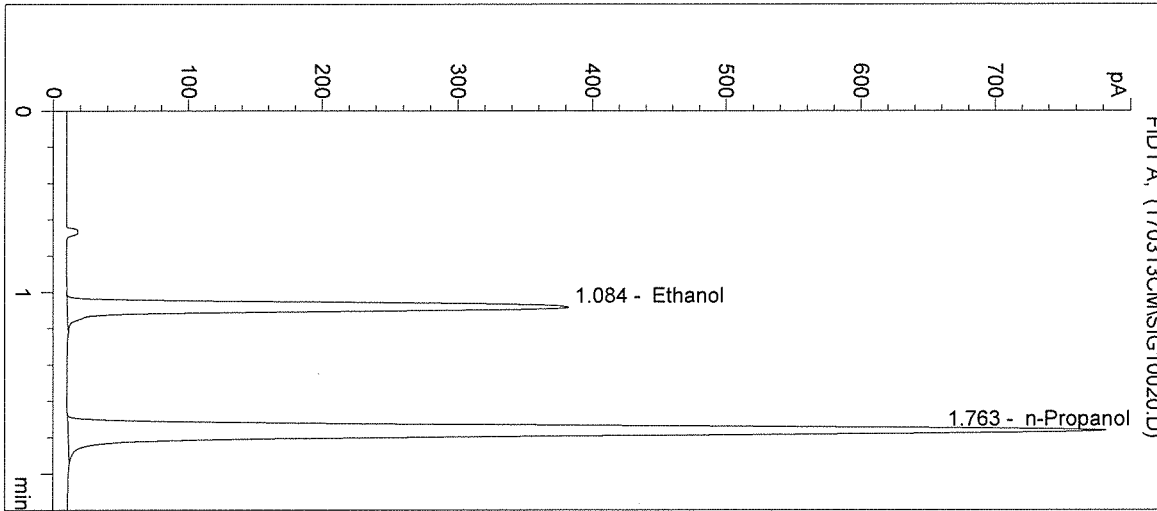


#	Compound	Peak Area	RT (min)
1	Ethanol	1246	1.084
2	n-Propanol	2892	1.763

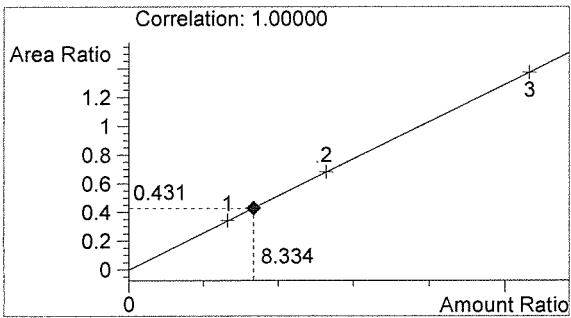

Ethanol 0.100 g/100mL

PLW

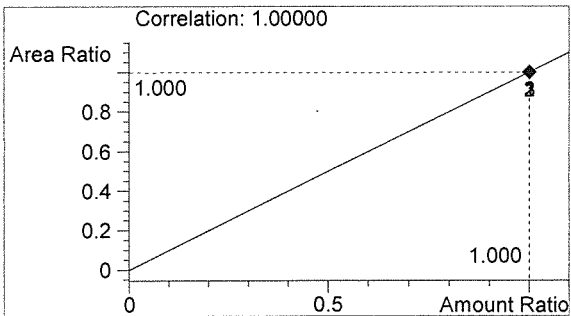

n-Propanol 0.012 g/100mL

CM

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:27:24 PM

Sample Name: 17027 #5

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 21

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info:

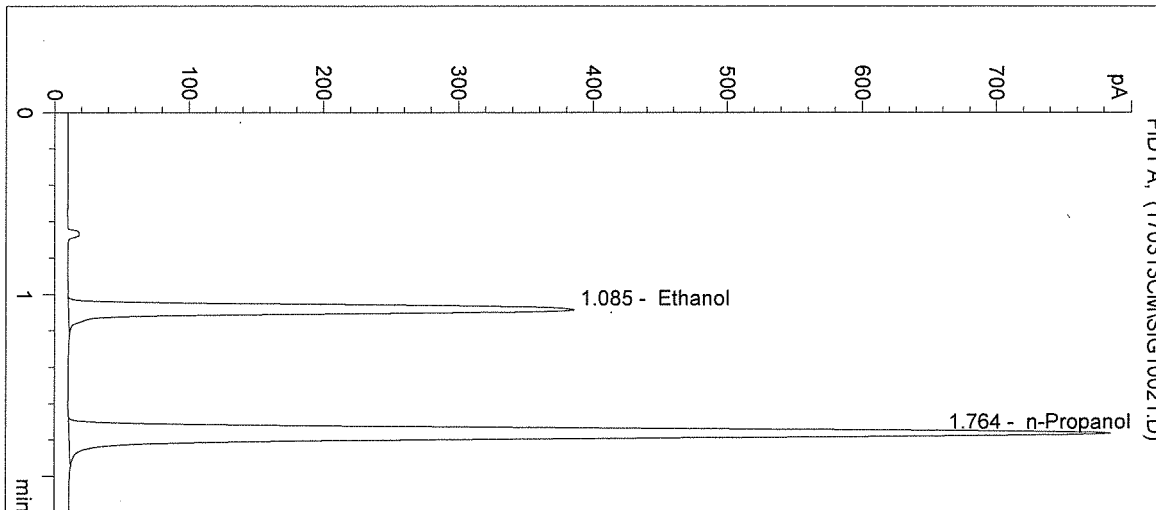


#	Compound	Peak Area	RT (min)
1	Ethanol	1260	1.085
2	n-Propanol	2915	1.764

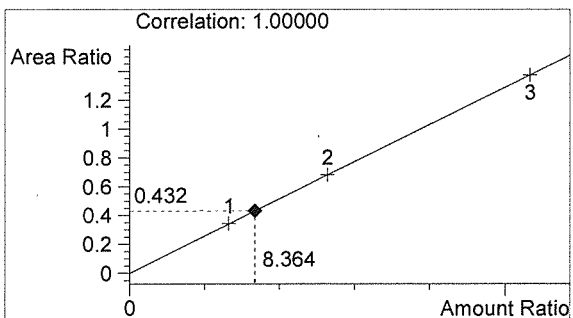

Ethanol 0.100 g/100mL

Handwritten: Buo

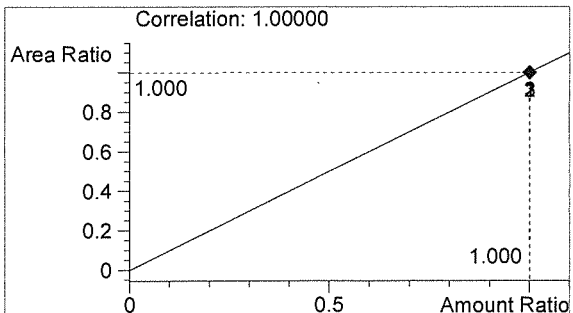

n-Propanol 0.012 g/100mL

Handwritten: 04

Washington State Patrol Toxicology Laboratory
 2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:30:37 PM

Sample Name: 0.10 CTRL

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 22

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17027

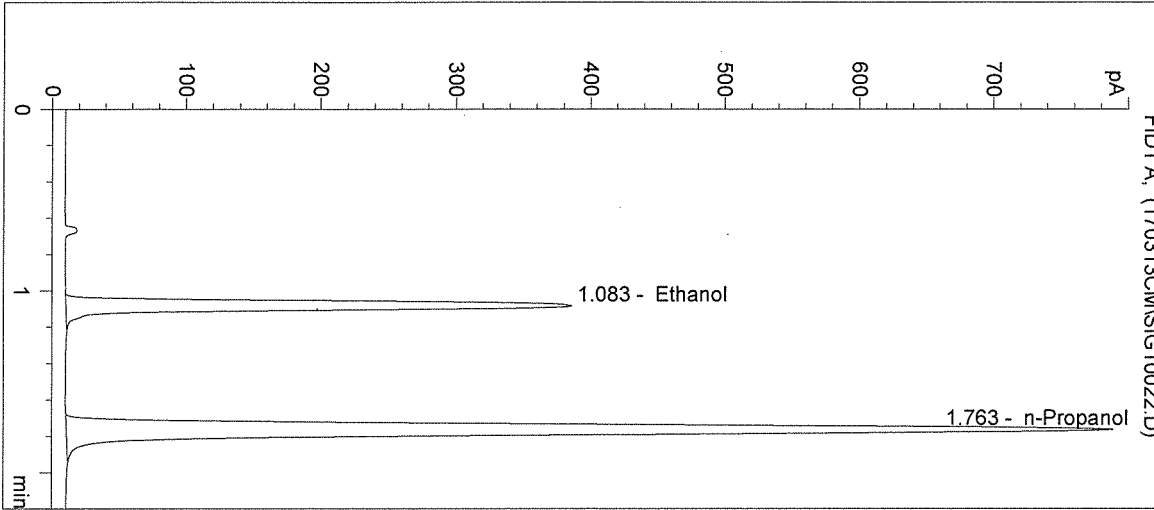


#	Compound	Peak Area	RT (min)
1	Ethanol	1259	1.083
2	n-Propanol	2921	1.763

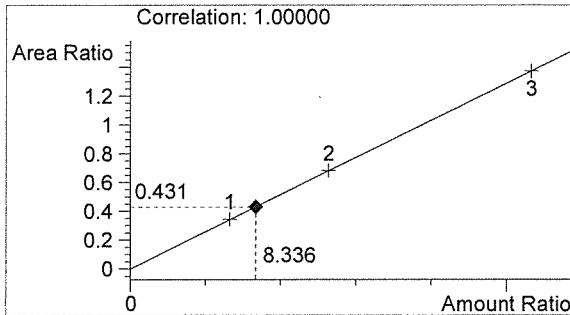

Ethanol 0.100 g/100mL

AW

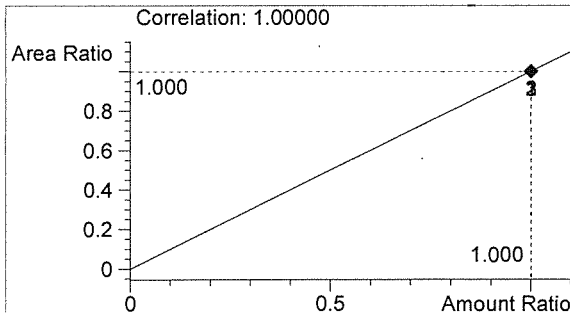

n-Propanol 0.012 g/100mL

AW

Washington State Patrol Toxicology Laboratory
2203 Airport Way S Seattle, WA 98134

Inj. Date: 3/13/2017 12:33:50 PM

Sample Name: Negative CTRL

Instrument: HSGC#1


Operator: Christie Mitchell-Mata

Column: DB-ALC1


Location: Vial 23

Method: C:\HPCHEM\1\METHODS\SIMALC1.M

Sample Info: 17027

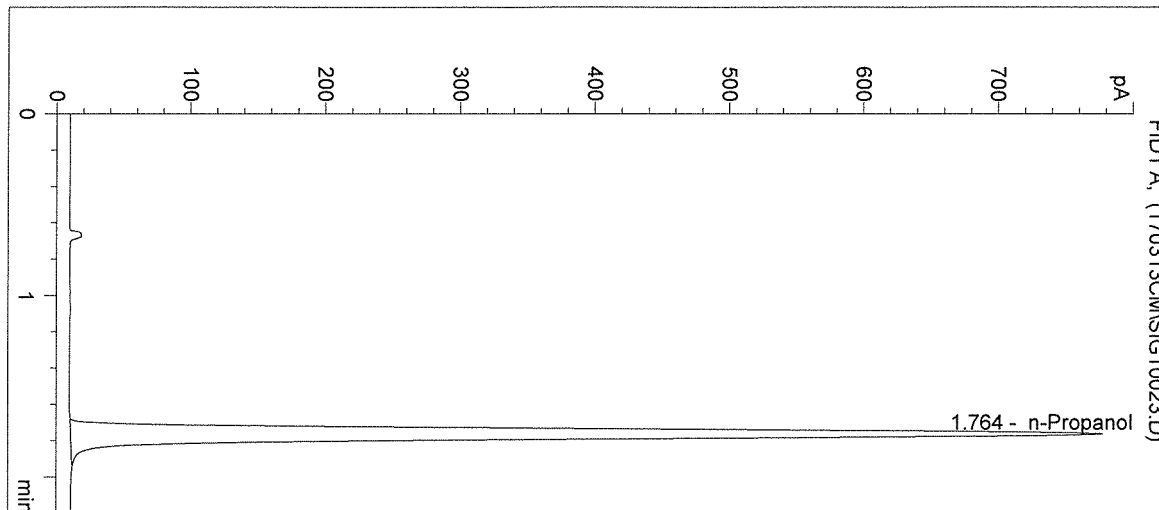


#	Compound	Peak Area	RT (min)
1	Ethanol	0	0.000
2	n-Propanol	2884	1.764

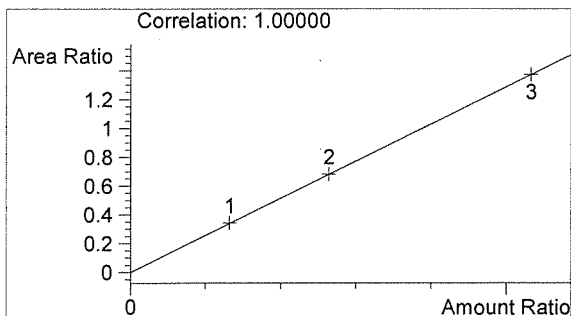

Ethanol 0.000 g/100mL

AW

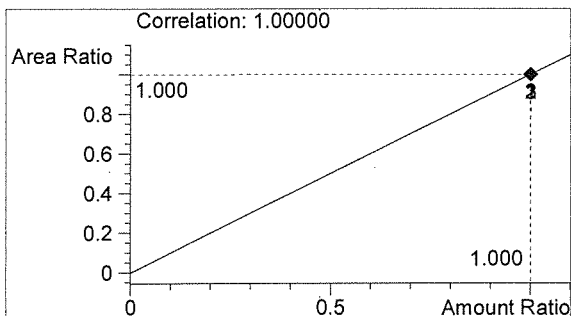

n-Propanol 0.012 g/100mL

AW